

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091127.D
 Acq On : 12 Nov 2015 00:33
 Operator : UM/NP
 Sample : G4322-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A4HR6

Quant Time: Nov 13 16:06:21 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/16/2015 12:42:11 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	3100	0.40	ng/ul	0.00
4) Naphthalene-d8	9.57	136	17326	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.40	164	10019	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.12	188	25866m	0.40	ng/ul	-0.01
18) Chrysene-d12	20.28	240	31770	0.40	ng/ul	0.00
22) Perylene-d12	22.19	264	28209m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.92	96	17258	7.74	ng/uL	-0.03
6) 2-Methylnaphthalene-d10	11.07	152	5349	0.23	ng/ul	0.00
16) Fluoranthene-d10	18.12	212	15284	0.21	ng/ul	0.00
Target Compounds						
5) Naphthalene	9.61	128	1303	0.03	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U.M
 11/24/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091127.D
 Acq On : 12 Nov 2015 00:33
 Operator : UM/NP
 Sample : G4322-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A4HR6

Quant Time: Nov 13 16:05:34 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/16/2015 12:42:11 PM

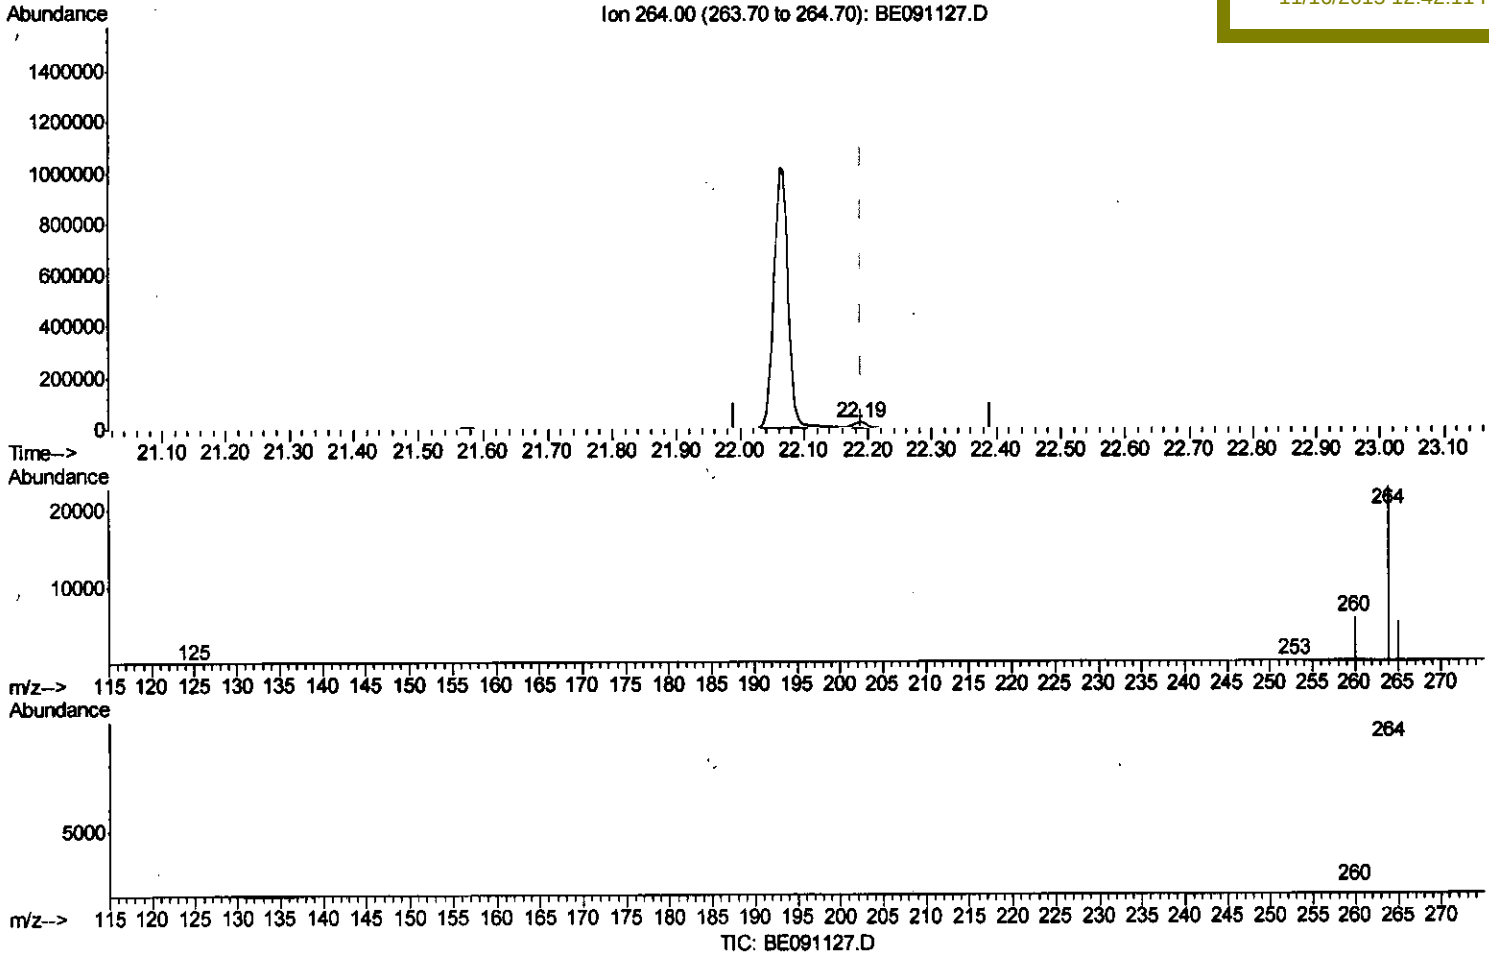

(22) Perylene-d12 (I)

22.186min (-0.004) 0.40ng/ul m

response 28209

Ion	Exp%	Act%
264.00	100	100
260.00	28.90	25.62
265.00	34.70	22.61#
0.00	0.00	0.00

U.M
 11/24/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091127.D
 Acq On : 12 Nov 2015 00:33
 Operator : UM/NP
 Sample : G4322-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 Client Sampled :
 A4HR6

Quant Time: Nov 13 16:05:34 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/16/2015 12:42:11 PM

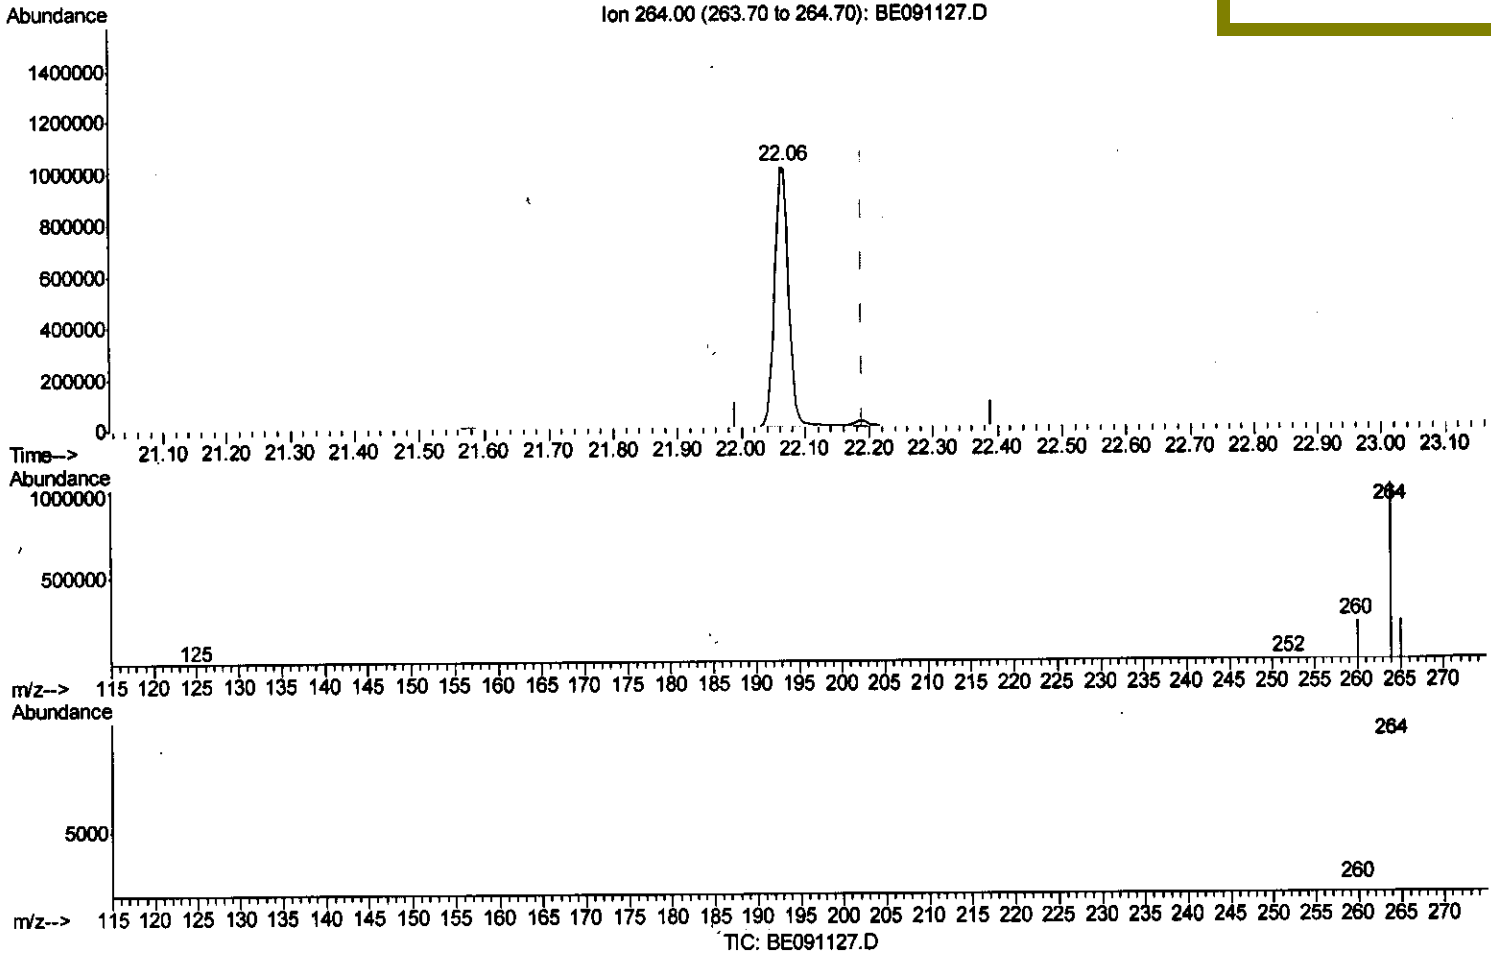

(22) Perylene-d12 (I)

22.063min (-0.127) 0.40ng/ul

response 1587279

Ion	Exp%	Act%
264.00	100	100
260.00	28.90	21.60#
265.00	34.70	21.98#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
 Data File : BE091127.D
 Acq On : 12 Nov 2015 00:33
 Operator : UM/NP
 Sample : G4322-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
ClientSampled :
 A4HR6

Quant Time: Nov 13 15:21:08 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
 11/16/2015 12:42:11 PM

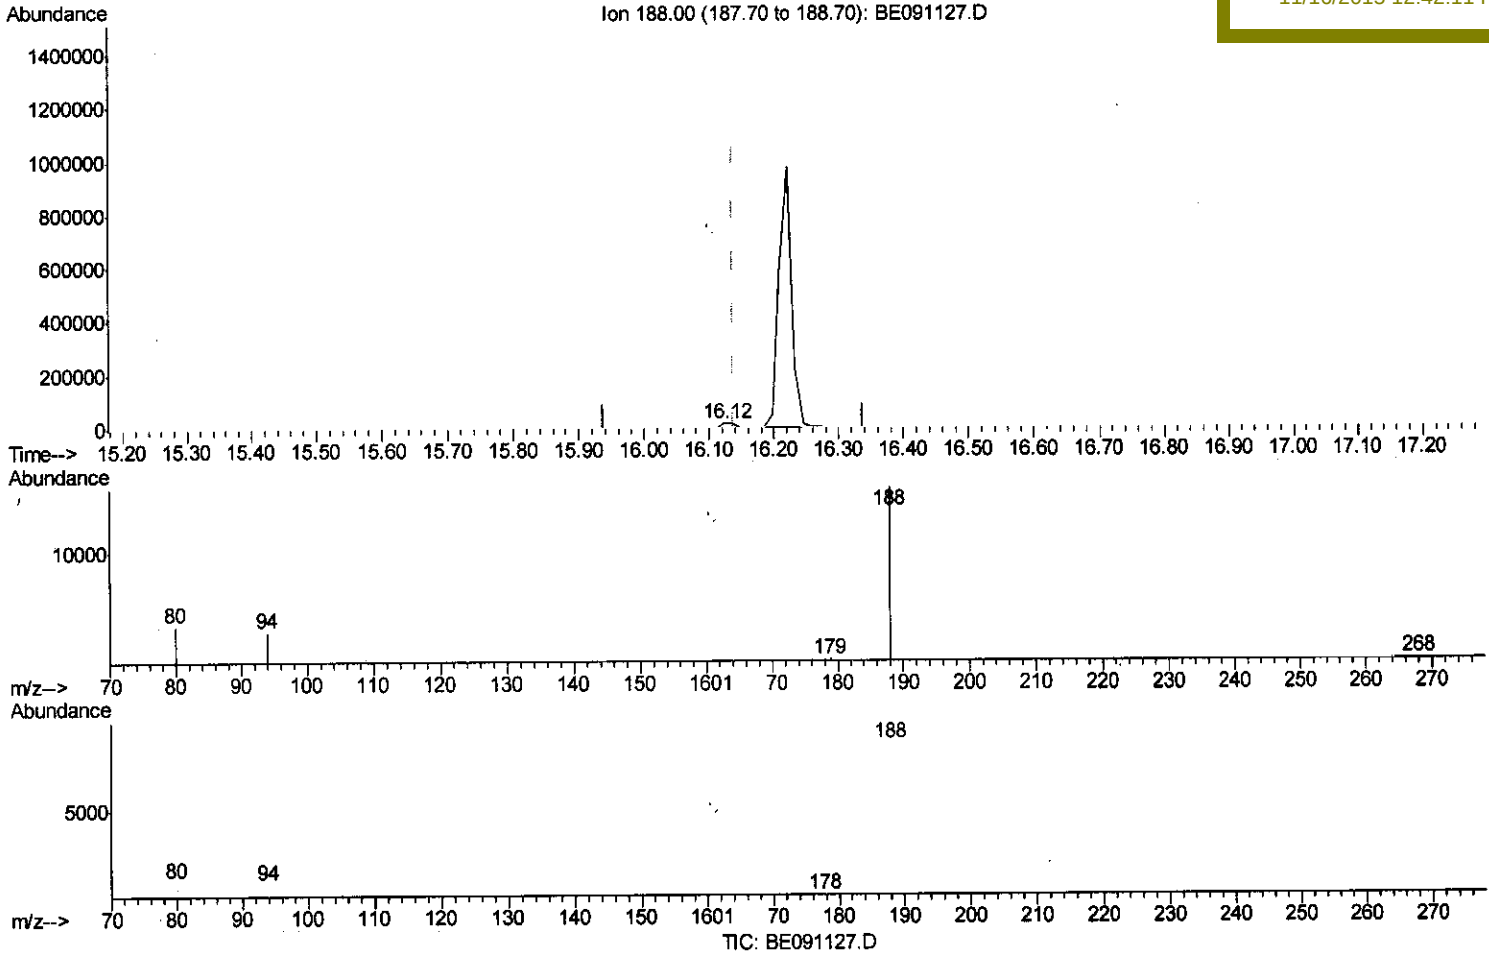

(12) Phenanthrene-d10 (I)

16.124min (-0.013) 0.40ng/ul m

response 25866

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	17.60#
80.00	8.90	21.04#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
Data File : BE091127.D
Acq On : 12 Nov 2015 00:33
Operator : UM/NP
Sample : G4322-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A4HR6

Quant Time: Nov 13 15:21:08 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/16/2015 12:42:11 PM

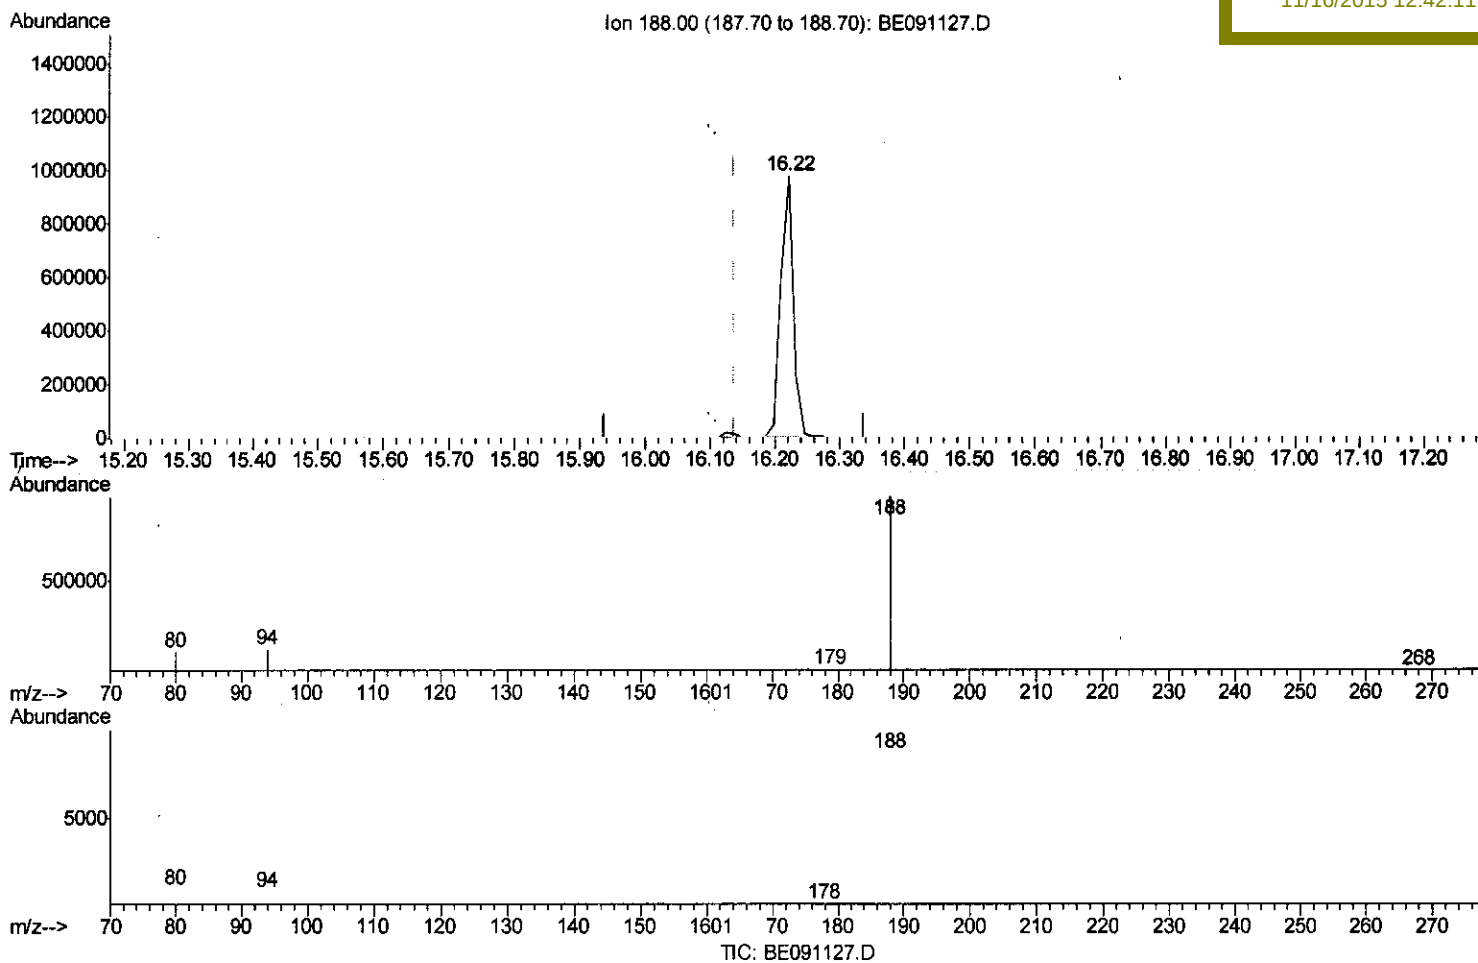

(12) Phenanthrene-d10 (I)

16.221min (+0.084) 0.40ng/ul

response 1351673

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	11.96#
80.00	8.90	10.78#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111115\
Data File : BE091127.D
Acq On : 12 Nov 2015 00:33
Operator : UM/NP
Sample : G4322-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A4HR6

Quant Time: Nov 13 16:06:21 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/16/2015 12:42:11 PM

