

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111115\
 Data File : BE091118.D
 Acq On : 11 Nov 2015 19:05
 Operator : UM/NP
 Sample : G4308-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 D9KS1

Manual Integrations
 APPROVED

Mmdadoda
 11/16/2015 12:42:01 PM

Quant Time: Nov 13 18:00:22 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 13 13:56:00 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	3026	0.40	ng/ul	0.00
4) Naphthalene-d8	9.57	136	17336	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.40	164	9782	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.12	188	25223m	0.40	ng/ul	-0.01
18) Chrysene-d12	20.29	240	30913	0.40	ng/ul	0.00
22) Perylene-d12	22.18	264	27328m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.95	96	4267	1.96	ng/uL	0.00
6) 2-Methylnaphthalene-d10	11.08	152	4950	0.21	ng/ul	0.00
16) Fluoranthene-d10	18.12	212	14426	0.20	ng/ul	0.00
Target Compounds						
5) Naphthalene	9.61	128	1626	0.04	ng/ul#	Ovalue 84
7) 2-Methylnaphthalene	11.15	142	1186	0.04	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE111115\
Data File : BE091118.D
Acq On : 11 Nov 2015 19:05
Operator : UM/NP
Sample : G4308-19
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
D9KS1

Manual Integrations
APPROVED

Mmdadoda
11/16/2015 12:42:01 PM

Quant Time: Nov 13 18:00:22 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 13 13:56:00 2015
Response via : Initial Calibration

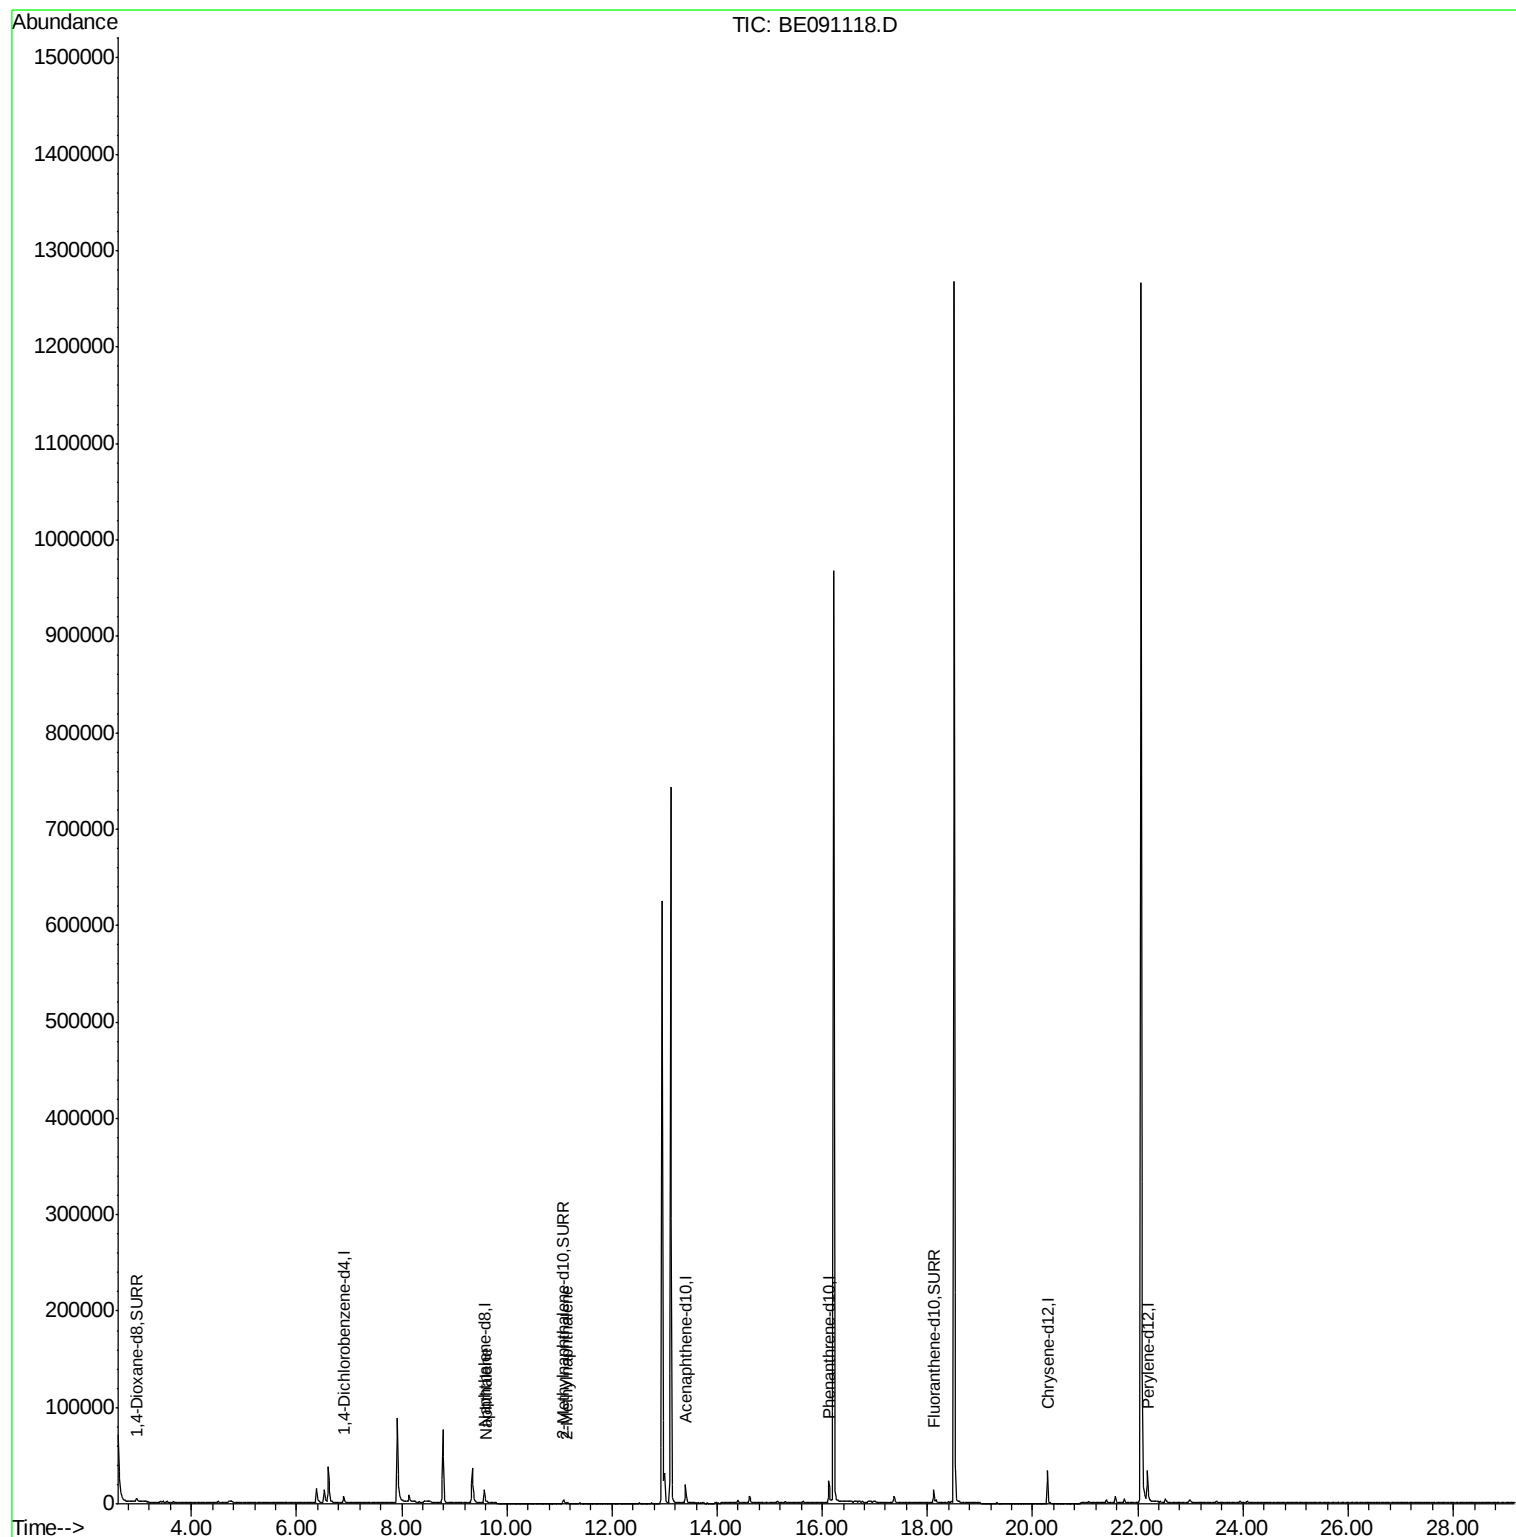

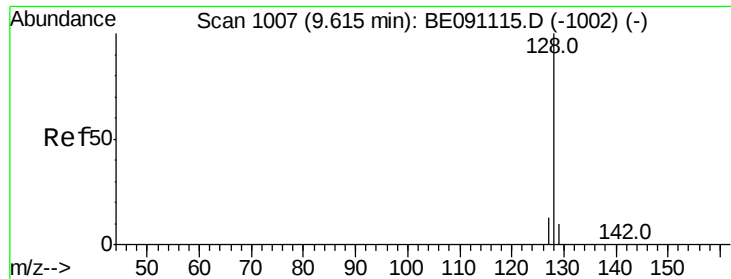

#5

Naphthalene

Concen: 0.04 ng/ul

RT: 9.61 min Scan# 1007

Delta R.T. -0.00 min

Lab File: BE091118.D

Acq: 11 Nov 2015 19:05

Instrument :

BNA_E


ClientSampleId :

D9KS1

Tot Ion	Ratio	Lower	Upper
128	100		
129	19.5	9.8	14.8#
127	18.8	10.7	16.1#

Manual Integrations
APPROVED




Mmdadoda
11/16/2015 12:42:01 PM

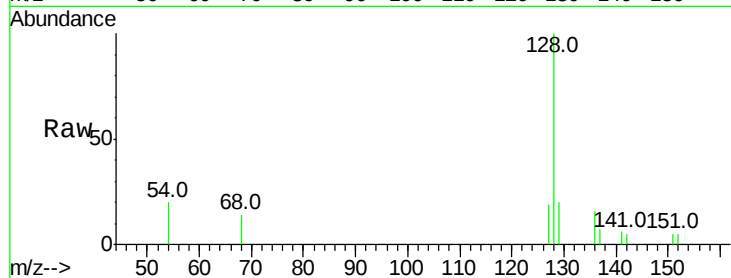

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

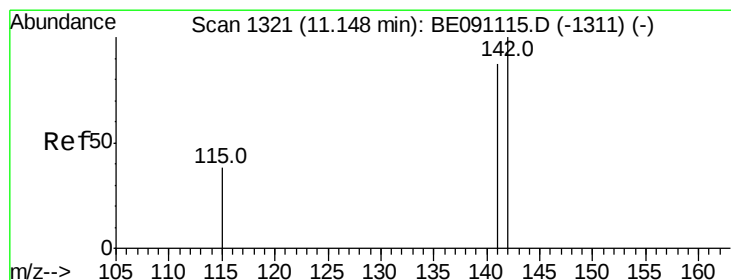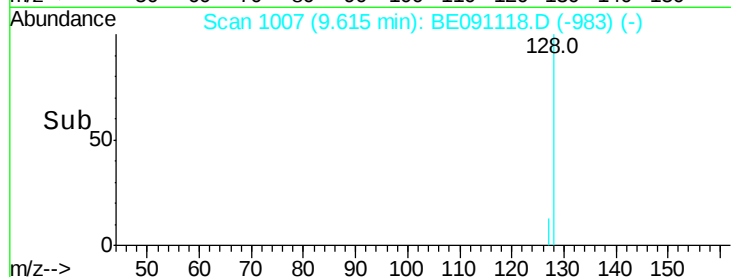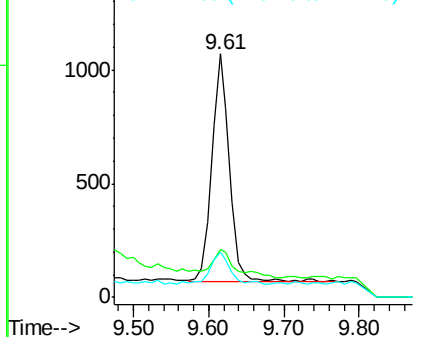

#7

2-Methylnaphthalene

Concen: 0.04 ng/ul


RT: 11.15 min Scan# 1321

Delta R.T. -0.00 min

Lab File: BE091118.D

Acq: 11 Nov 2015 19:05

Tgt Ion	Ratio	Lower	Upper
142	100		
141	88.4	70.3	105.5

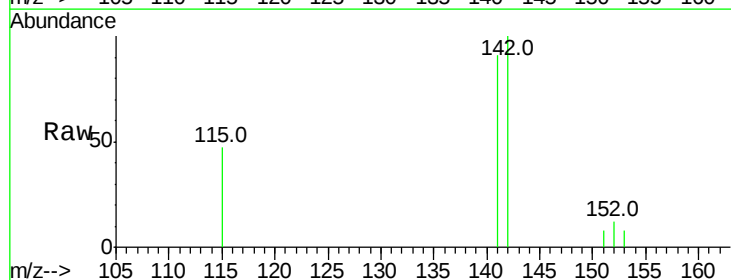

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

