

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111124\
 Data File : BE101571.D
 Acq On : 11 Nov 2024 14:33
 Operator : RC/JU
 Sample : P4795-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 LAW-23-00189

Quant Time: Nov 11 18:15:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.553	152	39706	20.000	ng	0.00
21) Naphthalene-d8	10.320	136	167207	20.000	ng	-0.01
39) Acenaphthene-d10	14.169	164	112501	20.000	ng	0.00
64) Phenanthrene-d10	16.901	188	270240	20.000	ng	-0.01
76) Chrysene-d12	21.067	240	338714	20.000	ng	-0.01
86) Perylene-d12	23.346	264	425347	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.309	112	368633	164.159	ng	0.00
7) Phenol-d6	6.936	99	423859	137.667	ng	-0.01
23) Nitrobenzene-d5	8.763	82	297927	112.546	ng	-0.01
42) 2,4,6-Tribromophenol	15.673	330	360088	170.099	ng	-0.01
45) 2-Fluorobiphenyl	12.788	172	720361	104.551	ng	-0.01
79) Terphenyl-d14	19.498	244	1819130	118.884	ng	0.00
Target Compounds						
32) Benzoic acid	9.962	122	85	6.880	ng	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111124\
Data File : BE101571.D
Acq On : 11 Nov 2024 14:33
Operator : RC/JU
Sample : P4795-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
LAW-23-00189


Quant Time: Nov 11 18:15:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

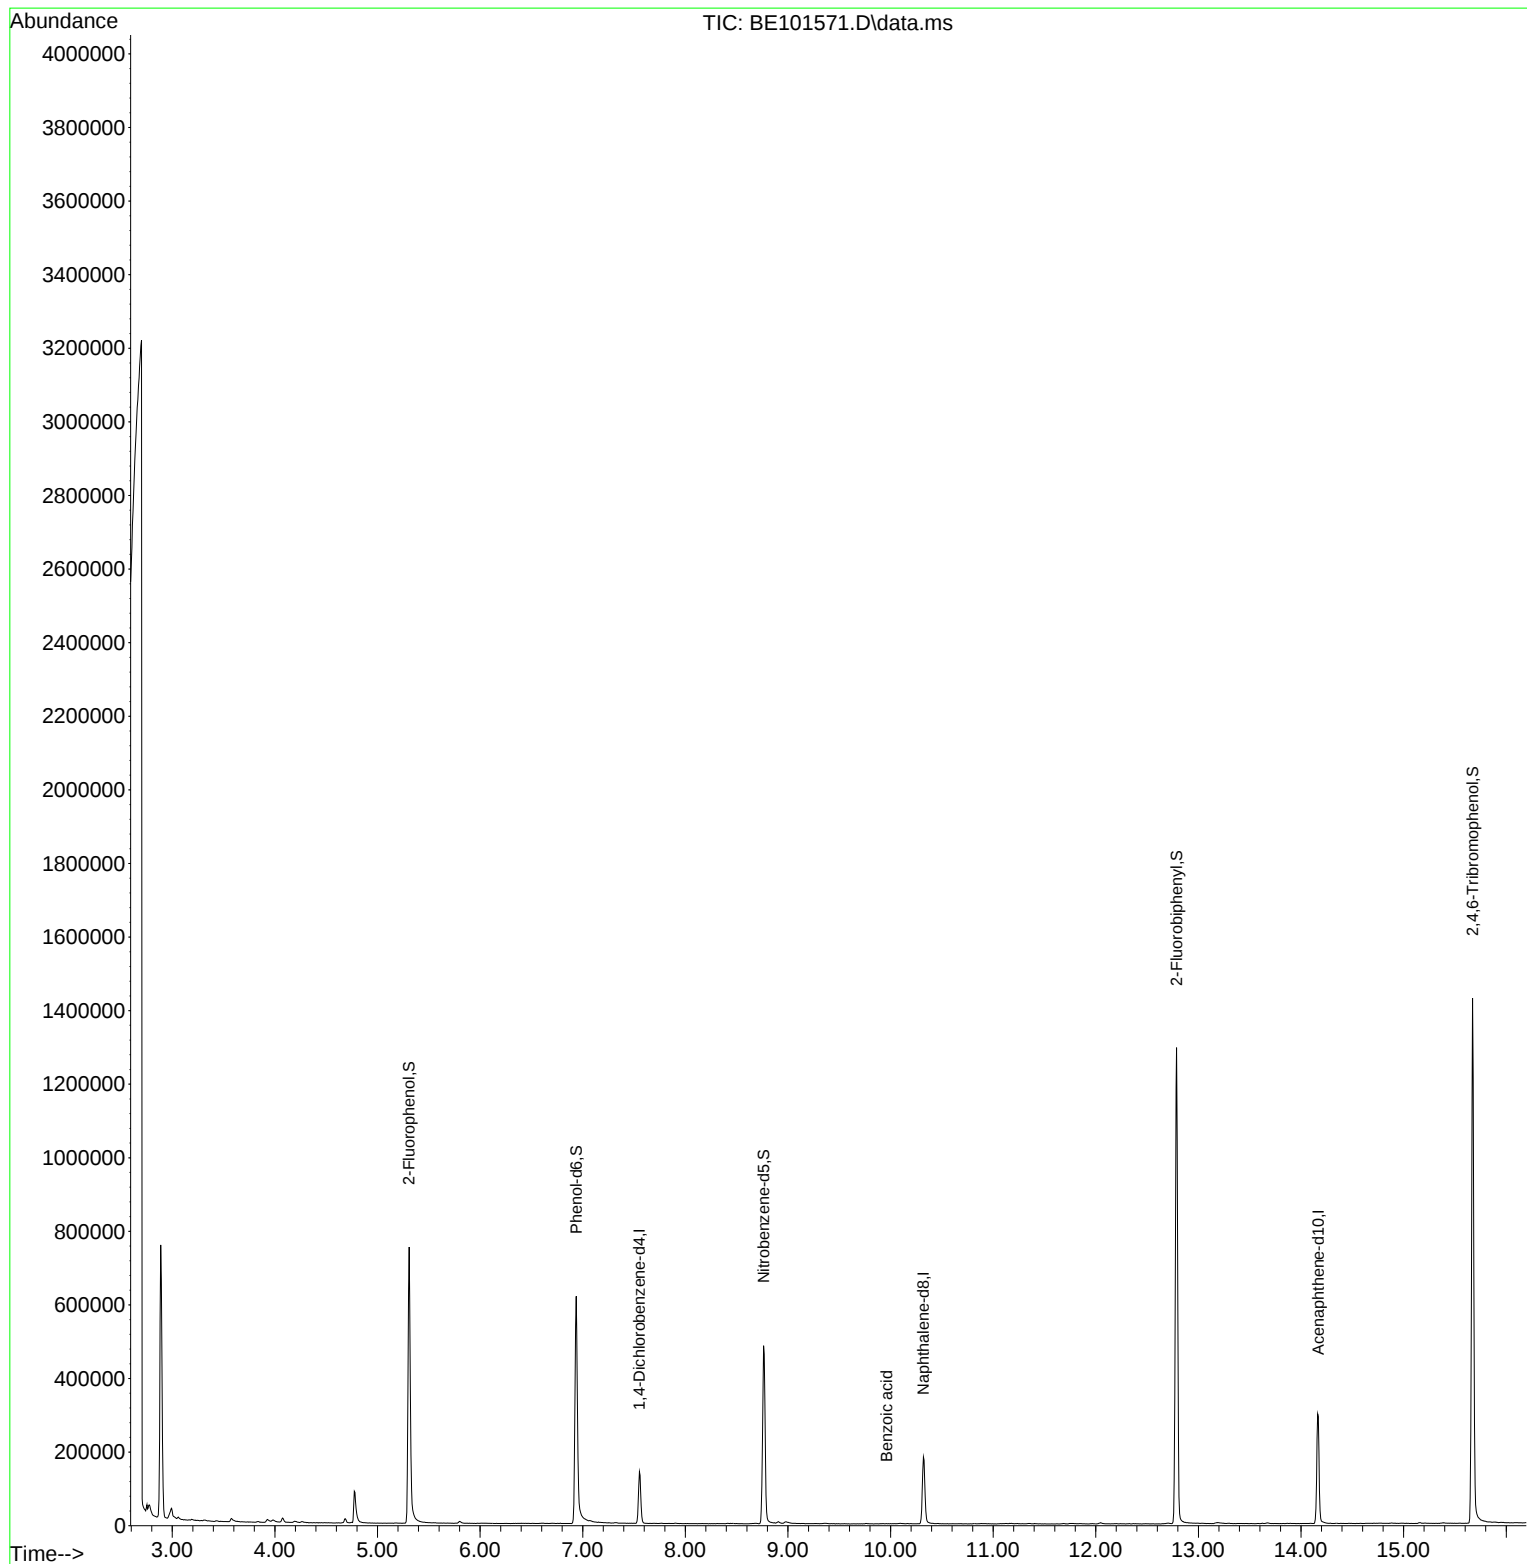


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111124\
Data File : BE101571.D
Acq On : 11 Nov 2024 14:33
Operator : RC/JU
Sample : P4795-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
LAW-23-00189

Quant Time: Nov 11 18:15:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration




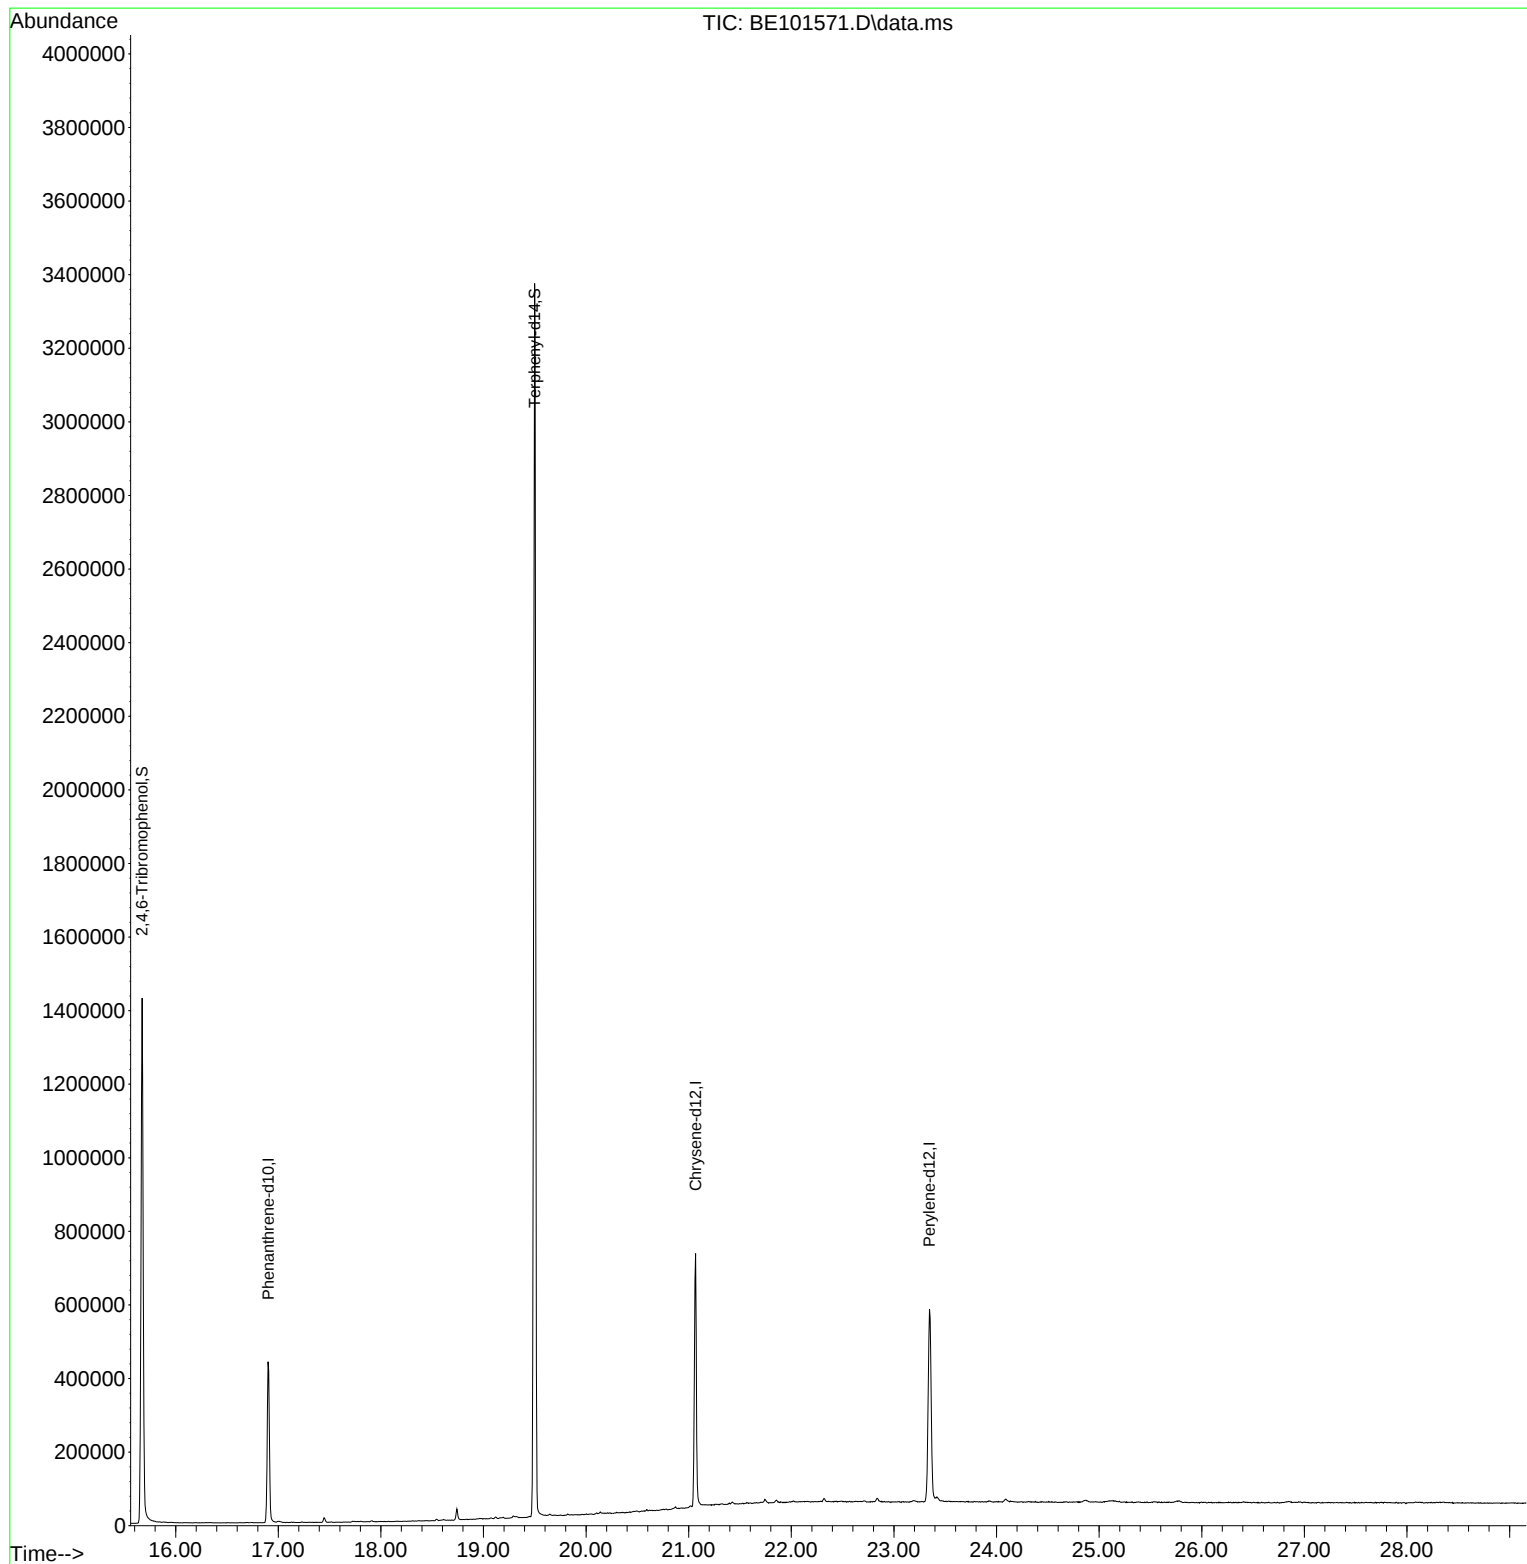


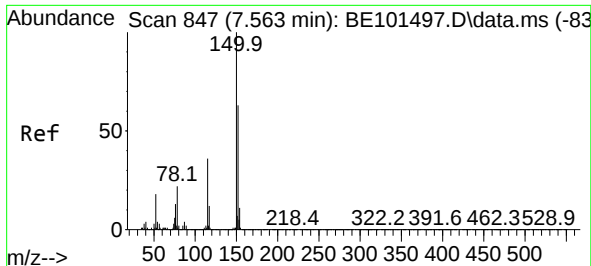

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.553 min Scan# 84
 Delta R.T. -0.010 min
 Lab File: BE101571.D
 Acq: 11 Nov 2024 14:33




Instrument :
 BNA_E
 ClientSampleId :
 LAW-23-00189


Tgt Ion:152 Resp: 39706
 Ion Ratio Lower Upper
 152 100
 150 153.9 126.3 189.5
 115 57.0 45.0 67.4

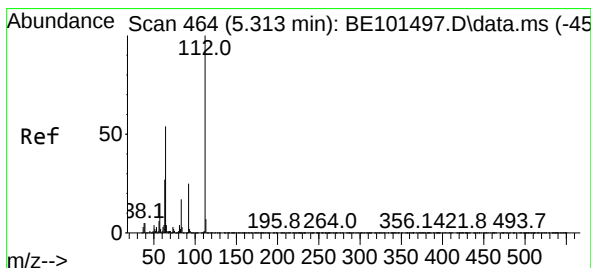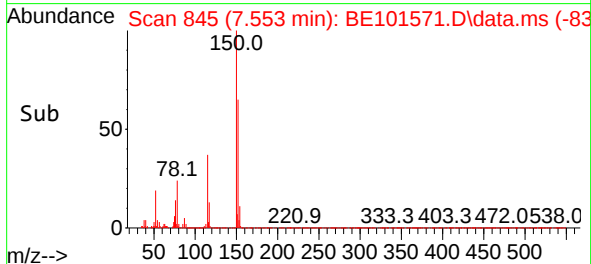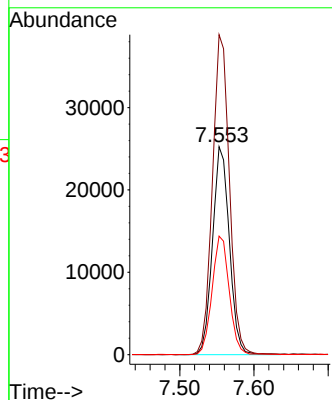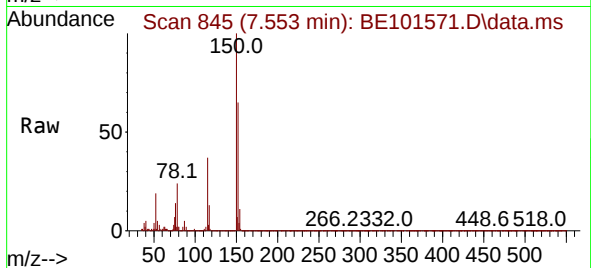

#5
 2-Fluorophenol
 Concen: 164.159 ng
 RT: 5.309 min Scan# 463
 Delta R.T. -0.004 min
 Lab File: BE101571.D
 Acq: 11 Nov 2024 14:33

Tgt Ion:112 Resp: 368633
 Ion Ratio Lower Upper
 112 100
 64 55.9 43.2 64.8
 63 28.5 21.8 32.6


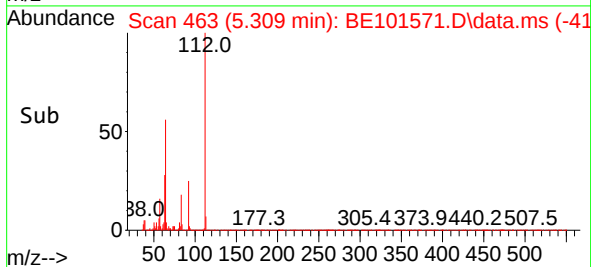
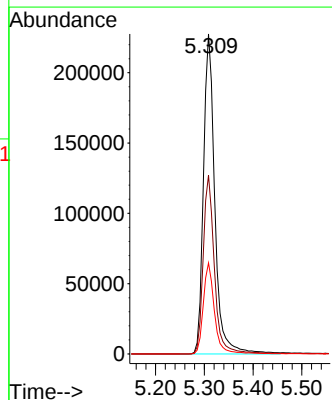
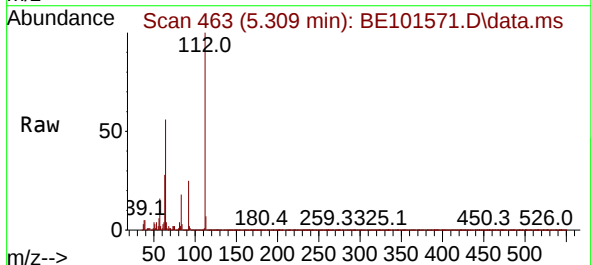


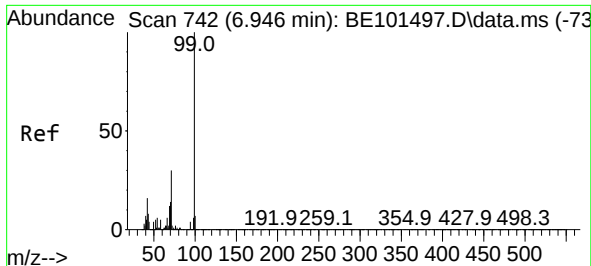

#7
Phenol-d6
Concen: 137.667 ng
RT: 6.936 min Scan# 742
Delta R.T. -0.010 min
Lab File: BE101571.D
Acq: 11 Nov 2024 14:33




Instrument :
BNA_E
ClientSampleId :
LAW-23-00189


Tgt Ion: 99 Resp: 423859
Ion Ratio Lower Upper
99 100
42 16.4 12.5 18.7
71 30.6 24.2 36.2

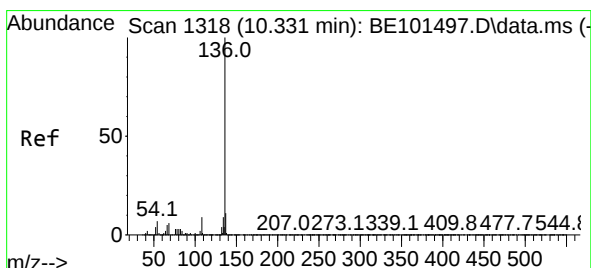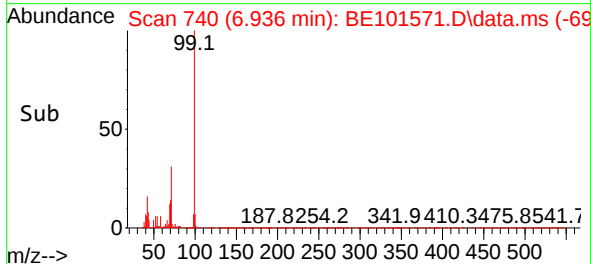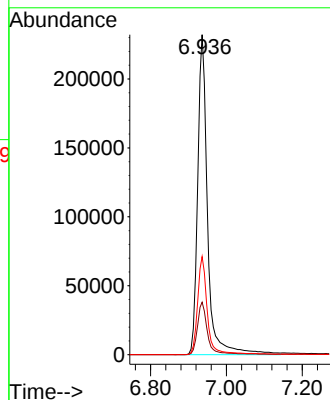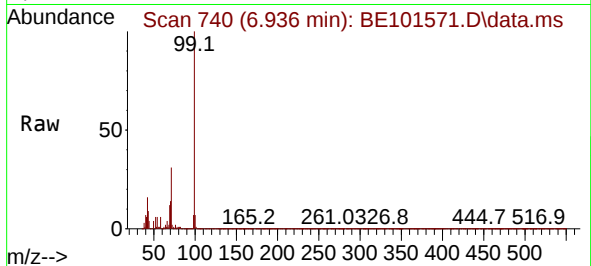

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.320 min Scan# 1316
Delta R.T. -0.010 min
Lab File: BE101571.D
Acq: 11 Nov 2024 14:33

Tgt Ion:136 Resp: 167207
Ion Ratio Lower Upper
136 100
137 10.6 8.6 13.0
54 7.5 5.6 8.4
68 6.0 4.8 7.2


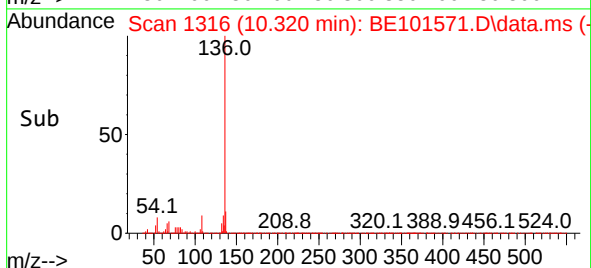
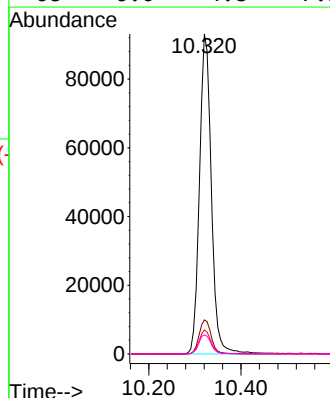
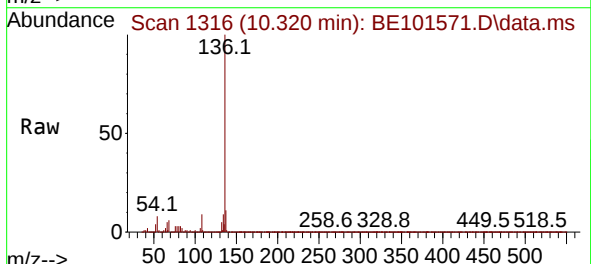


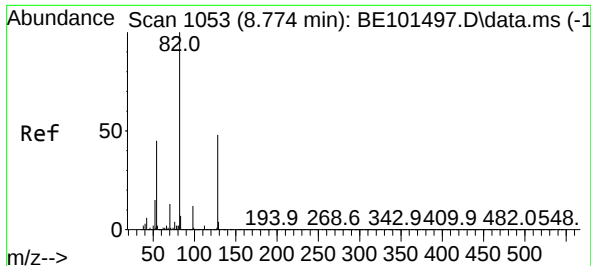

#23
Nitrobenzene-d5
Concen: 112.546 ng
RT: 8.763 min Scan# 1051
Delta R.T. -0.010 min
Lab File: BE101571.D
Acq: 11 Nov 2024 14:33




Instrument :
BNA_E
ClientSampleId :
LAW-23-00189


Tgt Ion: 82 Resp: 297927
Ion Ratio Lower Upper
82 100
128 46.4 38.6 58.0
54 46.2 36.3 54.5

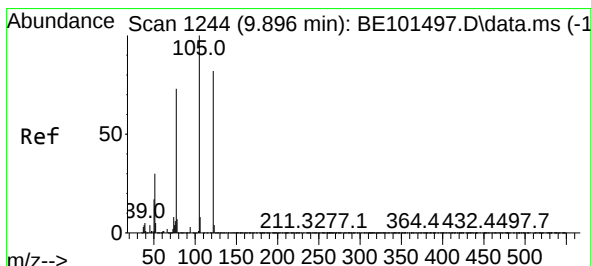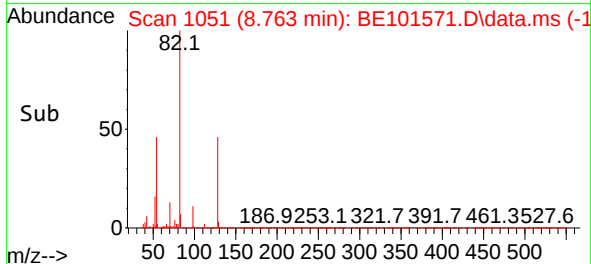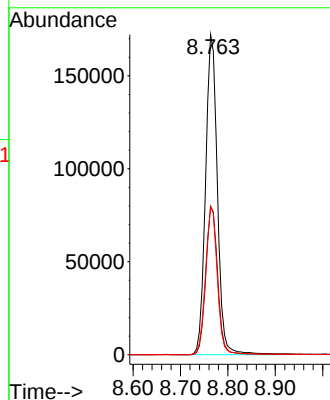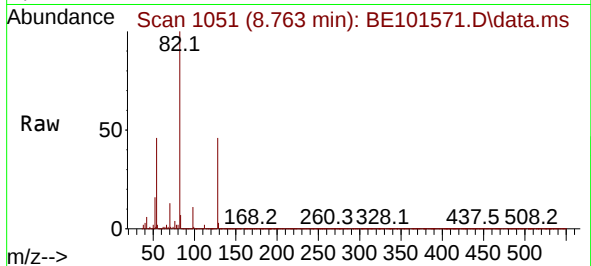

#32
Benzoic acid
Concen: 6.880 ng
RT: 9.962 min Scan# 1255
Delta R.T. 0.066 min
Lab File: BE101571.D
Acq: 11 Nov 2024 14:33

Tgt Ion: 122 Resp: 85
Ion Ratio Lower Upper
122 100
105 106.9 100.6 140.6
77 70.1 68.6 108.6


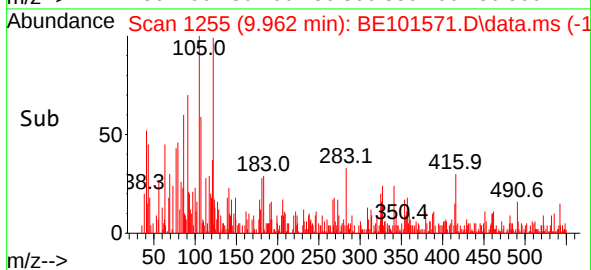
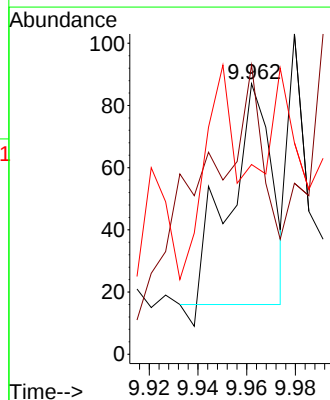
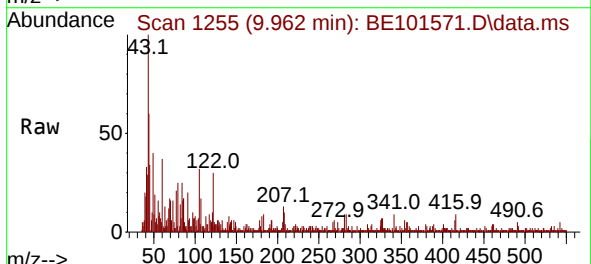


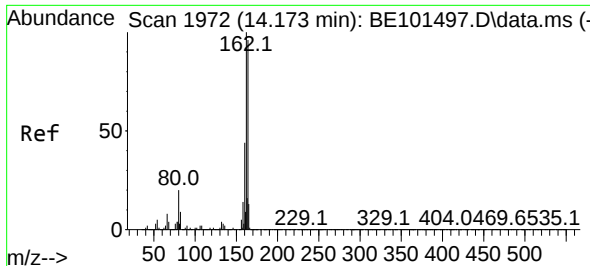

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.169 min Scan# 1972
Delta R.T. -0.004 min
Lab File: BE101571.D
Acq: 11 Nov 2024 14:33




Instrument :
BNA_E
ClientSampleId :
LAW-23-00189


Tgt Ion:164 Resp: 112501
Ion Ratio Lower Upper
164 100
162 101.4 83.7 125.5
160 44.3 37.1 55.7

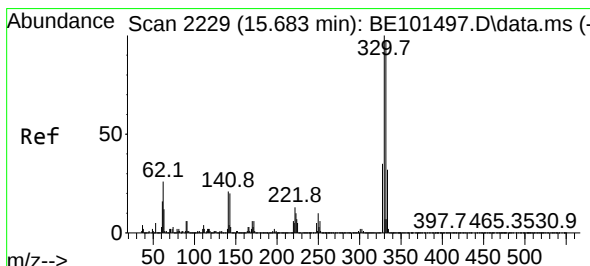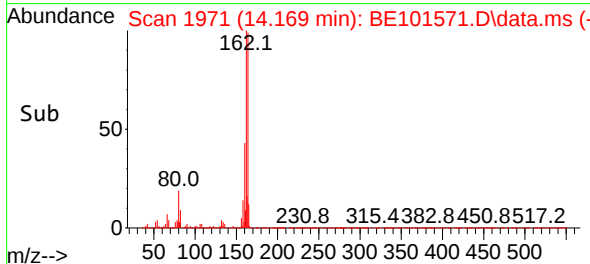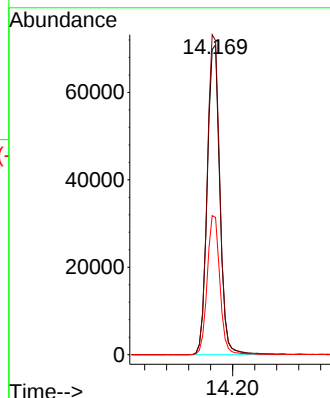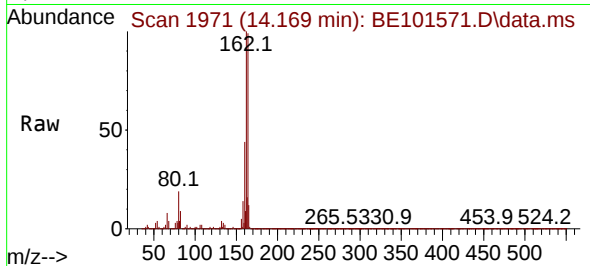

#42
2,4,6-Tribromophenol
Concen: 170.099 ng
RT: 15.673 min Scan# 2227
Delta R.T. -0.010 min
Lab File: BE101571.D
Acq: 11 Nov 2024 14:33

Tgt Ion:330 Resp: 360088
Ion Ratio Lower Upper
330 100
332 96.9 77.7 116.5
141 21.4 17.0 25.4

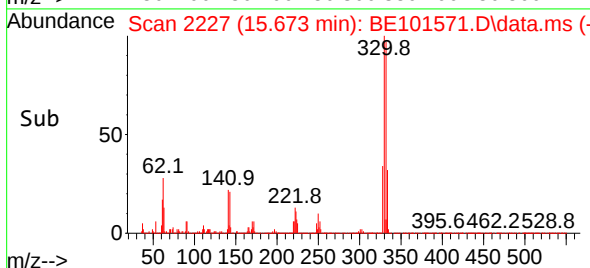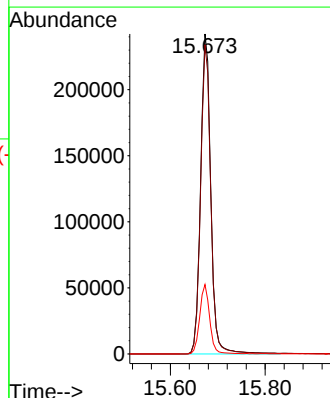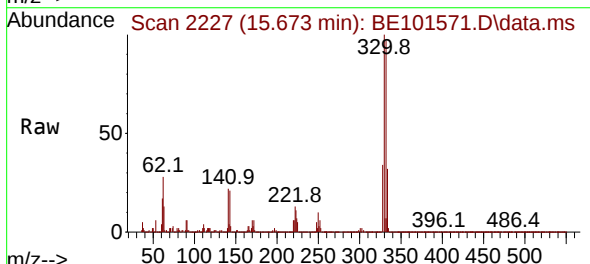

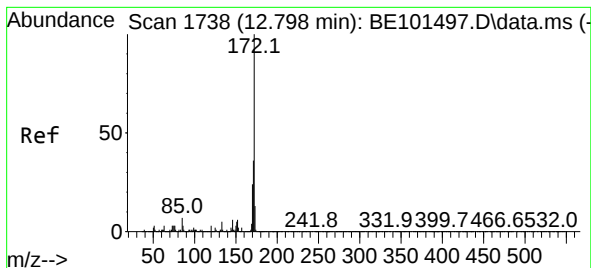

#45

2-Fluorobiphenyl

Concen: 104.551 ng

RT: 12.788 min Scan# 1

Delta R.T. -0.010 min

Lab File: BE101571.D

Acq: 11 Nov 2024 14:33

Instrument :

BNA_E

ClientSampleId :

LAW-23-00189





Tgt Ion:172 Resp: 720361

Ion Ratio Lower Upper

172 100

171 35.3 28.6 43.0

170 23.3 18.9 28.3

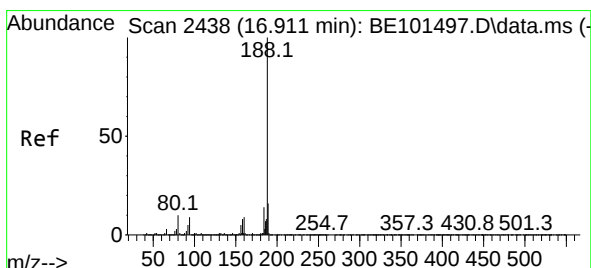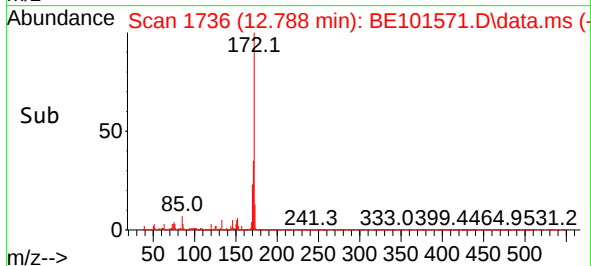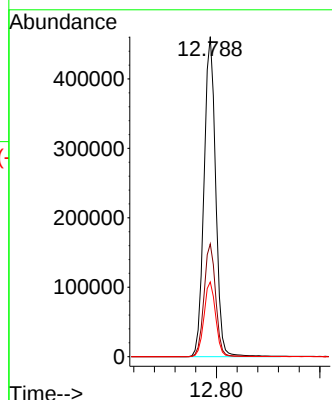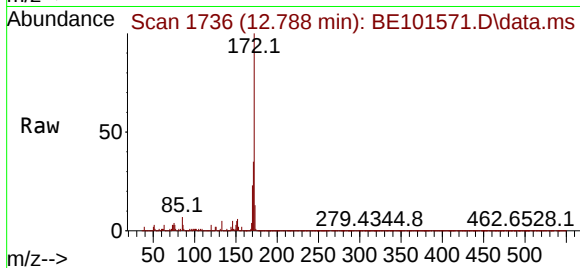

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.901 min Scan# 2436

Delta R.T. -0.010 min

Lab File: BE101571.D

Acq: 11 Nov 2024 14:33




Tgt Ion:188 Resp: 270240


Ion Ratio Lower Upper

188 100

94 9.3 7.4 11.2

80 10.7 8.0 12.0


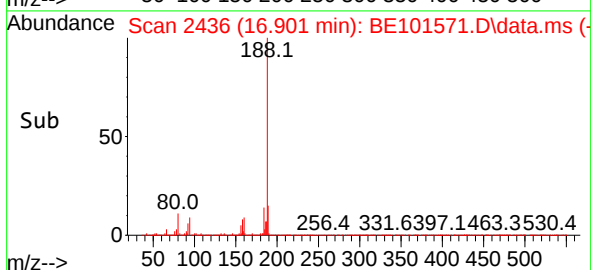
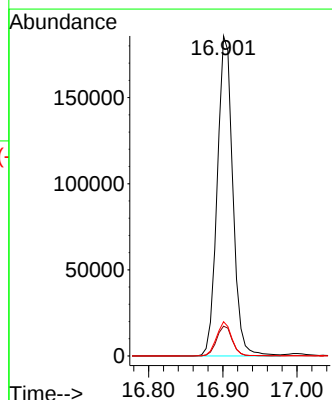
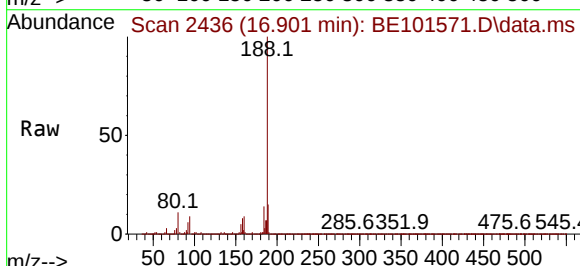


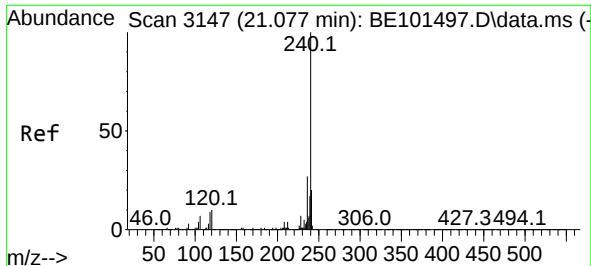

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.067 min Scan# 3147
Delta R.T. -0.010 min
Lab File: BE101571.D
Acq: 11 Nov 2024 14:33




Instrument :
BNA_E
ClientSampleId :
LAW-23-00189


Tgt Ion:240 Resp: 338714
Ion Ratio Lower Upper
240 100
120 10.6 8.2 12.4
236 26.9 21.4 32.2

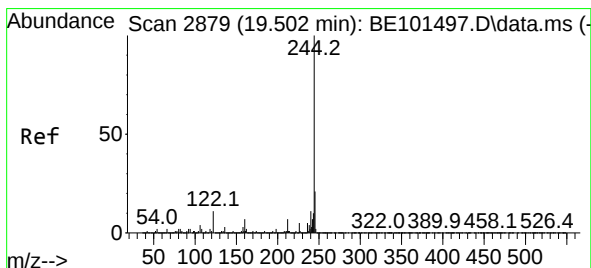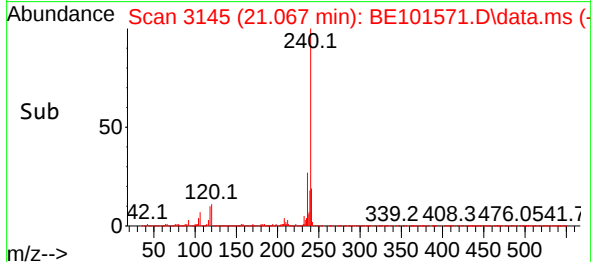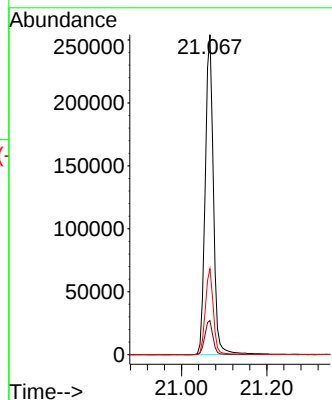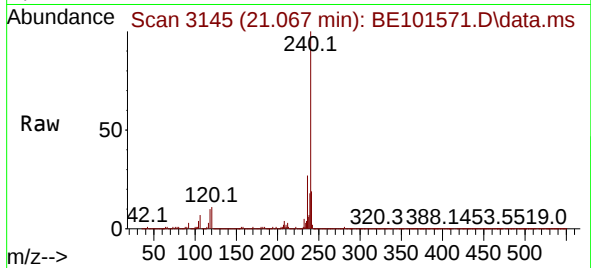

#79
Terphenyl-d14
Concen: 118.884 ng
RT: 19.498 min Scan# 2878
Delta R.T. -0.004 min
Lab File: BE101571.D
Acq: 11 Nov 2024 14:33

Tgt Ion:244 Resp: 1819130
Ion Ratio Lower Upper
244 100
212 6.9 5.8 8.8
122 10.7 8.4 12.6

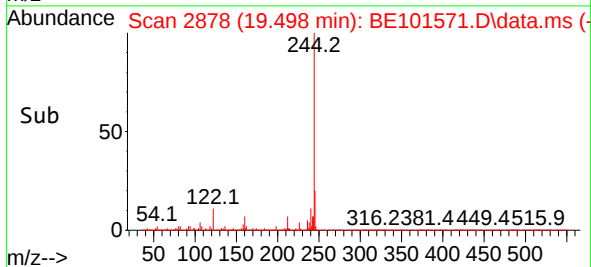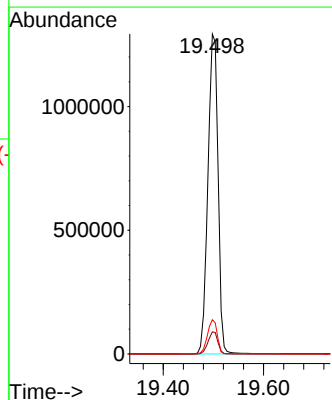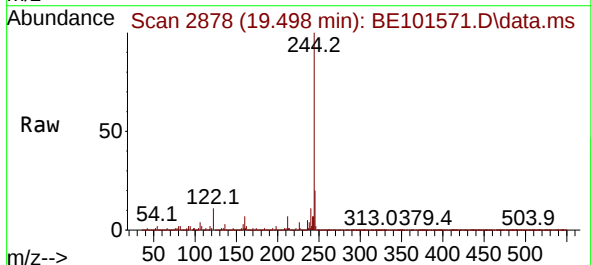

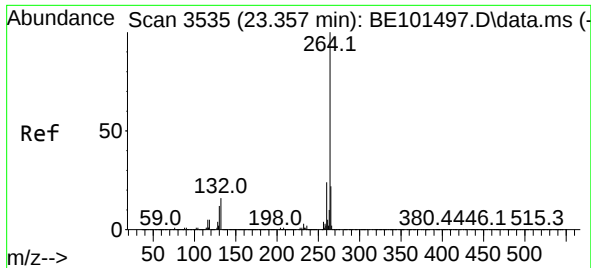

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.346 min Scan# 31
Delta R.T. -0.010 min
Lab File: BE101571.D
Acq: 11 Nov 2024 14:33

Instrument :
BNA_E
ClientSampleId :
LAW-23-00189

Tgt Ion:264 Resp: 425347
Ion Ratio Lower Upper
264 100
260 24.0 19.4 29.2
265 21.6 17.4 26.2

