
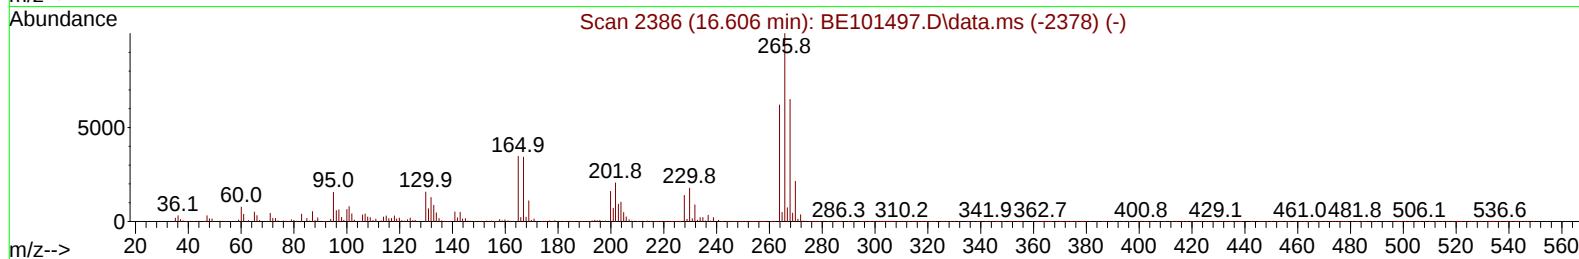
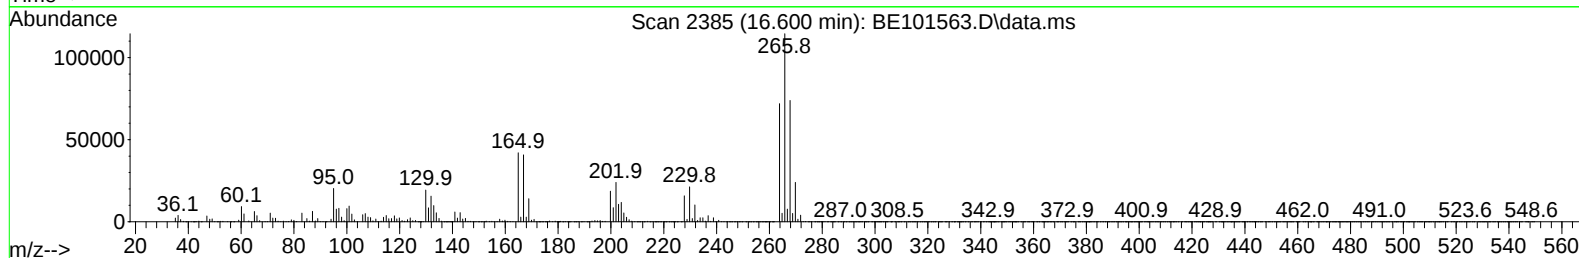


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111124\
Data File : BE101563.D
Acq On : 11 Nov 2024 9:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 10:20:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

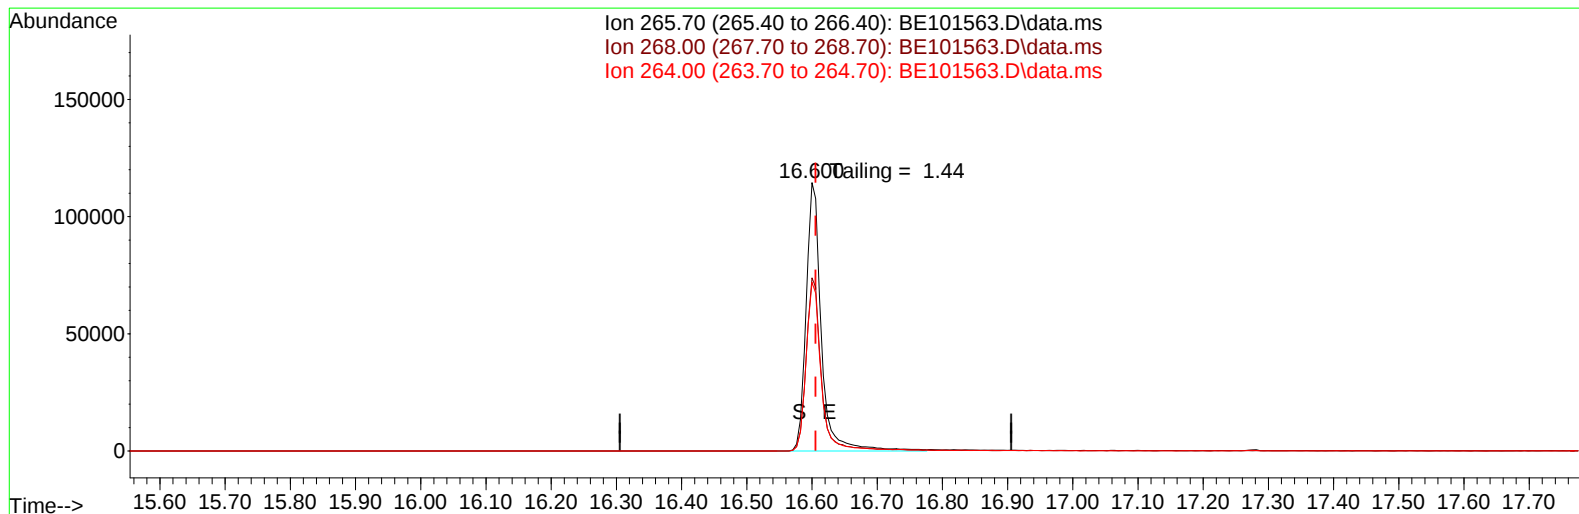

TIC: BE101563.D\data.ms

(70) Pentachlorophenol (C)




16.600min (-0.006) 2640600.09 ng

response 187173

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	64.53
264.00	62.00	62.83
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111124\  
Data File : BE101563.D  
Acq On    : 11 Nov 2024    9:43  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 11 10:20:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

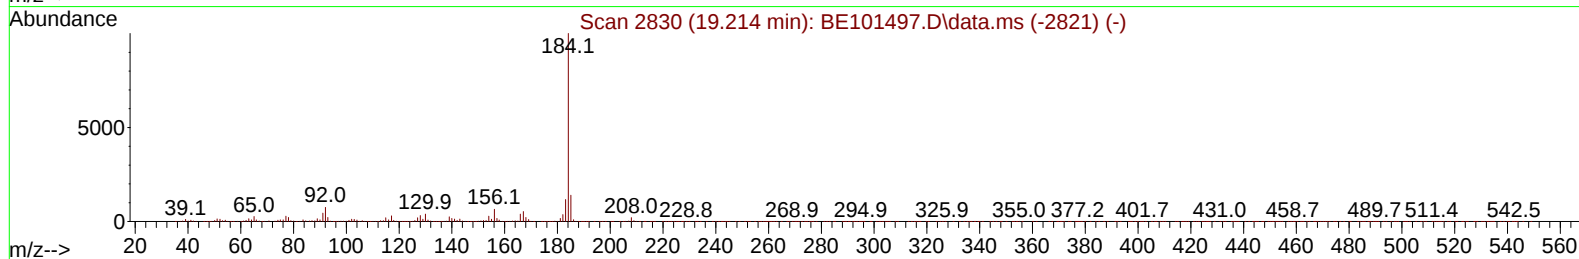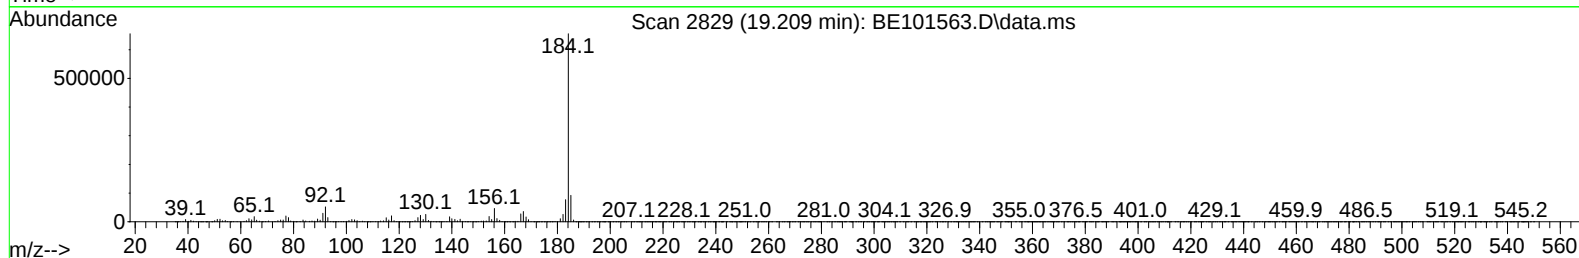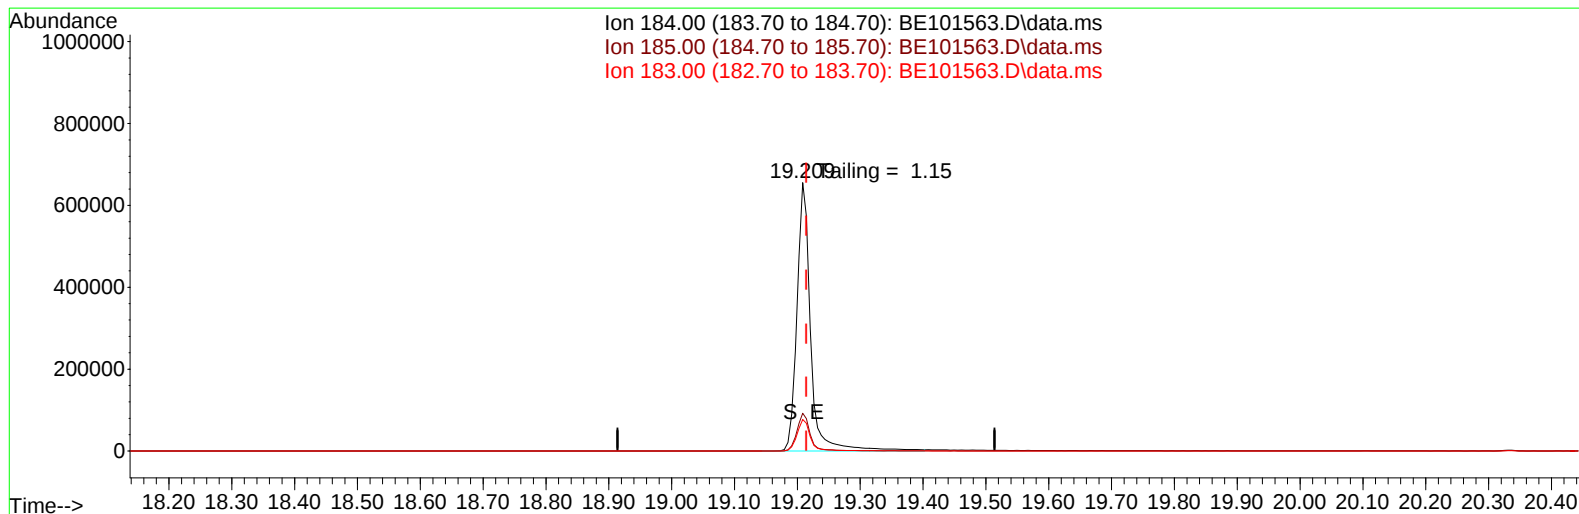

TIC: BE101563.D\data.ms

(77) Benzidine

19.209min (-0.005) 1105299.77 ng

response 997202

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.07
183.00	11.70	11.78
0.00	0.00	0.00