
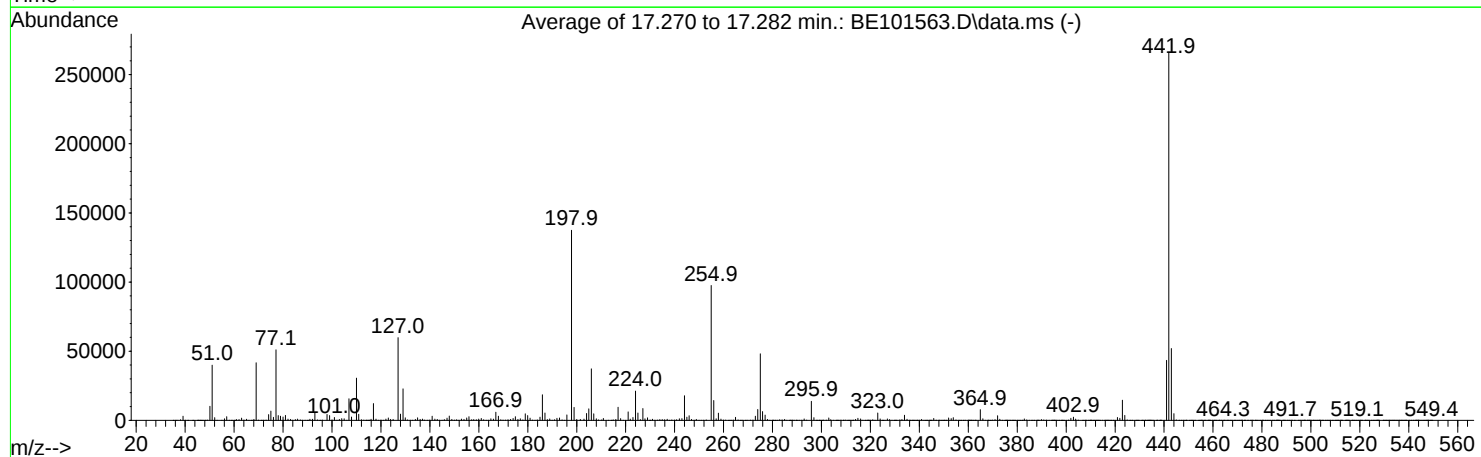


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111124\
Data File : BE101563.D
Acq On : 11 Nov 2024 9:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 07 00:01:20 2024

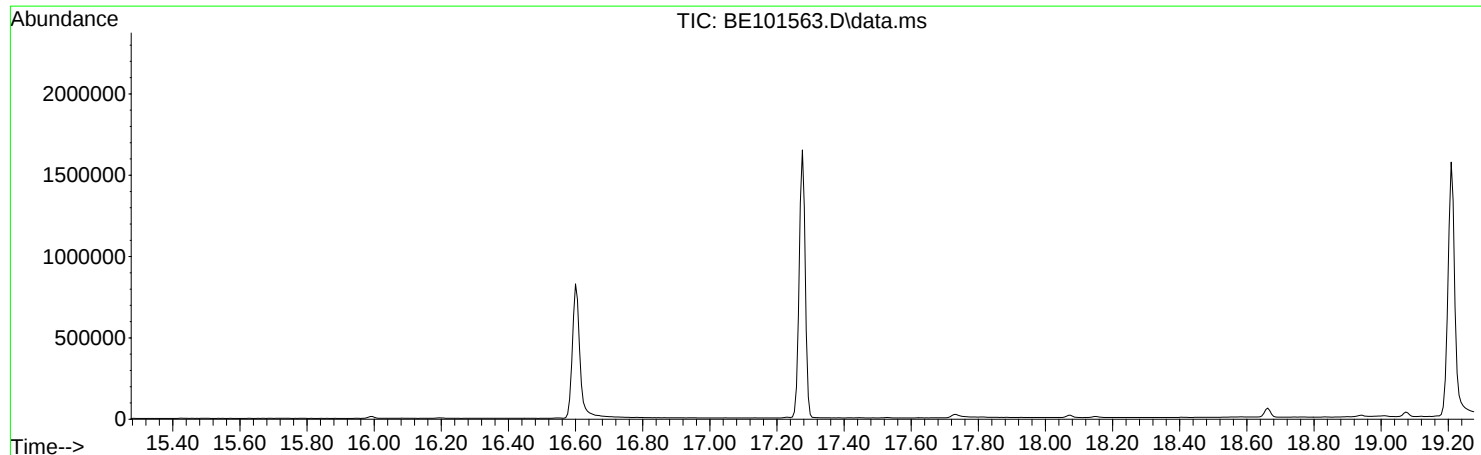




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	39897	PASS
68	69	0.00	2	1.8	758	PASS
69	198	0.00	100	30.3	41620	PASS
70	69	0.00	2	0.5	219	PASS
127	198	10	80	43.6	59887	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	137465	PASS
199	198	5	9	6.9	9428	PASS
275	198	10	60	35.0	48115	PASS
365	198	1	100	5.7	7810	PASS
441	198	0.01	100	31.6	43427	PASS
442	442	50	100	100.0	266002	PASS
443	442	15	24	19.6	52008	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111124\
Data File : BE101563.D
Acq On : 11 Nov 2024 9:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 11 10:20:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

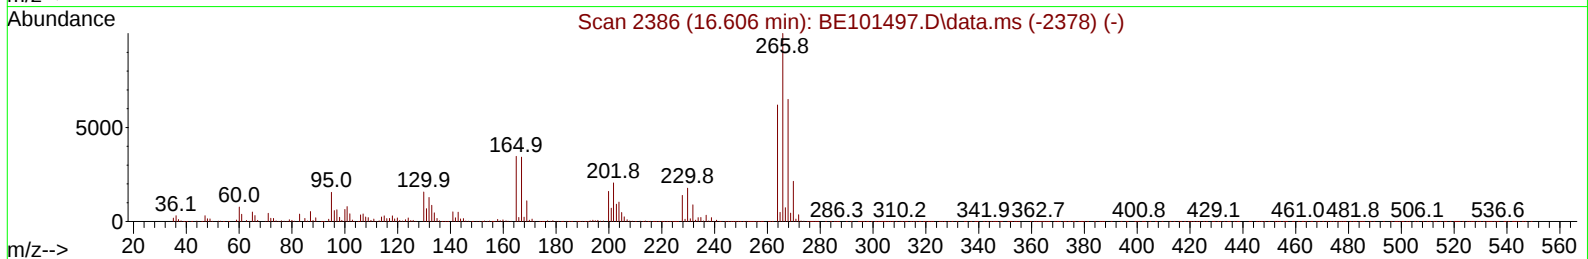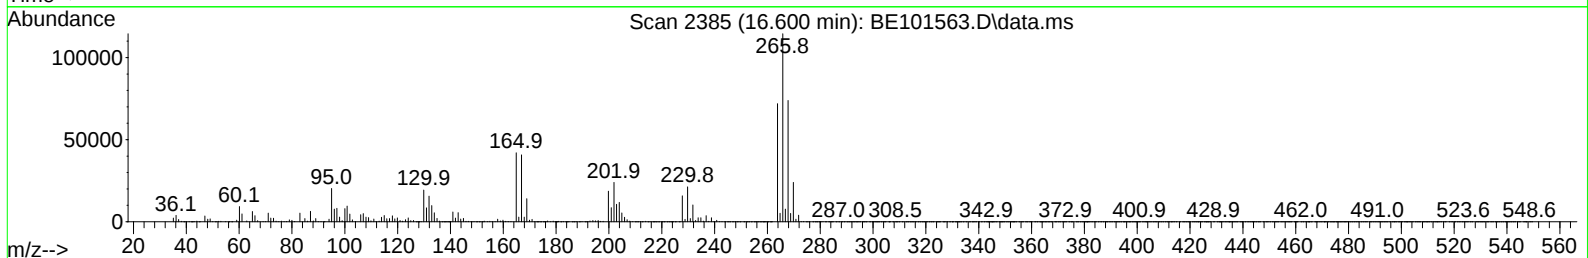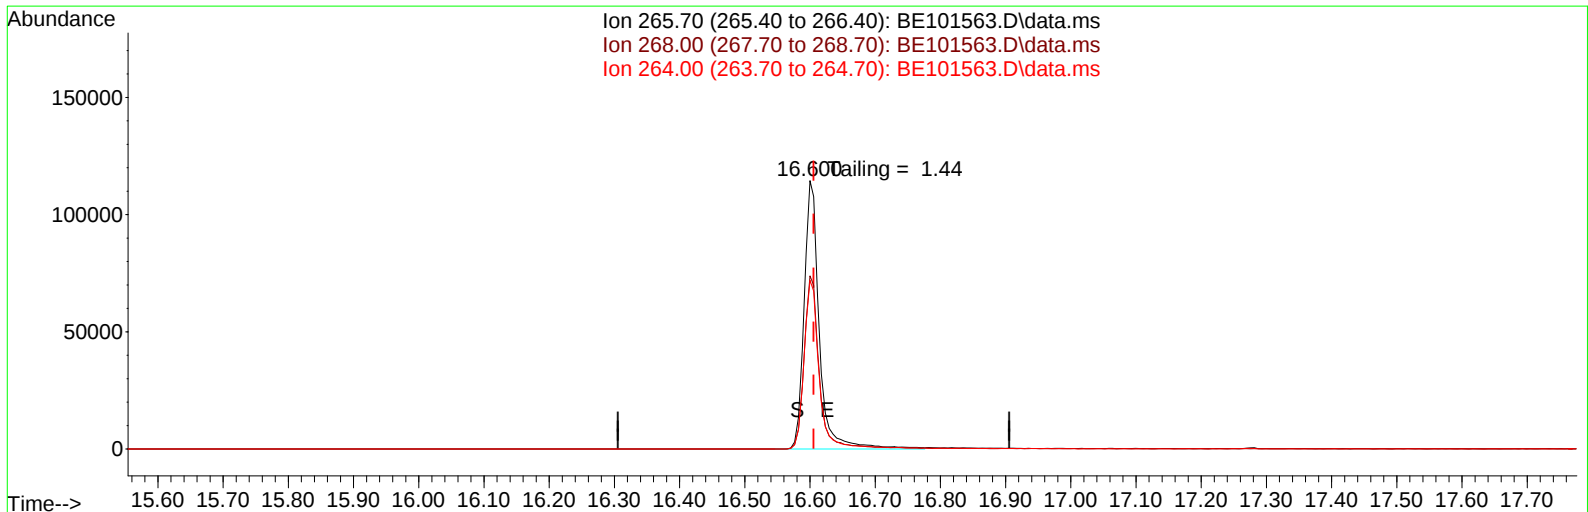

TIC: BE101563.D\data.ms

(70) Pentachlorophenol (C)

16.600min (-0.006) 2640600.09 ng

response 187173

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	64.53
264.00	62.00	62.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2024	BNA_E	<u>BE101563.D</u>
Compound Name	Response	Retention Time
DDT	616827	20.331
DDD	10976	19.955
DDE	415	19.391
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11391	628218	1.81

Instrument :
BNA_E
ClientSampleId :
DFTPP