

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101578.D
Acq On : 12 Nov 2024 12:29
Operator : RC/JU
Sample : P4722-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
WC-1(0-6)

Quant Time: Nov 12 13:03:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.553	152	37247	20.000	ng	-0.01
21) Naphthalene-d8	10.320	136	175455	20.000	ng	-0.01
39) Acenaphthene-d10	14.163	164	135773	20.000	ng	-0.01
64) Phenanthrene-d10	16.901	188	333737	20.000	ng	-0.01
76) Chrysene-d12	21.060	240	375483	20.000	ng	-0.02
86) Perylene-d12	23.346	264	475775	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.308	112	141573	67.207	ng	0.00
7) Phenol-d6	6.930	99	132207	45.775	ng	-0.02
23) Nitrobenzene-d5	8.763	82	260141	93.652	ng	-0.01
42) 2,4,6-Tribromophenol	15.673	330	389053	152.281	ng	-0.01
45) 2-Fluorobiphenyl	12.788	172	746659	89.793	ng	-0.01
79) Terphenyl-d14	19.498	244	1890961	111.477	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101578.D
Acq On : 12 Nov 2024 12:29
Operator : RC/JU
Sample : P4722-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
WC-1(0-6)

Quant Time: Nov 12 13:03:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

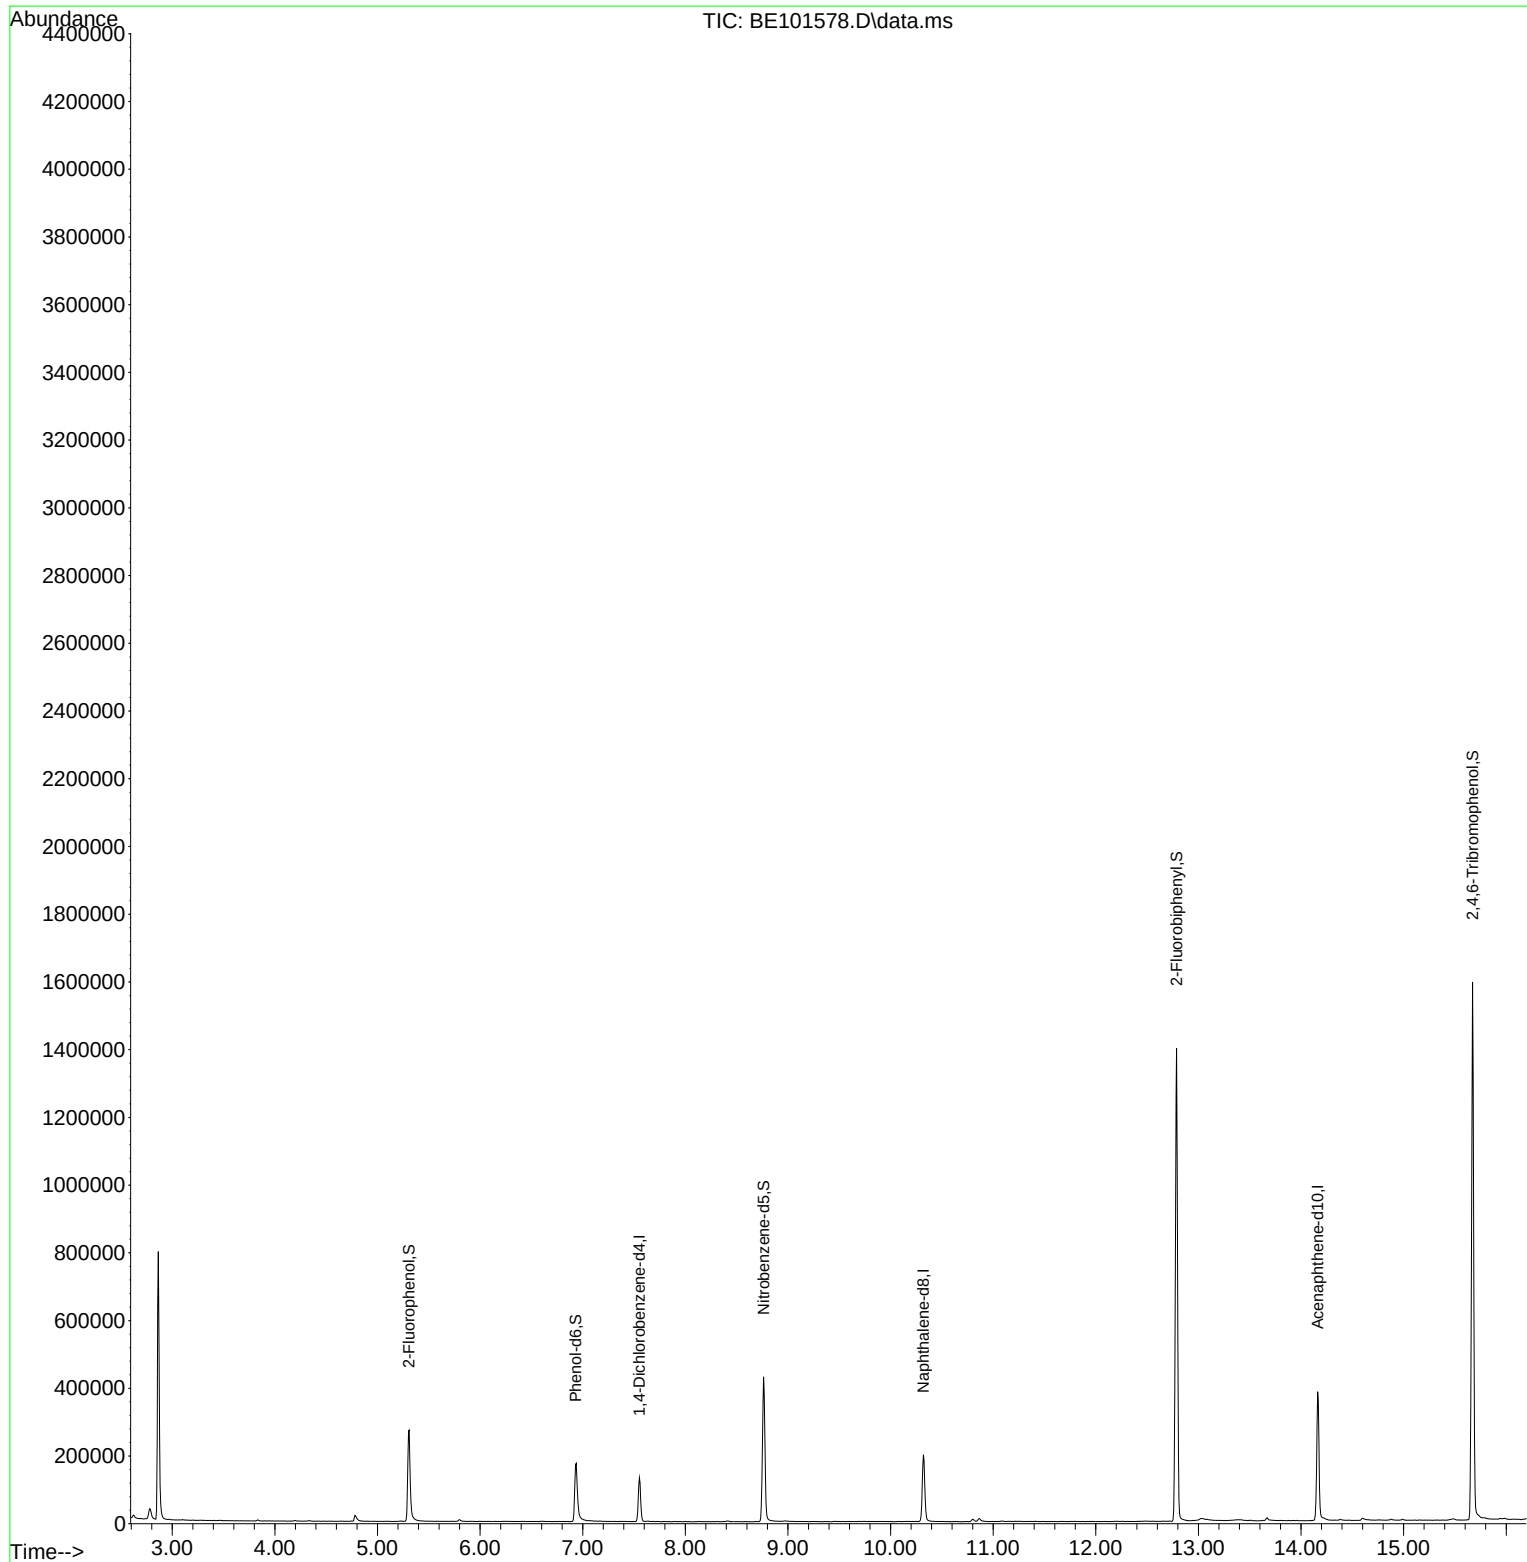

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101578.D
Acq On : 12 Nov 2024 12:29
Operator : RC/JU
Sample : P4722-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
WC-1(0-6)

Quant Time: Nov 12 13:03:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

