

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
 Data File : BE101580.D
 Acq On : 12 Nov 2024 13:38
 Operator : RC/JU
 Sample : P4722-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 WC-3(0-6)

Quant Time: Nov 12 14:09:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.556	152	34645	20.000	ng	0.00
21) Naphthalene-d8	10.323	136	155605	20.000	ng	0.00
39) Acenaphthene-d10	14.166	164	110687	20.000	ng	0.00
64) Phenanthrene-d10	16.904	188	269350	20.000	ng	0.00
76) Chrysene-d12	21.063	240	314208	20.000	ng	-0.01
86) Perylene-d12	23.343	264	409924	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.305	112	136411	69.620	ng	0.00
7) Phenol-d6	6.933	99	112470	41.866	ng	-0.01
23) Nitrobenzene-d5	8.760	82	242123	98.285	ng	-0.01
42) 2,4,6-Tribromophenol	15.676	330	334056	160.388	ng	0.00
45) 2-Fluorobiphenyl	12.785	172	667349	98.444	ng	-0.01
79) Terphenyl-d14	19.500	244	1730505	121.912	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101580.D
Acq On : 12 Nov 2024 13:38
Operator : RC/JU
Sample : P4722-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
WC-3(0-6)

Quant Time: Nov 12 14:09:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

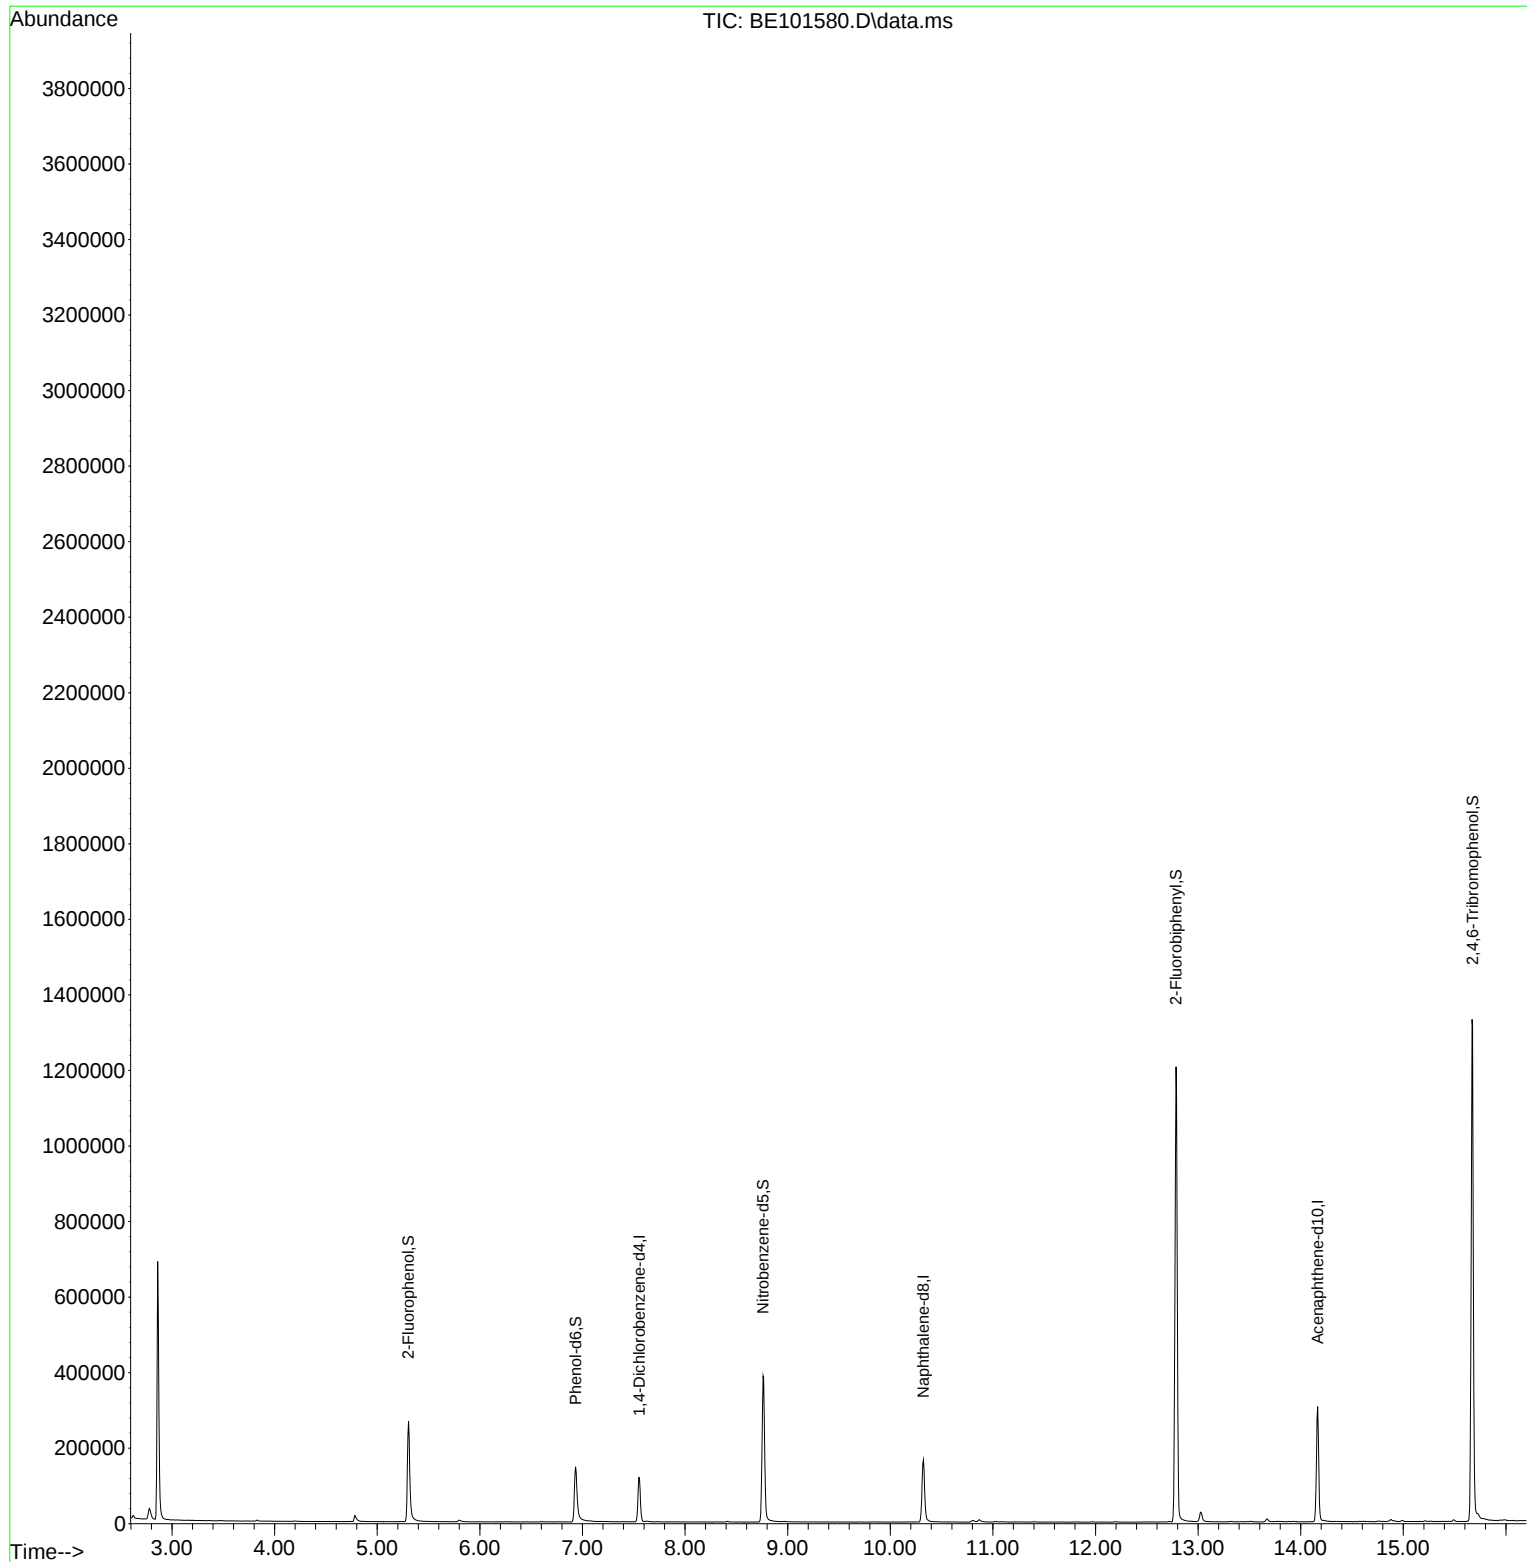

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101580.D
Acq On : 12 Nov 2024 13:38
Operator : RC/JU
Sample : P4722-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
WC-3(0-6)

Quant Time: Nov 12 14:09:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

