

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
 Data File : BE101587.D
 Acq On : 12 Nov 2024 22:14
 Operator : RC/JU
 Sample : P4722-08DL 2X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 WC-2(0-6)DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2024
 Supervised By :mohammad ahmed 11/13/2024

Quant Time: Nov 13 00:18:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.554	152	51821	20.000	ng	0.00
21) Naphthalene-d8	10.322	136	245161	20.000	ng	0.00
39) Acenaphthene-d10	14.164	164	168214	20.000	ng	0.00
64) Phenanthrene-d10	16.902	188	358727	20.000	ng	0.00
76) Chrysene-d12	21.068	240	362587	20.000	ng	0.00
86) Perylene-d12	23.353	264	466663	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.310	112	158923	54.226	ng	0.00
7) Phenol-d6	6.937	99	213942	53.242	ng	0.00
23) Nitrobenzene-d5	8.765	82	127245	32.784	ng	0.00
42) 2,4,6-Tribromophenol	15.674	330	137753	43.520	ng	0.00
45) 2-Fluorobiphenyl	12.783	172	355877	34.544	ng	-0.02
79) Terphenyl-d14	19.493	244	615043	37.548	ng	0.00
Target Compounds						Qvalue
31) Naphthalene	10.368	128	25371	2.050	ng	98
49) Acenaphthylene	13.900	152	32325	2.370	ng	99
52) Acenaphthene	14.229	154	29014	3.334	ng	98
58) Fluorene	15.210	166	29783	2.546	ng	99
71) Phenanthrene	16.943	178	534906	30.658	ng	99
72) Anthracene	17.031	178	132407	7.685	ng	96
73) Carbazole	17.360	167	45772	2.649	ng	100
75) Fluoranthene	18.953	202	854737	38.209	ng	100
78) Pyrene	19.323	202	794993	38.534	ng	99
81) Benzo(a)anthracene	21.044	228	455100	21.134	ng	99
83) Chrysene	21.103	228	422633	20.648	ng	98
87) Indeno(1,2,3-cd)pyrene	25.668	276	387507	12.083	ng	95
88) Benzo(b)fluoranthene	22.642	252	557363	21.769	ng	98
89) Benzo(k)fluoranthene	22.678	252	312950m	13.465	ng	
90) Benzo(a)pyrene	23.242	252	488034	22.079	ng	99
91) Dibenzo(a,h)anthracene	25.645	278	105695	3.957	ng	92
92) Benzo(g,h,i)perylene	26.420	276	382221	14.086	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101587.D
Acq On : 12 Nov 2024 22:14
Operator : RC/JU
Sample : P4722-08DL 2X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
WC-2(0-6)DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/13/2024

Quant Time: Nov 13 00:18:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

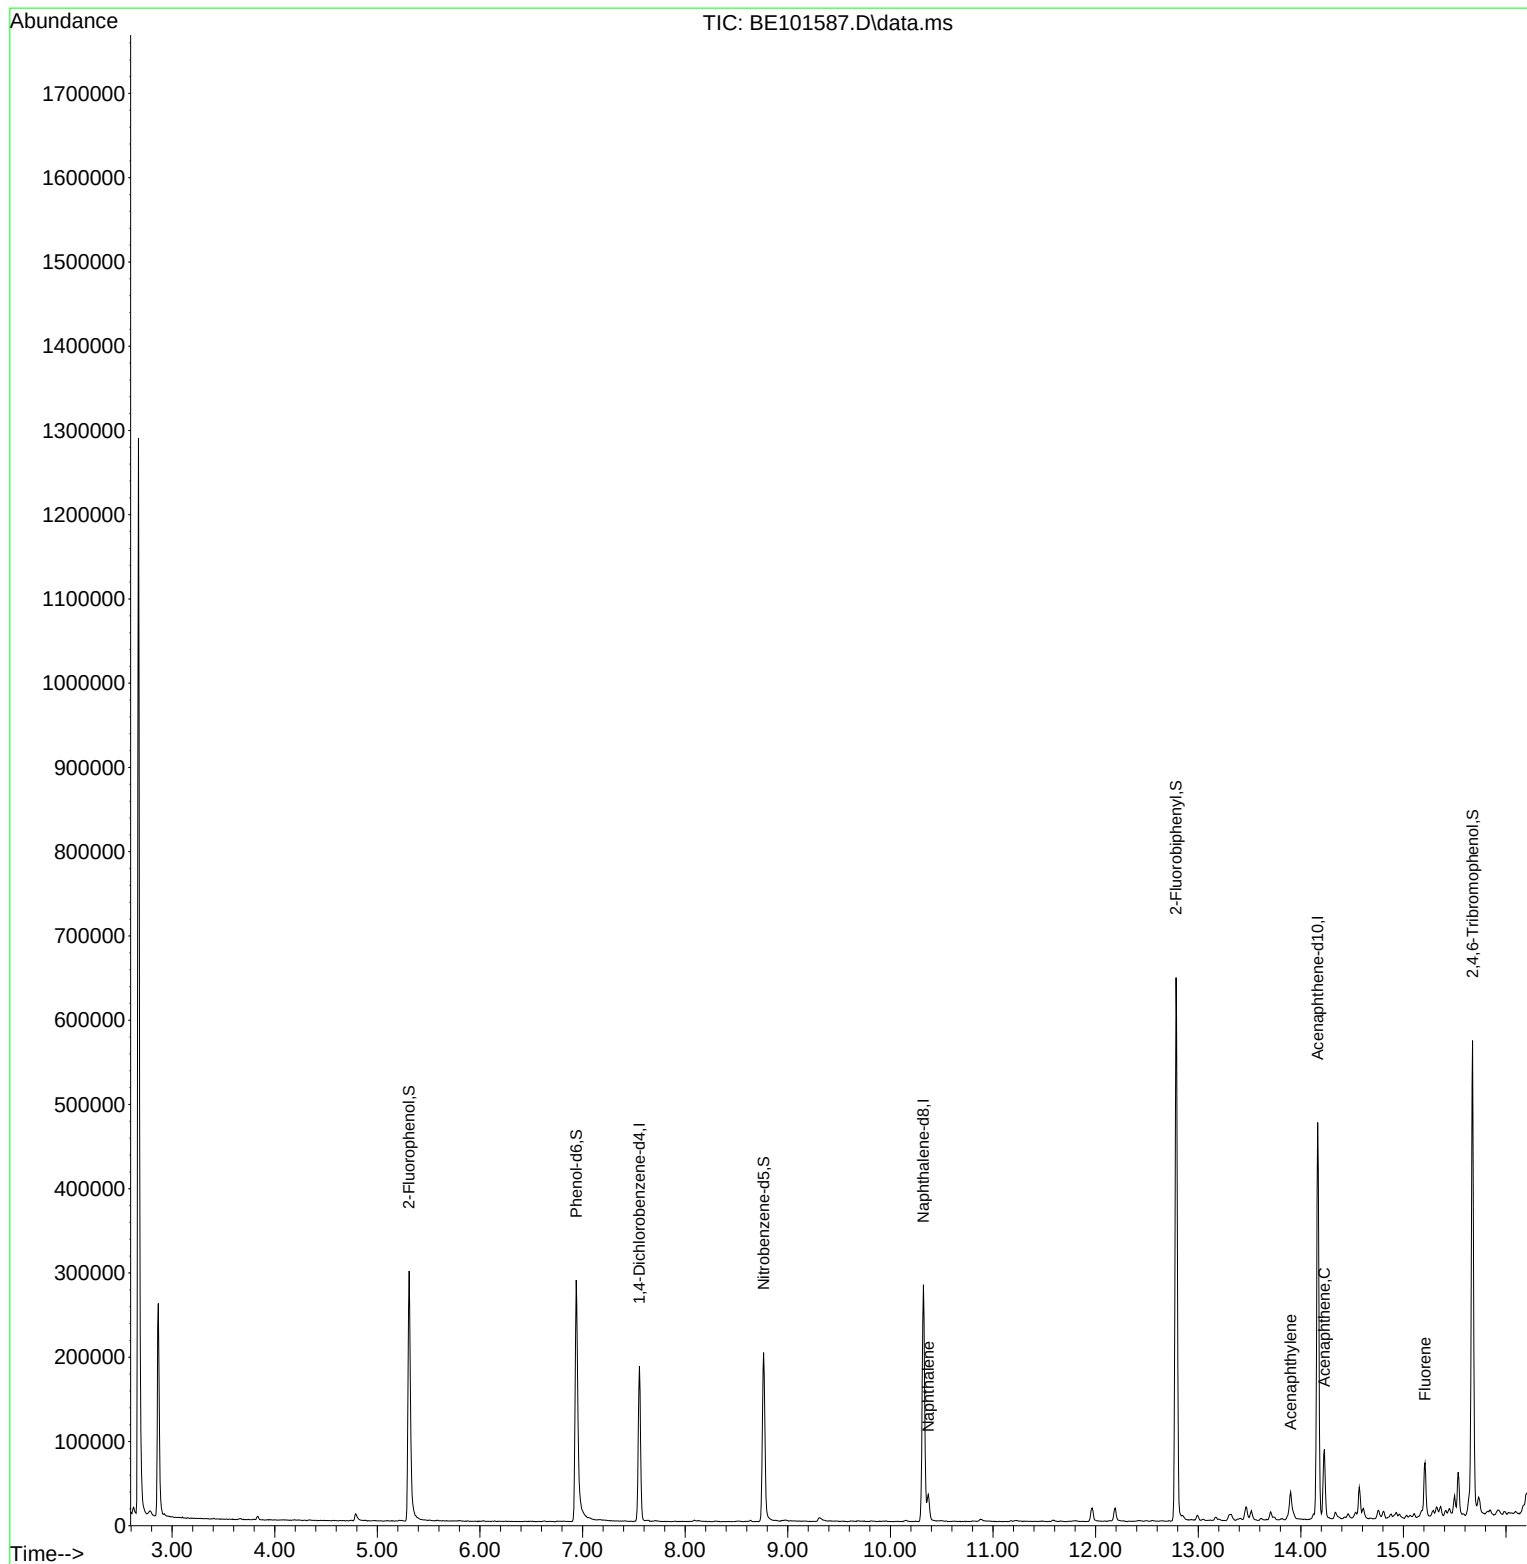

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101587.D
Acq On : 12 Nov 2024 22:14
Operator : RC/JU
Sample : P4722-08DL 2X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
WC-2(0-6)DL

Quant Time: Nov 13 00:18:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/13/2024

