

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
 Data File : BE101588.D
 Acq On : 12 Nov 2024 22:50
 Operator : RC/JU
 Sample : P4768-06DL 2X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-6-2DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2024
 Supervised By :mohammad ahmed 11/13/2024

Quant Time: Nov 13 00:18:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.552	152	53219	20.000	ng	-0.01
21) Naphthalene-d8	10.320	136	241831	20.000	ng	-0.01
39) Acenaphthene-d10	14.168	164	163173	20.000	ng	0.00
64) Phenanthrene-d10	16.906	188	354194	20.000	ng	0.00
76) Chrysene-d12	21.066	240	366638	20.000	ng	-0.01
86) Perylene-d12	23.351	264	478806	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.308	112	121122	40.242	ng	0.00
7) Phenol-d6	6.941	99	161141	39.048	ng	0.00
23) Nitrobenzene-d5	8.763	82	95283	24.887	ng	-0.01
42) 2,4,6-Tribromophenol	15.672	330	106170	34.578	ng	-0.01
45) 2-Fluorobiphenyl	12.787	172	273405	27.358	ng	-0.01
79) Terphenyl-d14	19.497	244	514083	31.038	ng	0.00
Target Compounds						Qvalue
49) Acenaphthylene	13.898	152	65119	4.922	ng	97
58) Fluorene	15.208	166	31711	2.795	ng	# 98
71) Phenanthrene	16.947	178	546695	31.735	ng	99
72) Anthracene	17.029	178	155450	9.138	ng	98
75) Fluoranthene	18.957	202	841620	38.104	ng	100
78) Pyrene	19.321	202	692212	33.182	ng	100
81) Benzo(a)anthracene	21.048	228	488034	22.413	ng	99
83) Chrysene	21.101	228	389924	18.840	ng	97
87) Indeno(1,2,3-cd)pyrene	25.666	276	211123	6.416	ng	96
88) Benzo(b)fluoranthene	22.646	252	334503	12.734	ng	99
89) Benzo(k)fluoranthene	22.676	252	323257m	13.556	ng	
90) Benzo(a)pyrene	23.240	252	359102	15.834	ng	97
91) Dibenzo(a,h)anthracene	25.649	278	71844	2.622	ng	# 87
92) Benzo(g,h,i)perylene	26.418	276	174673	6.274	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101588.D
Acq On : 12 Nov 2024 22:50
Operator : RC/JU
Sample : P4768-06DL 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-6-2DL

Quant Time: Nov 13 00:18:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/13/2024

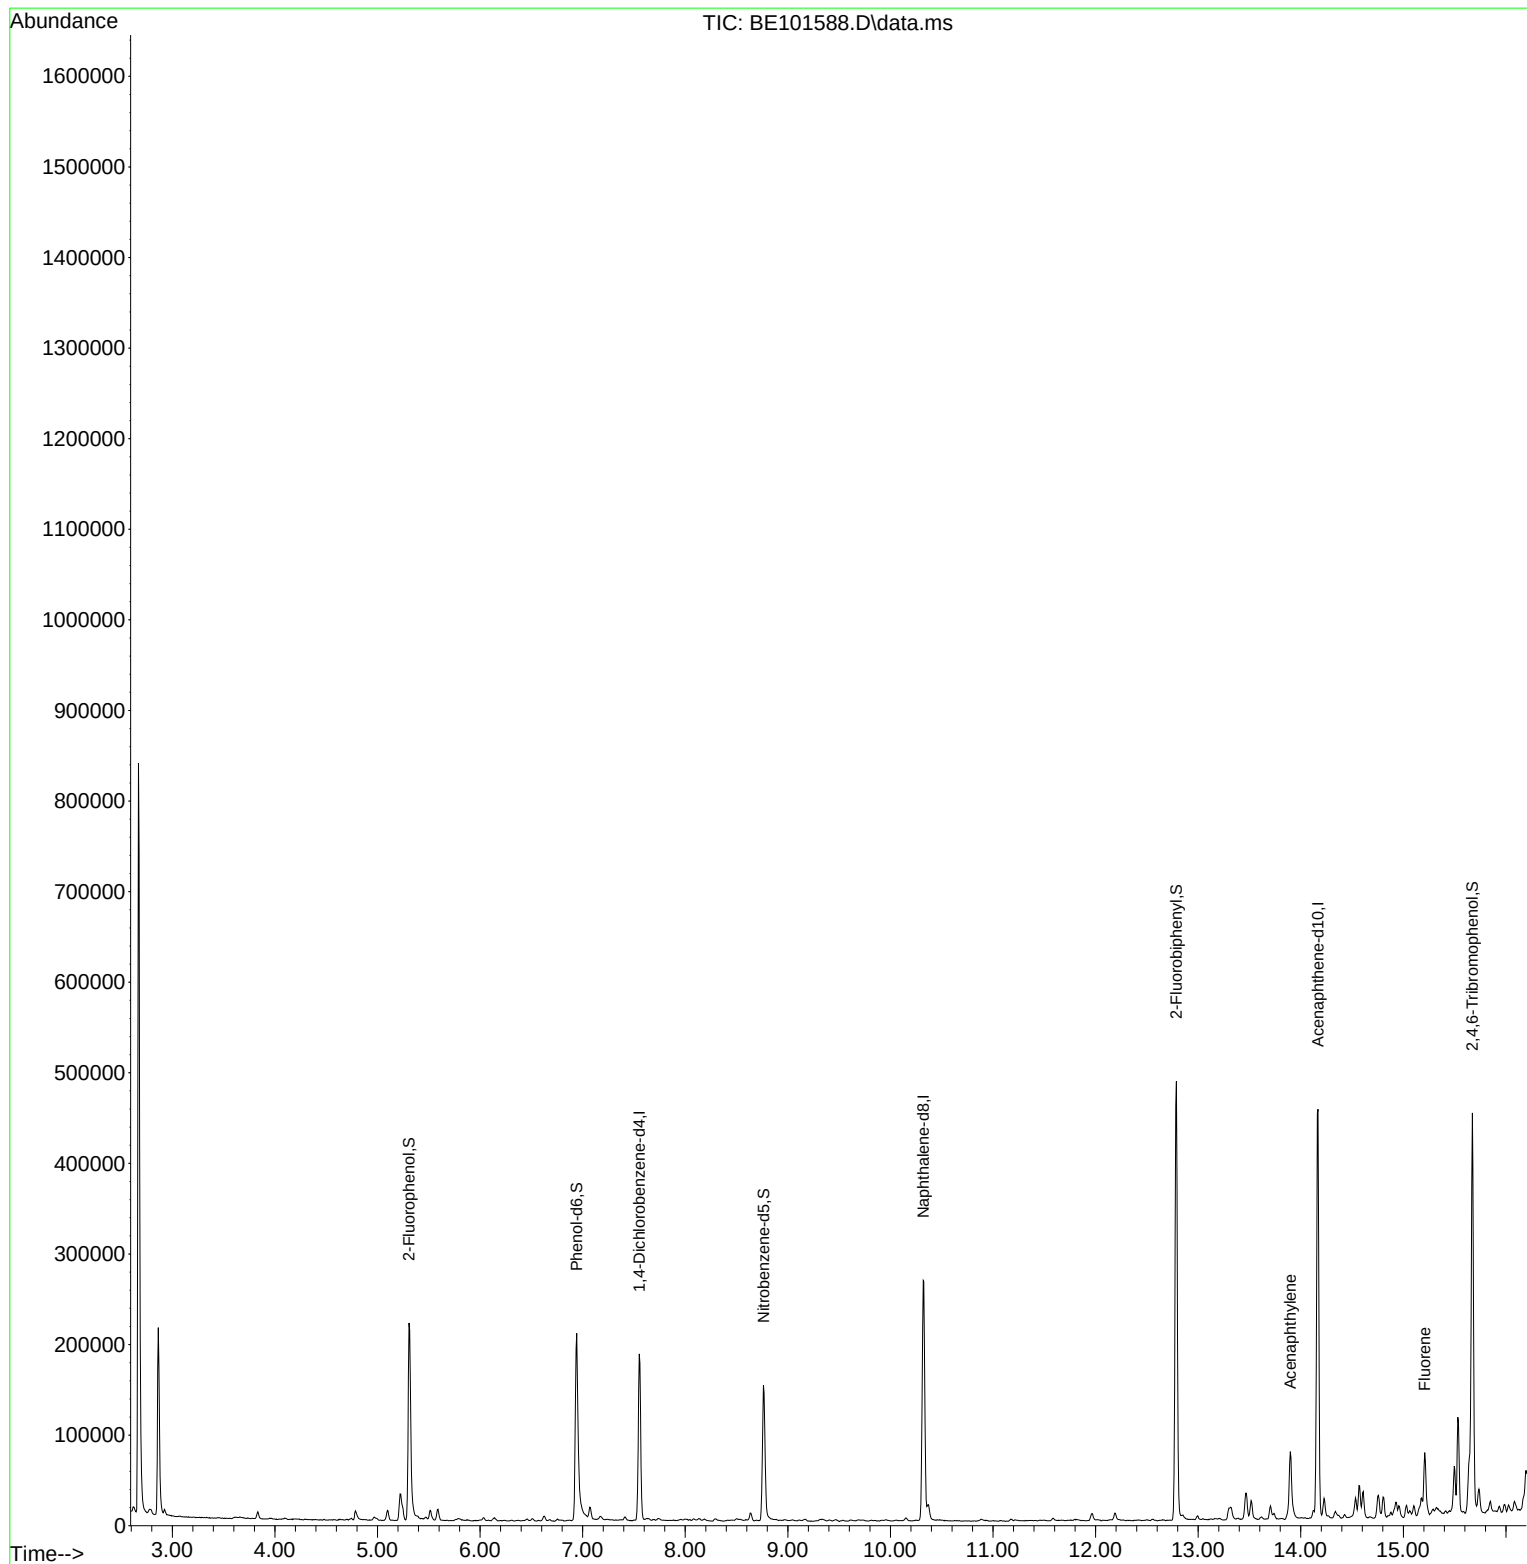

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101588.D
Acq On : 12 Nov 2024 22:50
Operator : RC/JU
Sample : P4768-06DL 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-6-2DL

Quant Time: Nov 13 00:18:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/13/2024

