

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
 Data File : BE101589.D
 Acq On : 12 Nov 2024 23:25
 Operator : RC/JU
 Sample : P4739-09DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-B2DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2024
 Supervised By :mohammad ahmed 11/13/2024

Quant Time: Nov 13 00:19:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	52986	20.000	ng	0.00
21) Naphthalene-d8	10.325	136	247444	20.000	ng	0.00
39) Acenaphthene-d10	14.168	164	164286	20.000	ng	0.00
64) Phenanthrene-d10	16.906	188	339948	20.000	ng	0.00
76) Chrysene-d12	21.065	240	335442	20.000	ng	-0.01
86) Perylene-d12	23.351	264	433450	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.313	112	55109	18.390	ng	0.00
7) Phenol-d6	6.941	99	75062	18.269	ng	0.00
23) Nitrobenzene-d5	8.768	82	48142	12.289	ng	0.00
42) 2,4,6-Tribromophenol	15.672	330	48092	15.557	ng	-0.01
45) 2-Fluorobiphenyl	12.787	172	133246	13.243	ng	-0.01
79) Terphenyl-d14	19.491	244	218237	14.401	ng	-0.01
Target Compounds					Qvalue	
31) Naphthalene	10.372	128	283444	22.690	ng	98
37) 2-Methylnaphthalene	11.964	142	164094	18.494	ng	100
38) 1-Methylnaphthalene	12.188	142	79990m	9.040	ng	
78) Pyrene	19.320	202	42429	2.223	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101589.D
Acq On : 12 Nov 2024 23:25
Operator : RC/JU
Sample : P4739-09DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-B2DL

Quant Time: Nov 13 00:19:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/13/2024

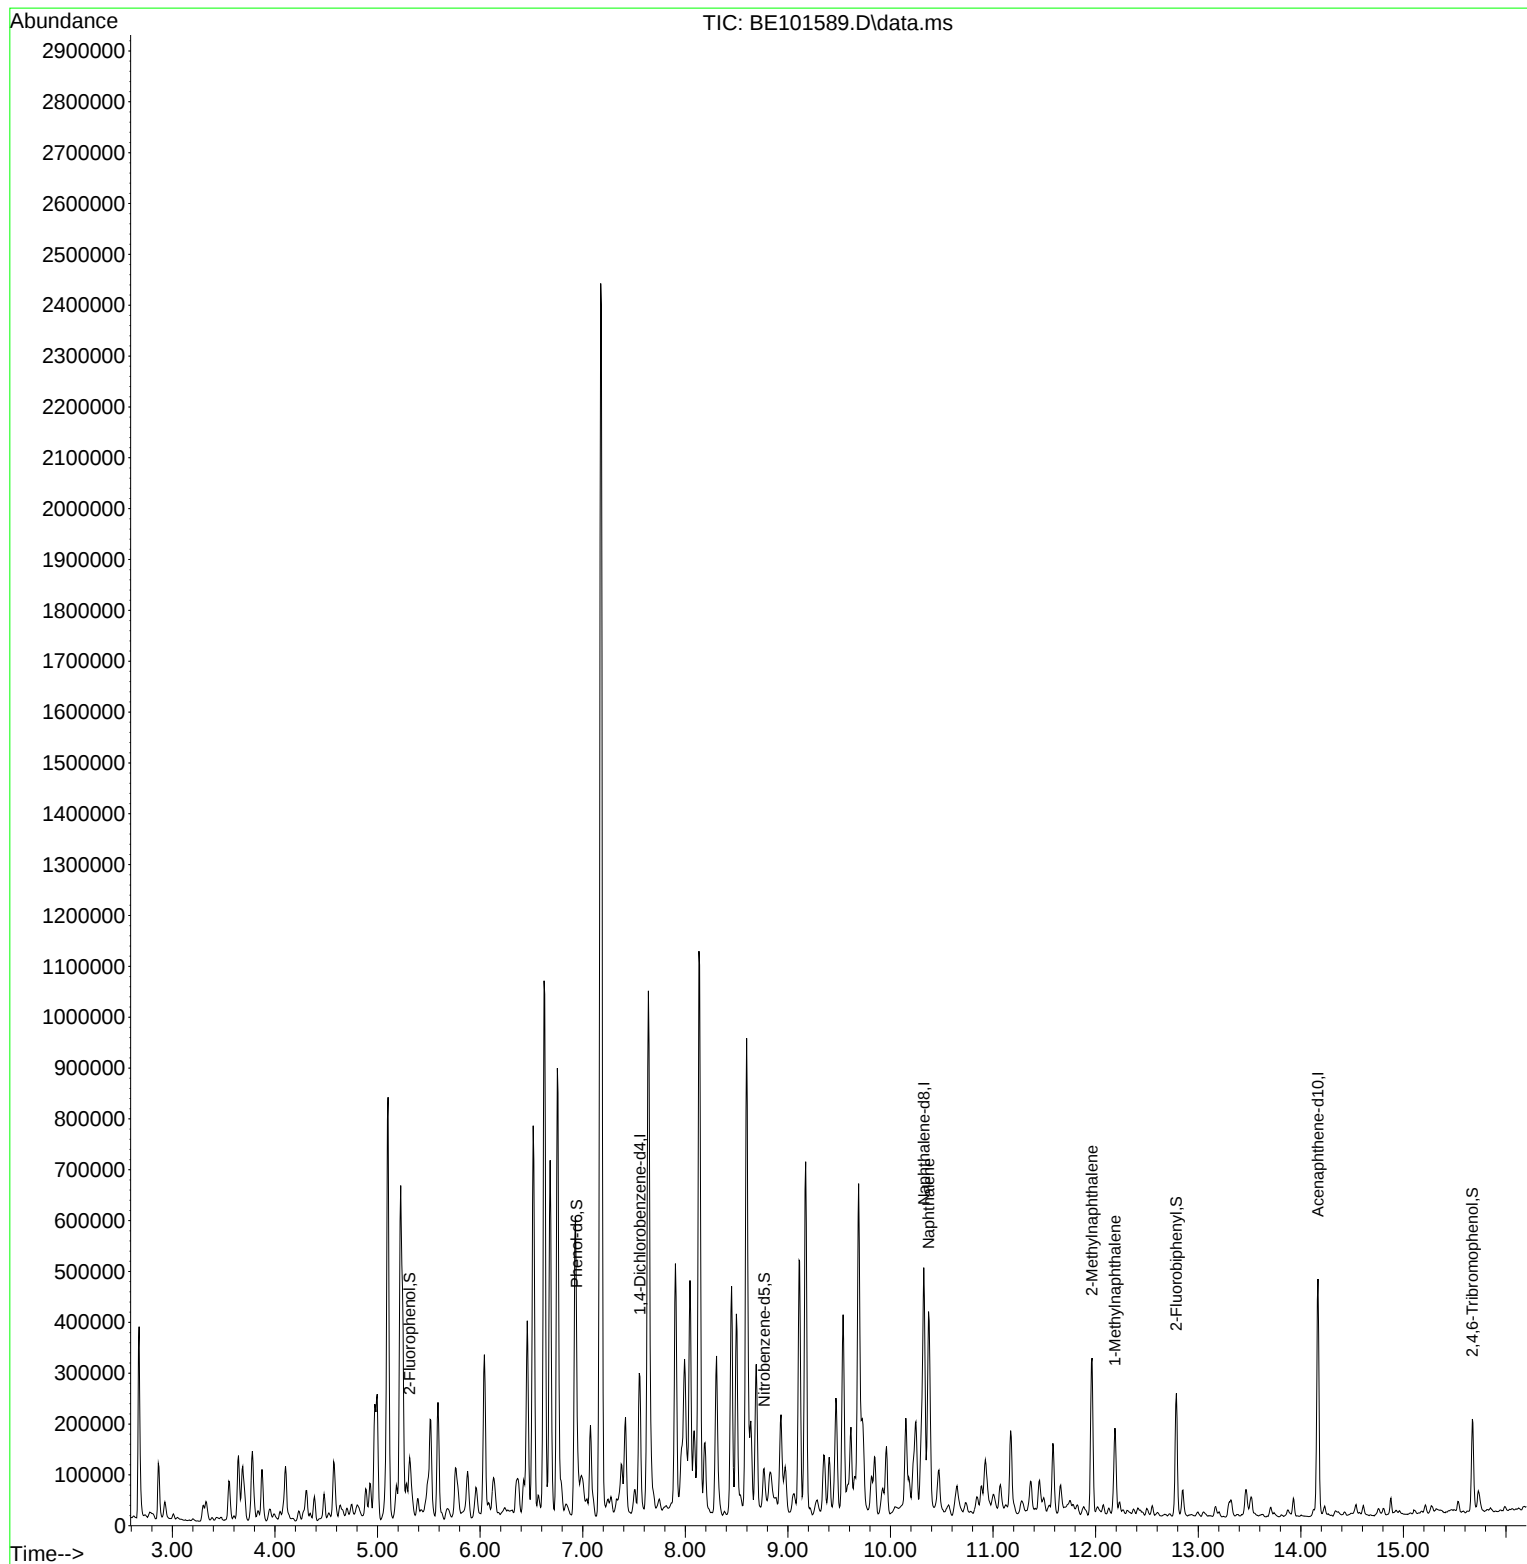

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101589.D
Acq On : 12 Nov 2024 23:25
Operator : RC/JU
Sample : P4739-09DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-B2DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/13/2024

Quant Time: Nov 13 00:19:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

