
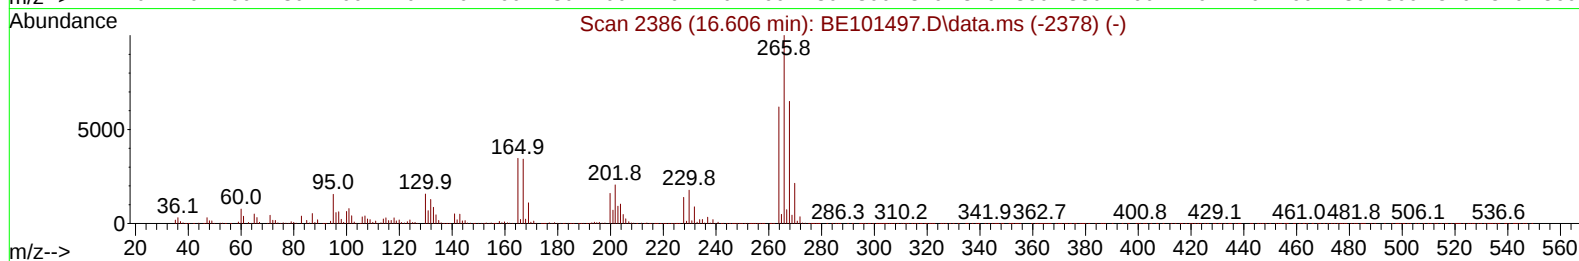
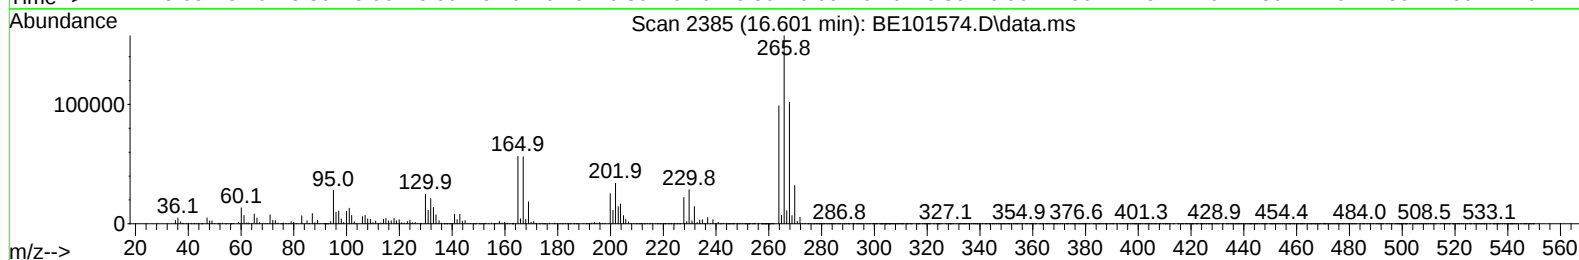


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101574.D
Acq On : 12 Nov 2024 9:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 11:49:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

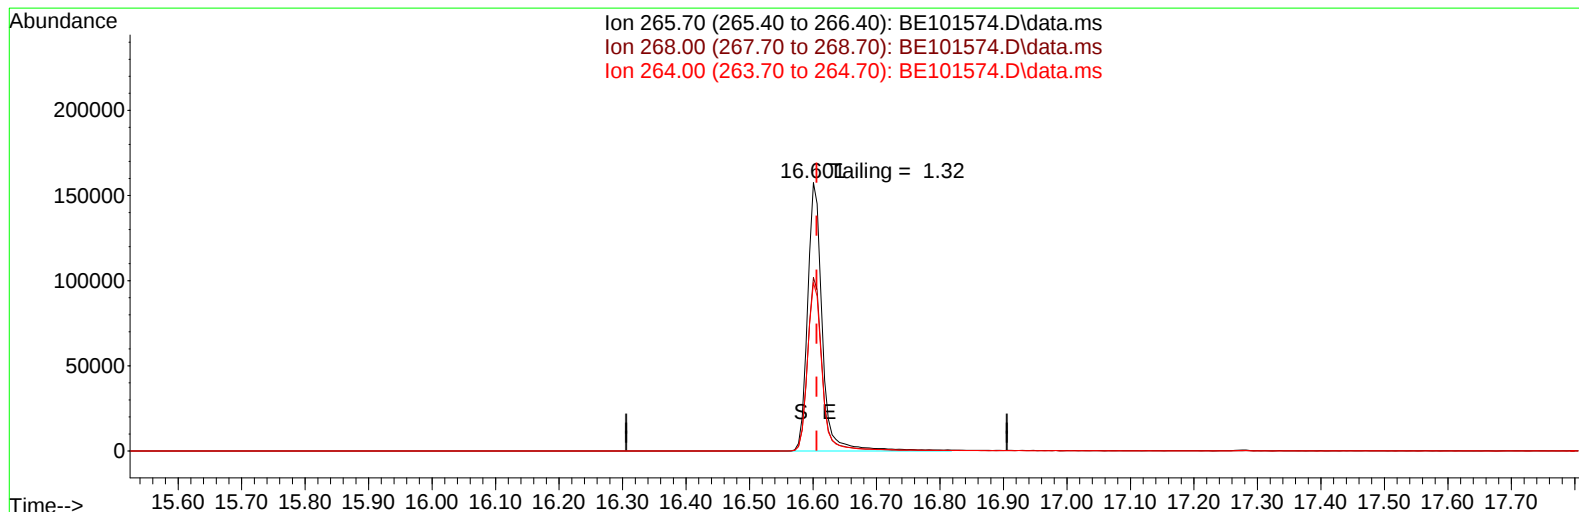

TIC: BE101574.D\data.ms

(70) Pentachlorophenol (C)




16.601min (-0.005) 60825.00 ng

response 252938

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	64.63
264.00	62.00	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111224\
Data File : BE101574.D
Acq On : 12 Nov 2024 9:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 11:49:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

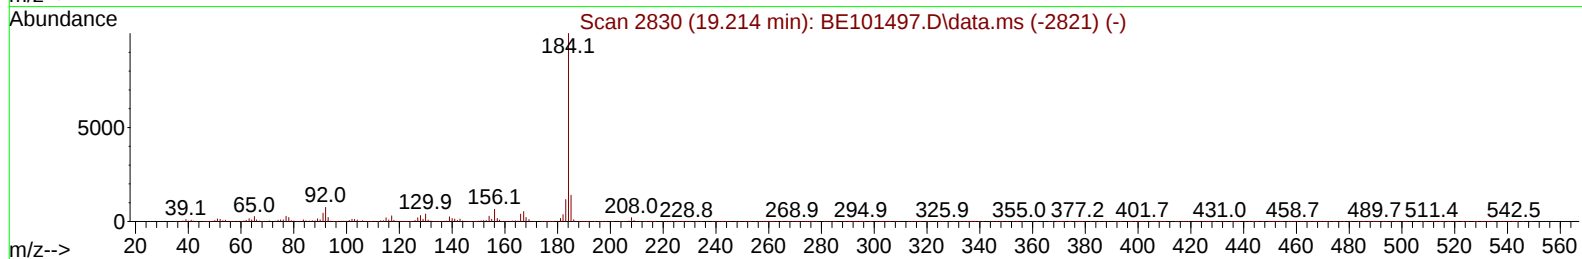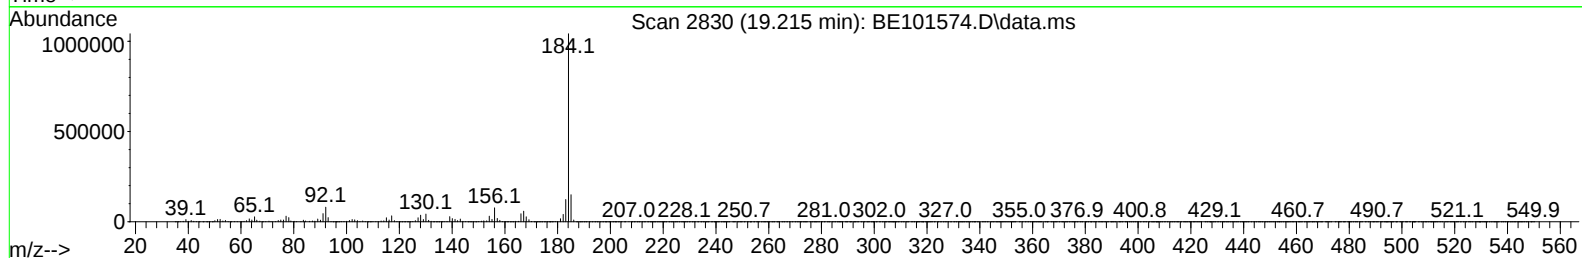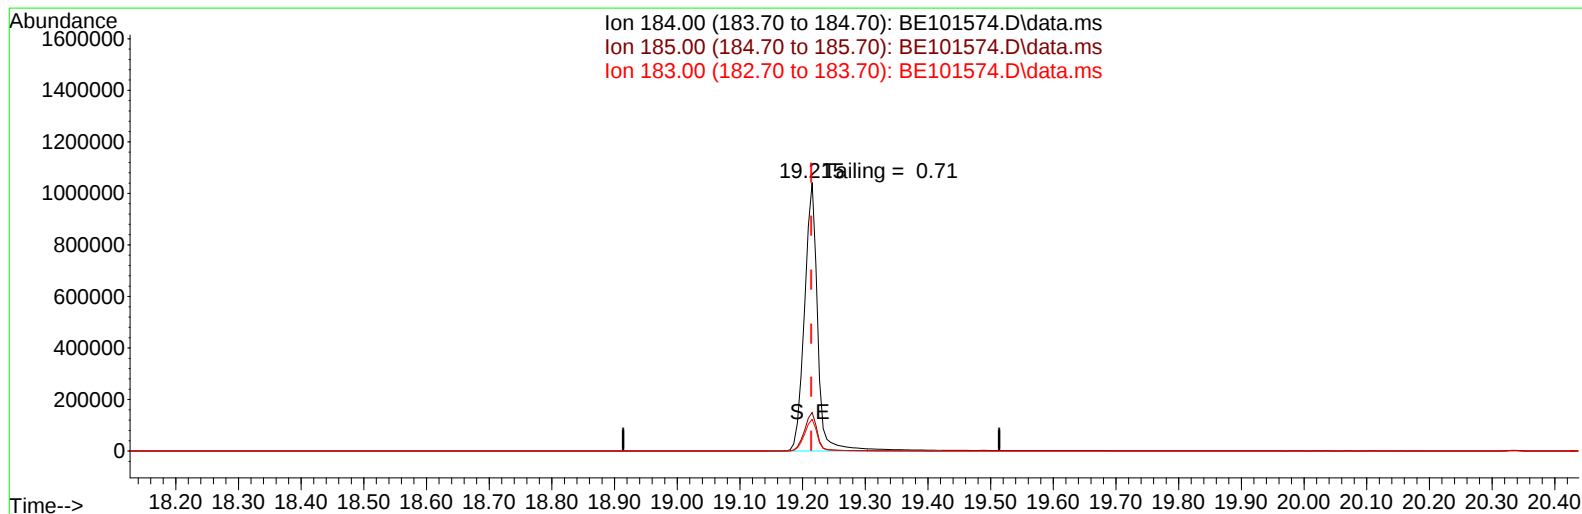

TIC: BE101574.D\data.ms

(77) Benzidine**19.215min (+ 0.001) 5484.13 ng****response 1525802**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.36
183.00	11.70	11.81
0.00	0.00	0.00