

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111315\
 Data File : BE091152.D
 Acq On : 13 Nov 2015 21:57
 Operator : UM/NP
 Sample : PB86557BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK57

Quant Time: Nov 14 02:52:50 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 14 02:47:44 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	5682	0.40	ng/ul	-0.08
4) Naphthalene-d8	9.57	136	27901	0.40	ng/ul	-0.04
8) Acenaphthene-d10	13.39	164	16941	0.40	ng/ul	-0.01
12) Phenanthrene-d10	16.19	188	2481396	0.40	ng/ul	0.07
18) Chrysene-d12	20.26	240	53925	0.40	ng/ul	0.00
22) Perylene-d12	22.01	264	3269693	0.40	ng/ul	-0.13
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.05	96	45018	11.01	ng/uL	-0.10
6) 2-Methylnaphthalene-d10	11.12	152	11617	0.31	ng/ul	0.00
16) Fluoranthene-d10	18.09	212	32416	0.00	ng/ul	0.00
Target Compounds						
					Qvalue	
11) Fluorene	14.36	166	4487	0.06	ng/ul#	9
19) Pyrene	18.47	202	19138	0.03	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111315\
Data File : BE091152.D
Acq On : 13 Nov 2015 21:57
Operator : UM/NP
Sample : PB86557BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK57

Quant Time: Nov 14 02:52:50 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 14 02:47:44 2015
Response via : Initial Calibration

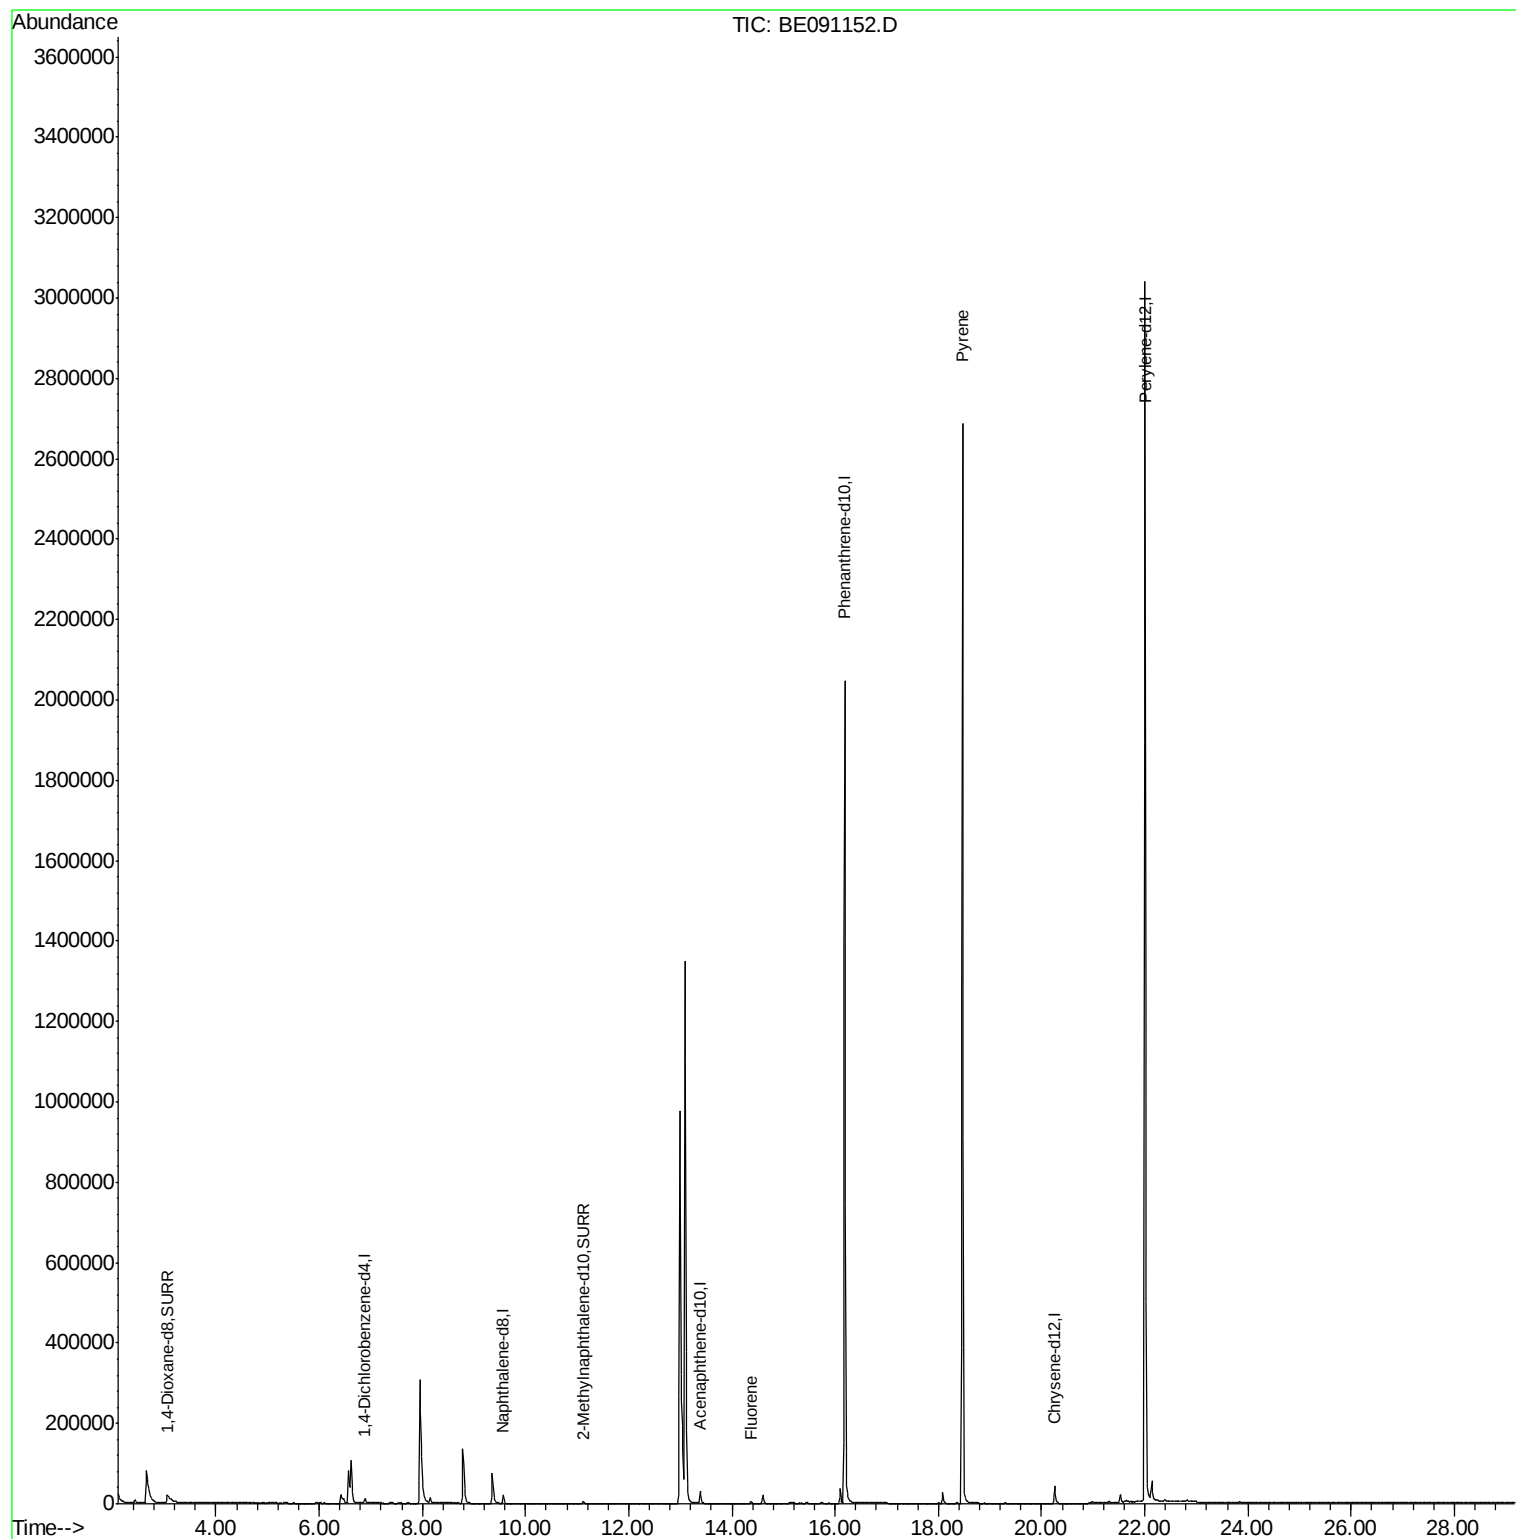

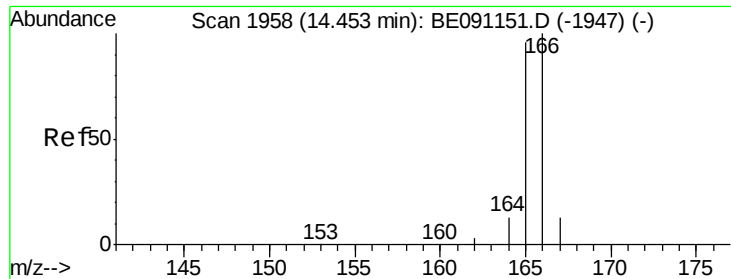

#11

Fluorene

Concen: 0.06 ng/ul

RT: 14.36 min Scan# 1946

Delta R.T. -0.09 min

Lab File: BE091152.D

Acq: 13 Nov 2015 21:57

Instrument :

BNA_E

ClientSampleId :

SBLK57





Tgt Ion:166 Resp: 4487

Ion Ratio Lower Upper

166 100

165 7.7 87.6 131.4#

167 33.9 11.1 16.7#

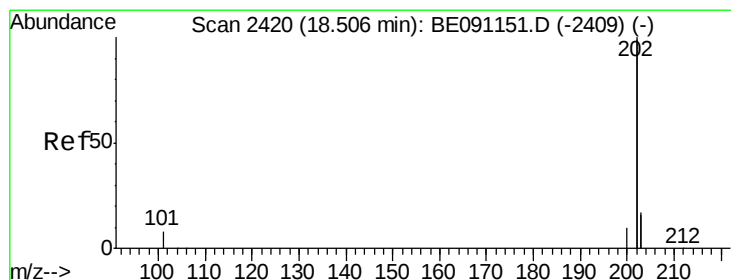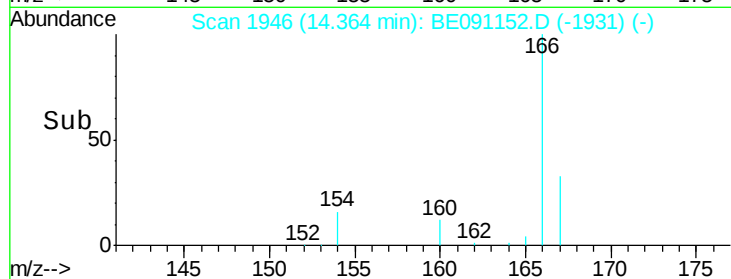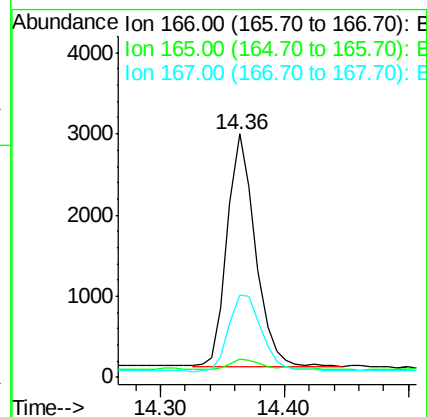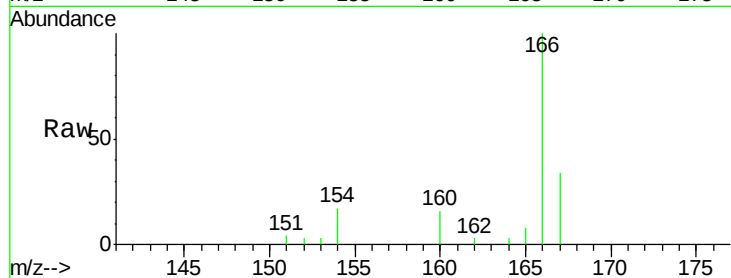

#19

Pyrene

Concen: 0.03 ng/ul

RT: 18.47 min Scan# 2414

Delta R.T. -0.04 min

Lab File: BE091152.D

Acq: 13 Nov 2015 21:57

Tgt Ion:202 Resp: 19138

Ion Ratio Lower Upper

202 100

200 1.4 18.0 27.0#

203 182.5 13.8 20.6#

