

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111315\
 Data File : BE091162.D
 Acq On : 14 Nov 2015 3:58
 Operator : UM/NP
 Sample : G4342-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 D9KR0

Quant Time: Nov 14 05:47:55 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 14 03:28:24 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	3736	0.40	ng/ul	-0.07
4) Naphthalene-d8	9.56	136	18178	0.40	ng/ul	-0.05
8) Acenaphthene-d10	13.38	164	11420	0.40	ng/ul	-0.02
12) Phenanthrene-d10	16.18	188	1185782	0.40	ng/ul	0.07
18) Chrysene-d12	20.24	240	45694	0.40	ng/ul	0.00
22) Perylene-d12	22.13	264	55217	0.40	ng/ul	-0.01
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.07	96	17810	6.63	ng/uL	-0.09
6) 2-Methylnaphthalene-d10	11.09	152	4979	0.20	ng/ul	-0.03
16) Fluoranthene-d10	18.08	212	14958	0.00	ng/ul	-0.01
Target Compounds						
25) Benzo(a)pyrene	22.00	252	7375	0.05	ng/ul#	Ovalue 24




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111315\
Data File : BE091162.D
Acq On : 14 Nov 2015 3:58
Operator : UM/NP
Sample : G4342-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
D9KR0

Quant Time: Nov 14 05:47:55 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 14 03:28:24 2015
Response via : Initial Calibration

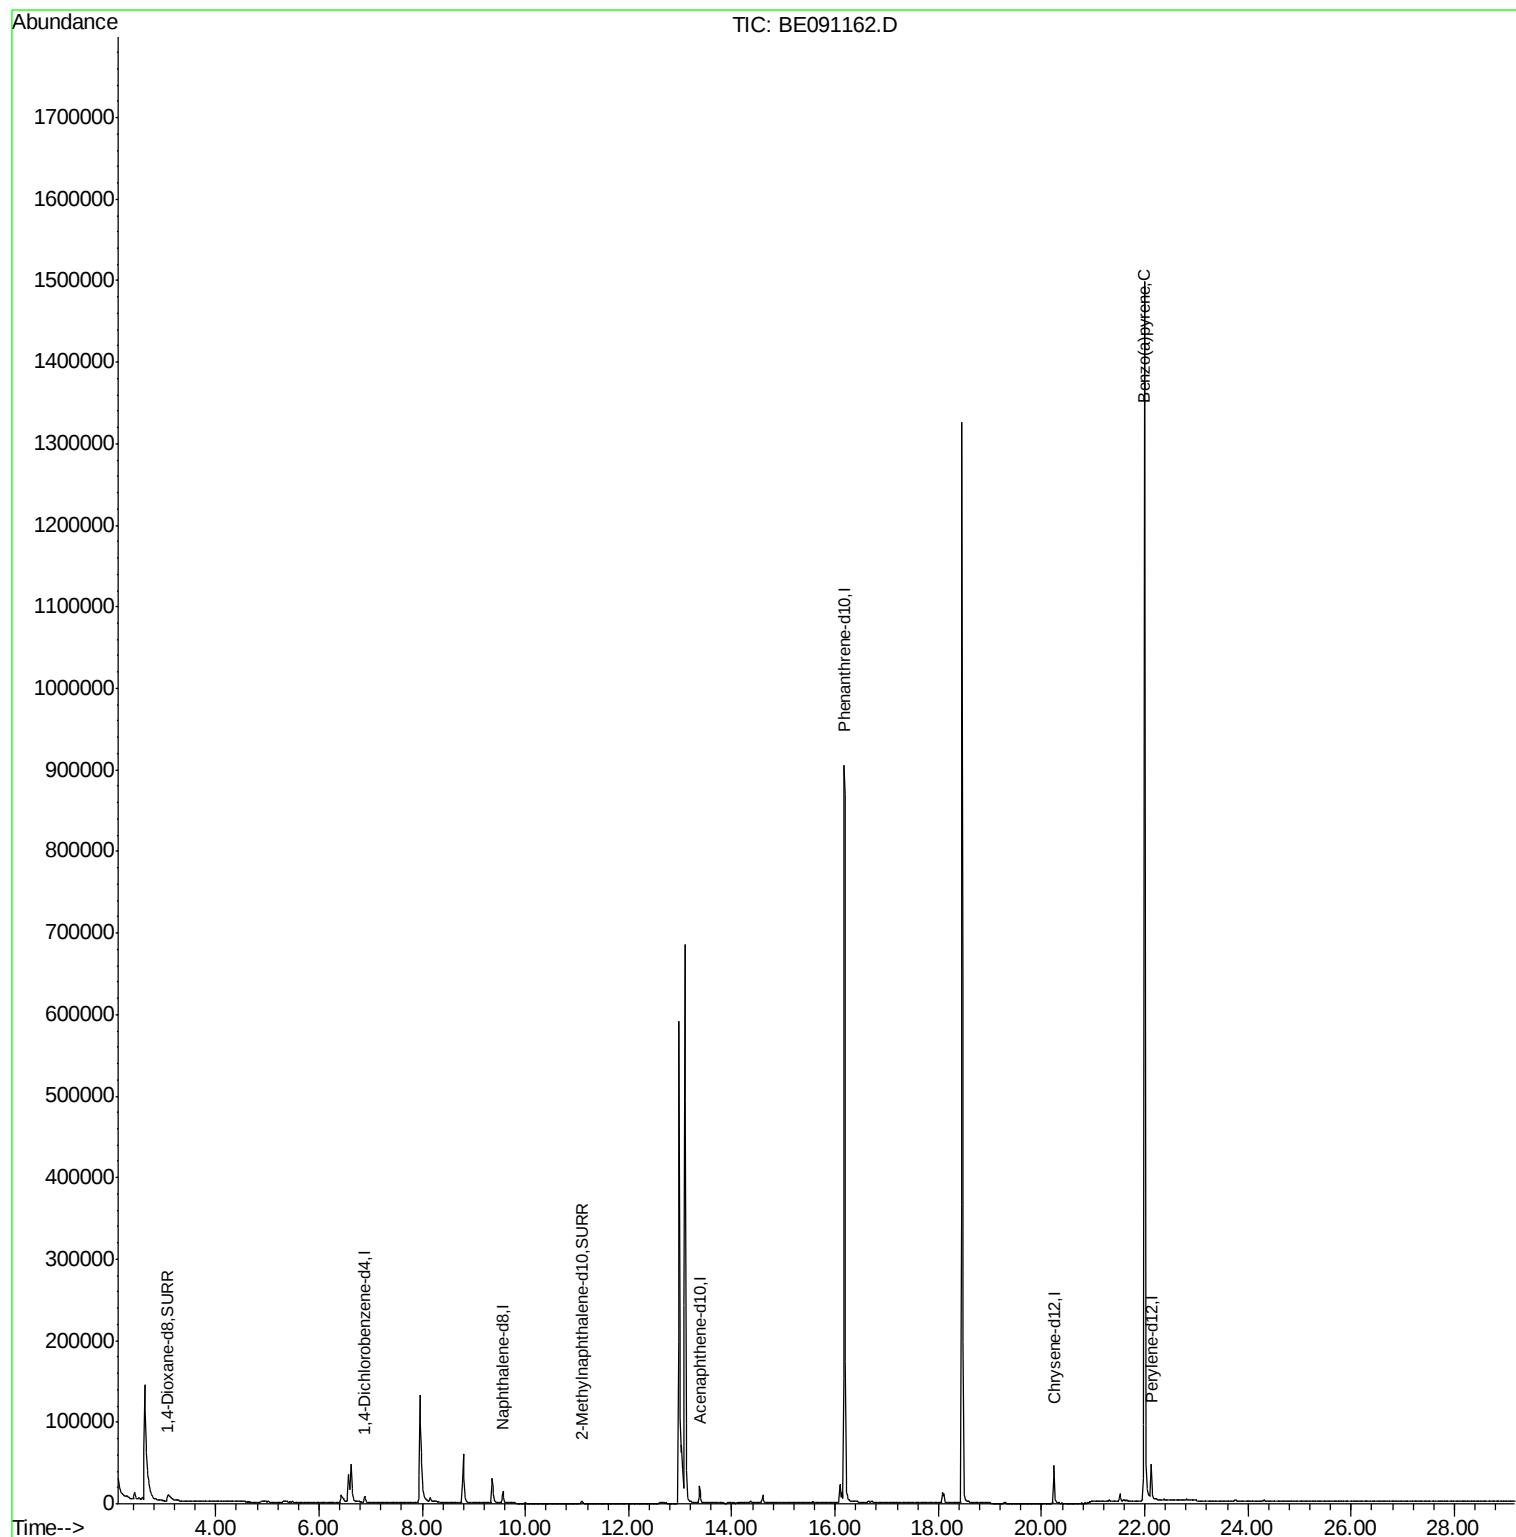

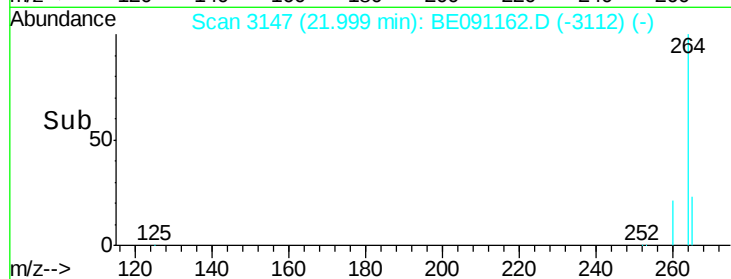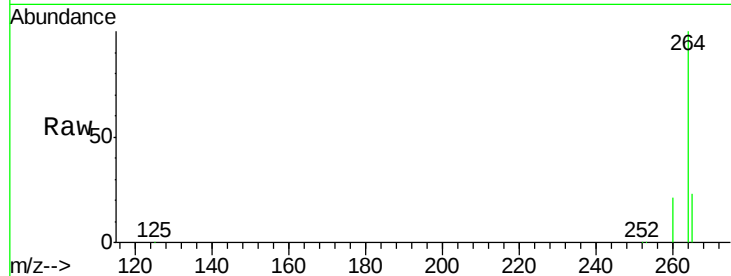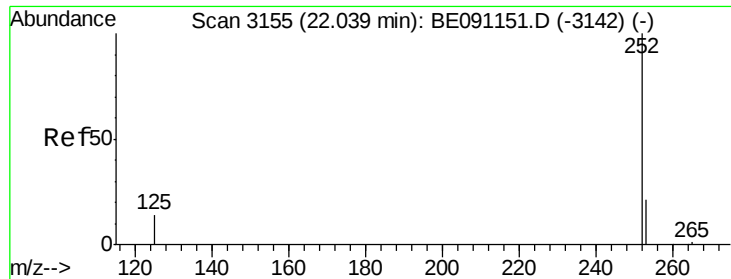

#25

Benzo(a)pyrene

Concen: 0.05 ng/ul

RT: 22.00 min Scan# 3147

Delta R.T. -0.04 min

Lab File: BE091162.D

Acq: 14 Nov 2015 3:58

Instrument :

BNA_E

ClientSampleId :

D9KR0

Tot Ion: 252 Resp: 7375

Ion Ratio Lower Upper

252 100

253 54.7 21.8 32.8#

125 67.5 14.5 21.7#

