


Data Path : Z:\HPCHEM1\BNA_E\Data\BE111315\
Data File : BE091160.D
Acq On : 14 Nov 2015 2:47
Operator : UM/NP
Sample : G4342-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
D9KQ6

Quant Time: Nov 16 11:04:01 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 14 03:28:24 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

mmdadoda
11/16/2015 3:25:08 PM

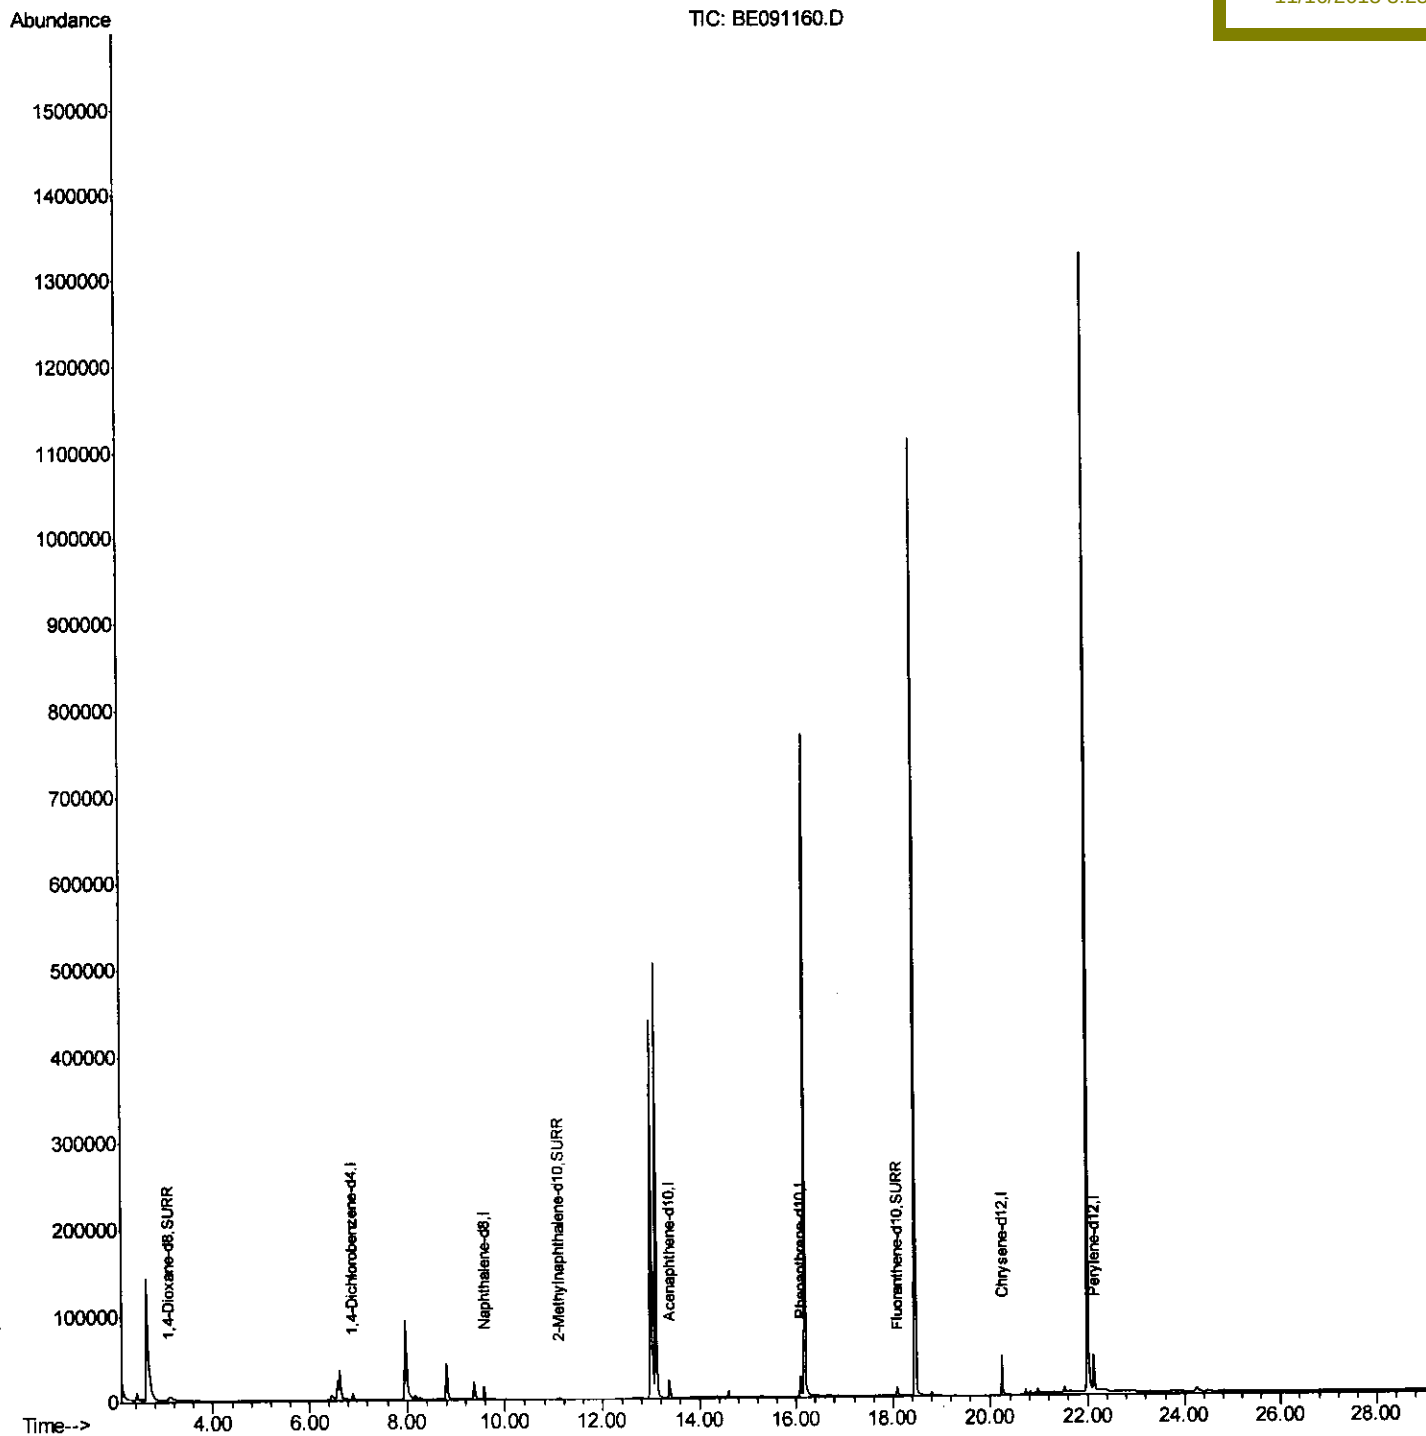

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE111315\
 Data File : BE091160.D
 Acq On : 14 Nov 2015 2:47
 Operator : UM/NP
 Sample : G4342-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 D9KQ6

Quant Time: Nov 14 05:57:39 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 14 03:28:24 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mmdadoda
 11/16/2015 3:25:08 PM

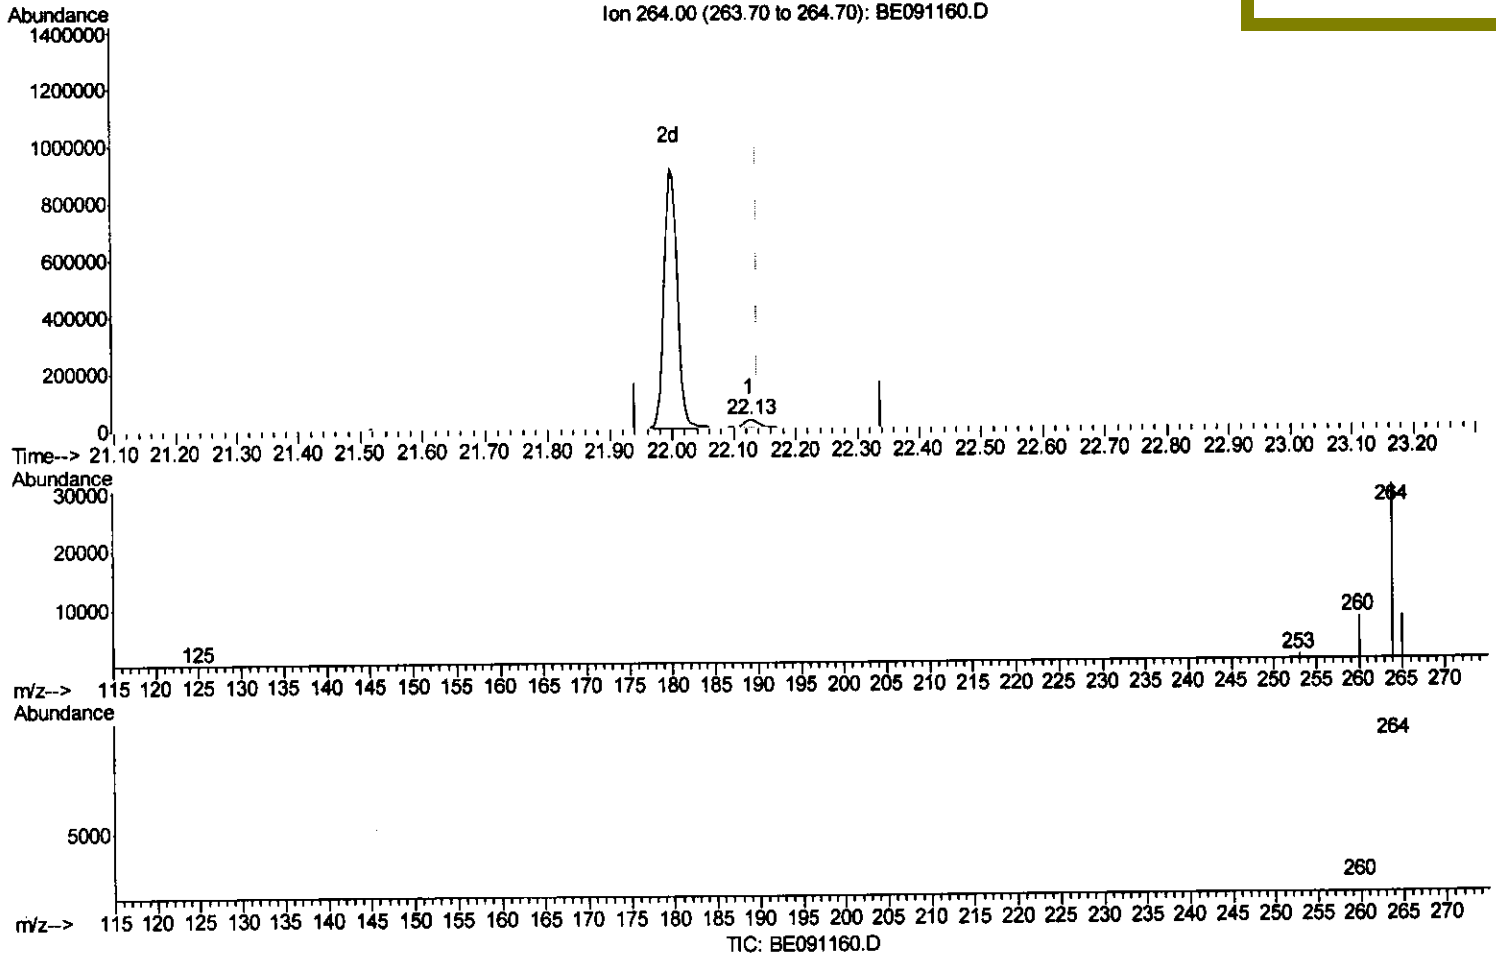

(22) Perylene-d12 (I)

22.125min (-0.014) 0.40ng/ul

response 56435

Ion	Exp%	Act%
264.00	100	100
260.00	28.90	25.22
265.00	34.70	26.27#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE111315\
 Data File : BE091160.D
 Acq On : 14 Nov 2015 2:47
 Operator : UM/NP
 Sample : G4342-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 D9KQ6

Manual Integrations
 APPROVED

mmdadoda
 11/16/2015 3:25:08 PM

Quant Time: Nov 14 05:57:39 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 14 03:28:24 2015
 Response via : Initial Calibration

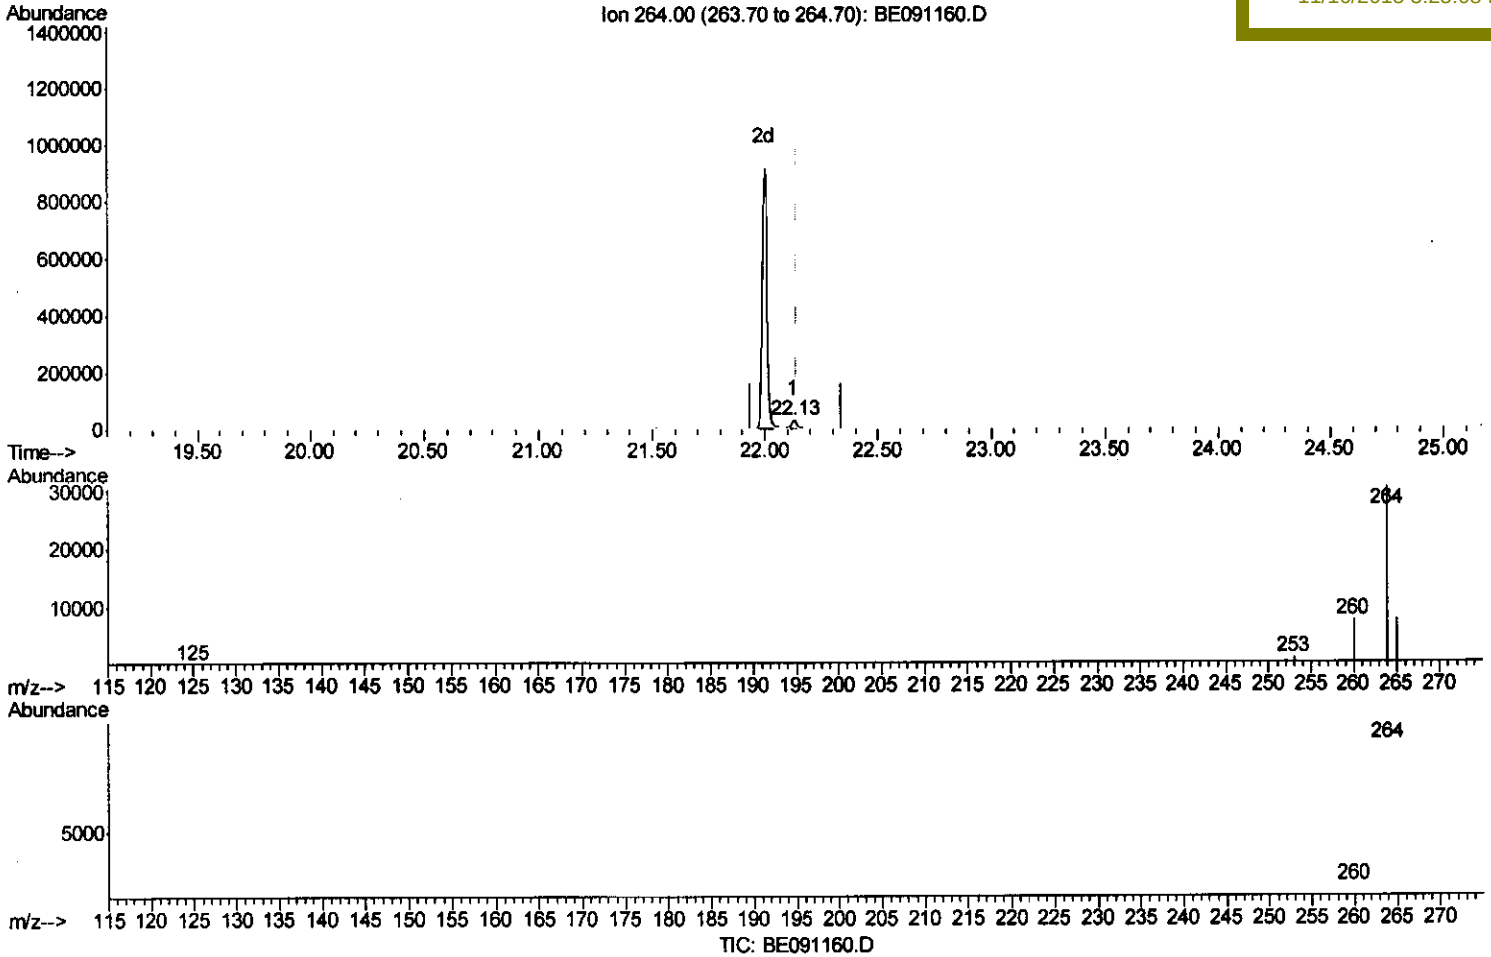

(22) Perylene-d12 (I)

22.125min (-0.014) 0.40ng/ul m

response 42455

Ion	Exp%	Act%
264.00	100	100
260.00	28.90	25.22
265.00	34.70	26.27#
0.00	0.00	0.00

U M
 11/17/15

Data Path : Z:\HPCHEM1\BNA_E\Data\BE111315\
Data File : BE091160.D
Acq On : 14 Nov 2015 2:47
Operator : UM/NP
Sample : G4342-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
D9KQ6

Quant Time: Nov 16 11:04:01 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 14 03:28:24 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

mmdadoda
11/16/2015 3:25:08 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	4380	0.40	ng/ul	-0.07
4) Naphthalene-d8	9.57	136	21175	0.40	ng/ul	-0.04
8) Acenaphthene-d10	13.38	164	12750	0.40	ng/ul	-0.02
12) Phenanthrene-d10	16.10	188	31397	0.40	ng/ul	-0.01
18) Chrysene-d12	20.24	240	47763	0.40	ng/ul	0.00
22) Perylene-d12	22.13	264	42455m	0.40	ng/ul	-0.01

Sum
11/17/15

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.09	96	13160	4.18	ng/uL	-0.06
6) 2-Methylnaphthalene-d10	11.10	152	3551	0.12	ng/ul	-0.02
16) Fluoranthene-d10	18.08	212	12428	0.14	ng/ul	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed