

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111315\
 Data File : BE091162.D
 Acq On : 14 Nov 2015 3:58
 Operator : UM/NP
 Sample : G4342-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 D9KR0

Manual Integrations
 APPROVED

mmdadoda
 11/16/2015 3:25:17 PM

Quant Time: Nov 16 11:09:52 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 14 03:28:24 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	3736	0.40	ng/ul	-0.07
4) Naphthalene-d8	9.56	136	18178	0.40	ng/ul	-0.05
8) Acenaphthene-d10	13.38	164	11420	0.40	ng/ul	-0.02
12) Phenanthrene-d10	16.10	188	28813m	0.40	ng/ul	-0.01
18) Chrysene-d12	20.24	240	45694	0.40	ng/ul	0.00
22) Perylene-d12	22.13	264	39931m	0.40	ng/ul	-0.01
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.07	96	17810	6.63	ng/uL	-0.09
6) 2-Methylnaphthalene-d10	11.09	152	4979	0.20	ng/ul	-0.03
16) Fluoranthene-d10	18.08	212	14958	0.18	ng/ul	-0.01
Target Compounds						
14) Phenanthrene	16.12	178	13557	0.04	ng/ul	92
17) Fluoranthene	18.11	202	12094	0.03	ng/ul	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE111315\
Data File : BE091162.D
Acq On : 14 Nov 2015 3:58
Operator : UM/NP
Sample : G4342-12
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
D9KR0

Manual Integrations
APPROVED

mmdadoda
11/16/2015 3:25:17 PM

Quant Time: Nov 16 11:09:52 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 14 03:28:24 2015
Response via : Initial Calibration

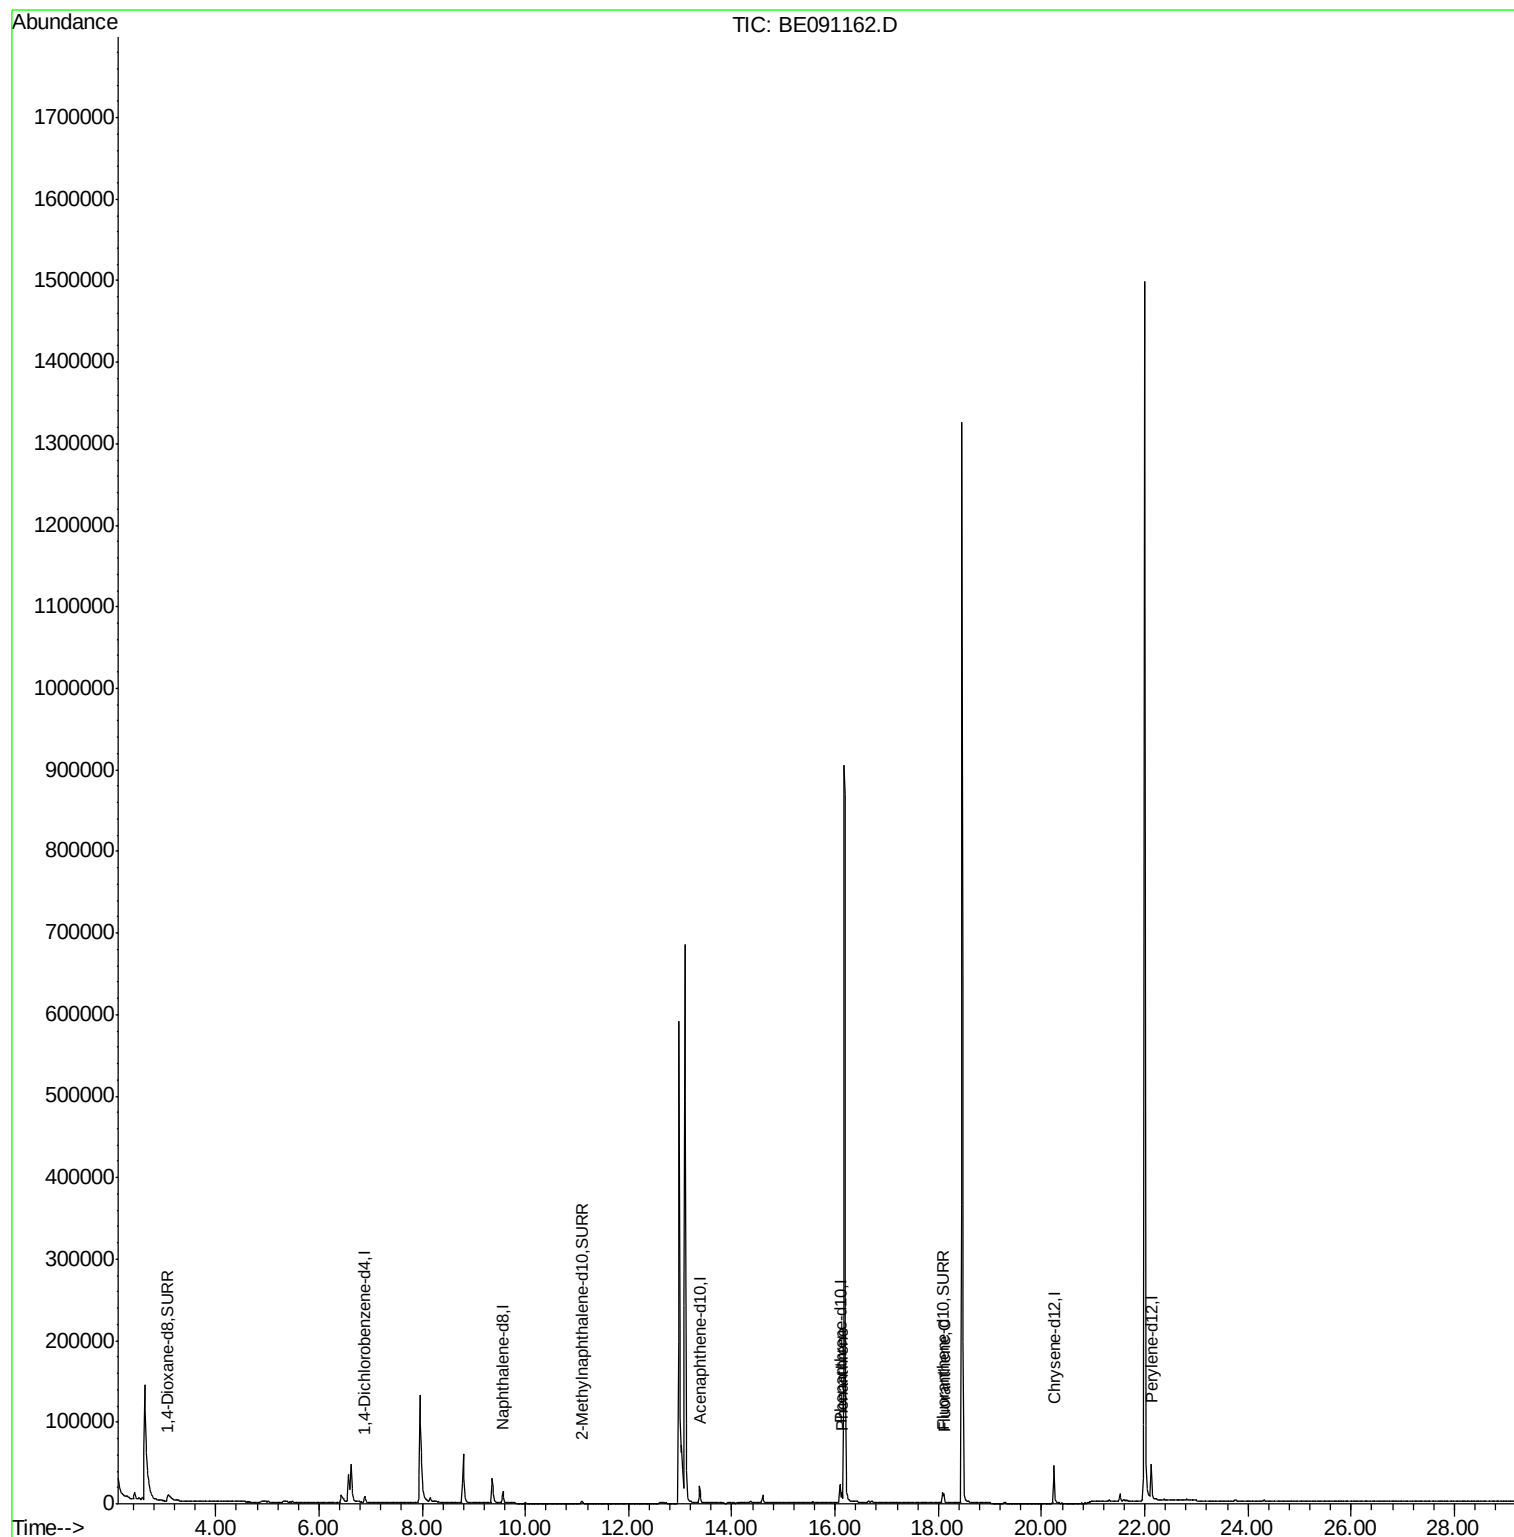

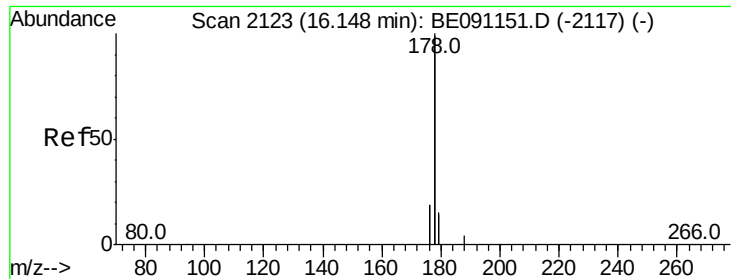





#14
Phenanthrene
Concen: 0.04 ng/ul
RT: 16.12 min Scan# 2121
Delta R.T. -0.02 min
Lab File: BE091162.D
Acq: 14 Nov 2015 3:58

Instrument :
BNA_E
ClientSampleId :
D9KR0

Tot Ion	Ratio	Lower	Upper
178	100		
176	24.2	16.2	24.4
179	18.9	12.8	19.2

Manual Integrations
APPROVED

mmdadoda
11/16/2015 3:25:17 PM

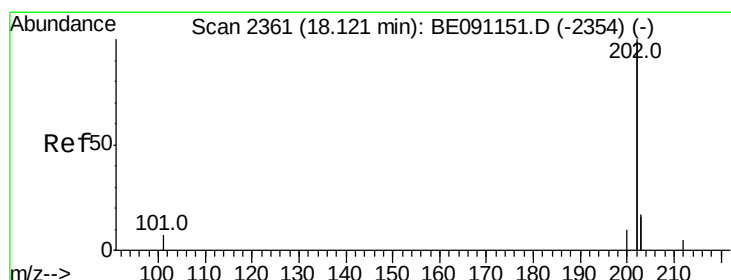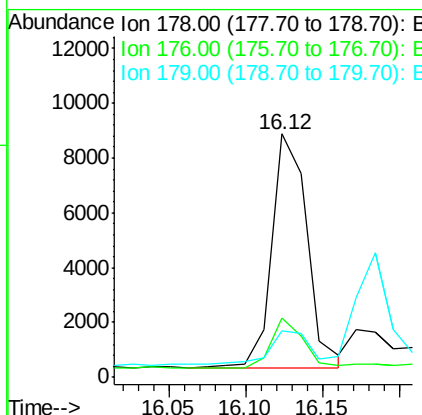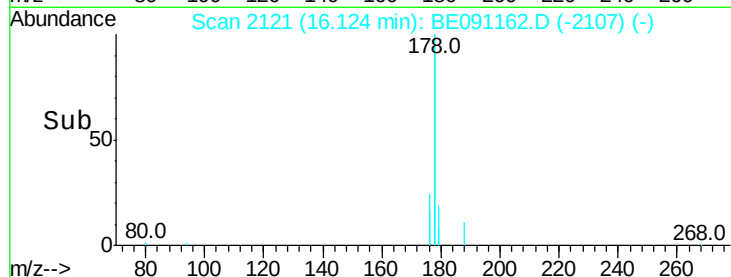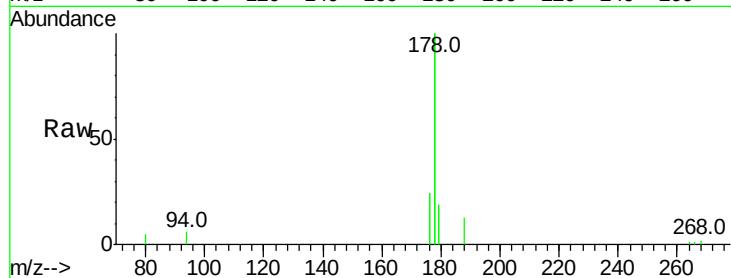

#17
Fluoranthene
Concen: 0.03 ng/ul
RT: 18.11 min Scan# 2359
Delta R.T. -0.01 min
Lab File: BE091162.D
Acq: 14 Nov 2015 3:58

Tgt Ion	Ratio	Lower	Upper
202	100		
101	4.4	0.0	33.1
203	21.7	0.0	37.2

