
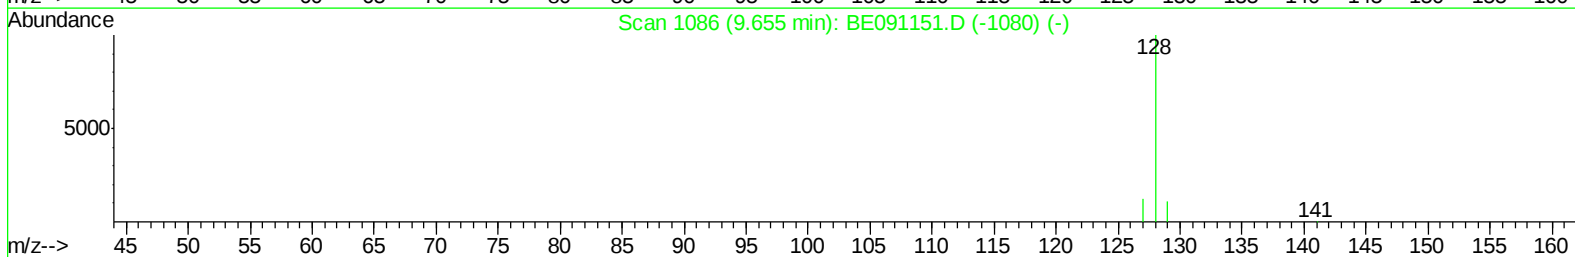
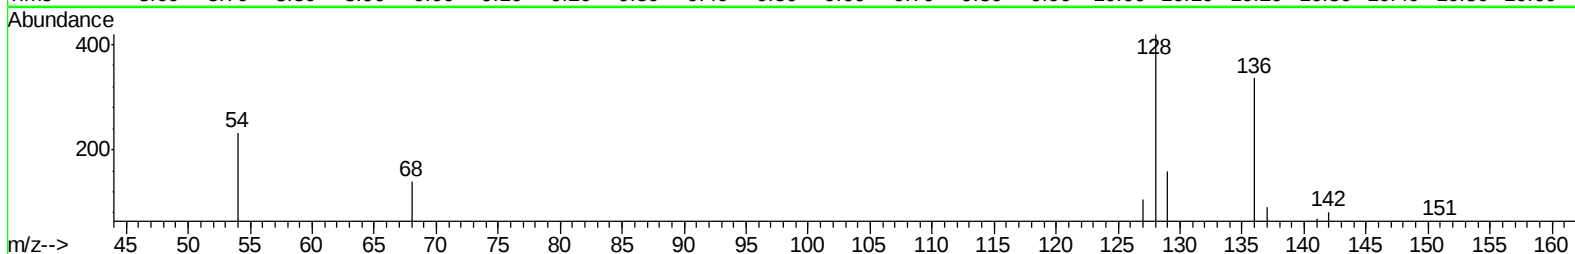


Data Path : Z:\HPCHEM1\BNA E\DATA\BE111615\
Data File : BE091177.D
Acq On : 16 Nov 2015 10:52
Operator : UM/NP
Sample : G4309-21MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 17 10:32:18 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 16 04:54:02 2015
Response via : Initial Calibration

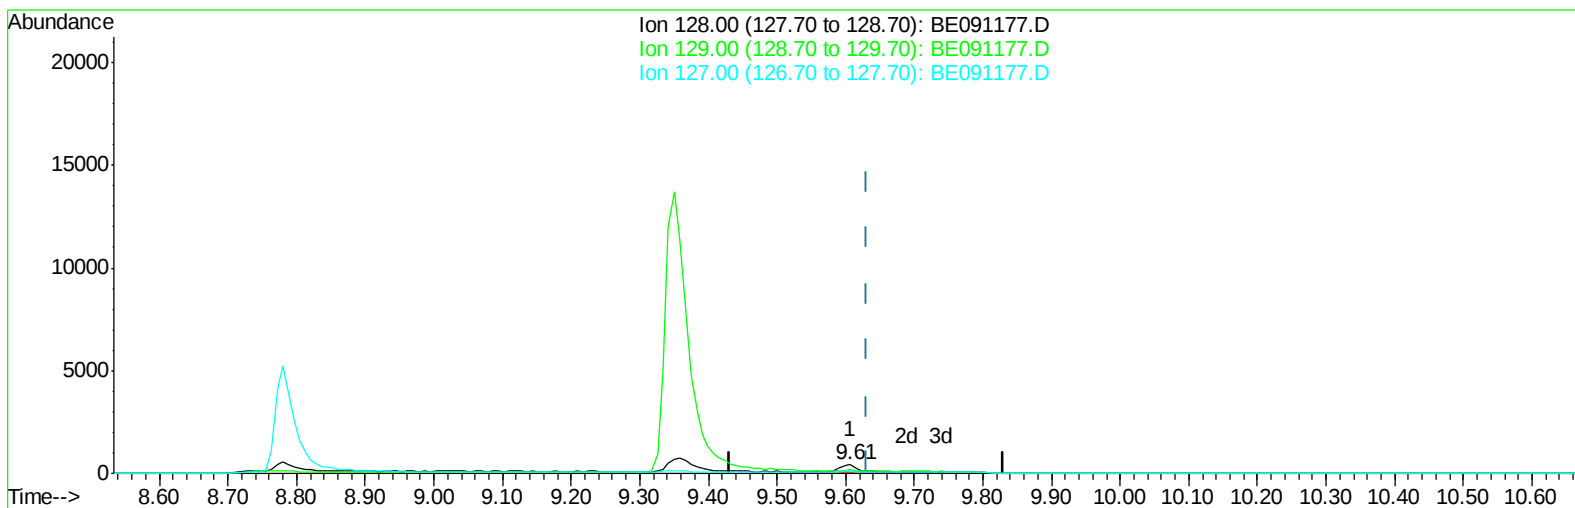

TIC: BE091177.D

(5) Naphthalene




9.606min (-0.025) 0.01ng/ul

response 597

Ion	Exp%	Act%
128.00	100	100
129.00	12.30	38.19#
127.00	13.40	25.06#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111615\
Data File : BE091177.D
Acq On : 16 Nov 2015 10:52
Operator : UM/NP
Sample : G4309-21MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 17 10:32:18 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 16 04:54:02 2015
Response via : Initial Calibration

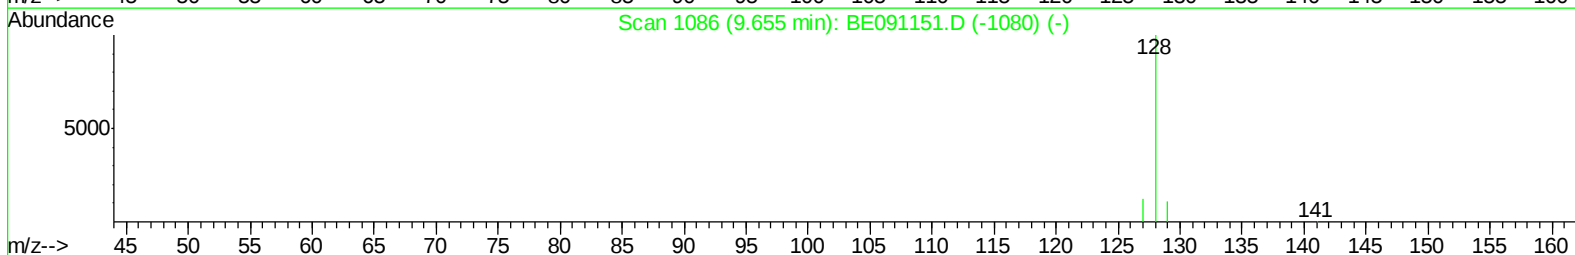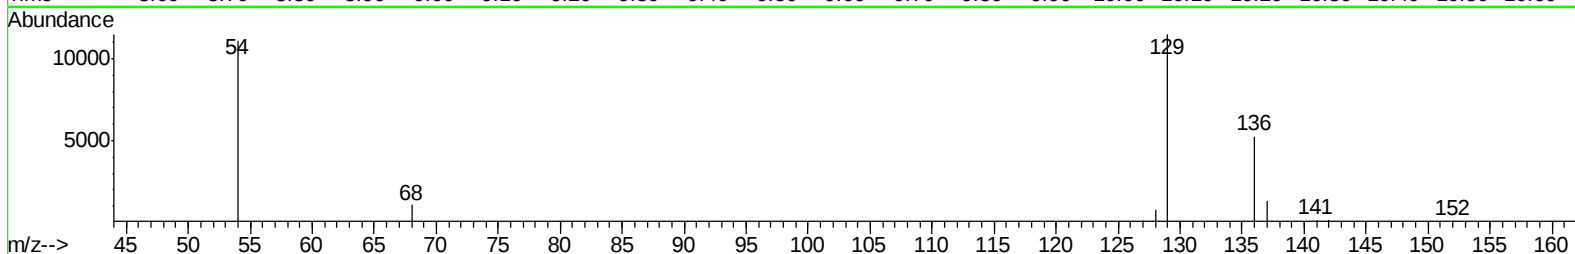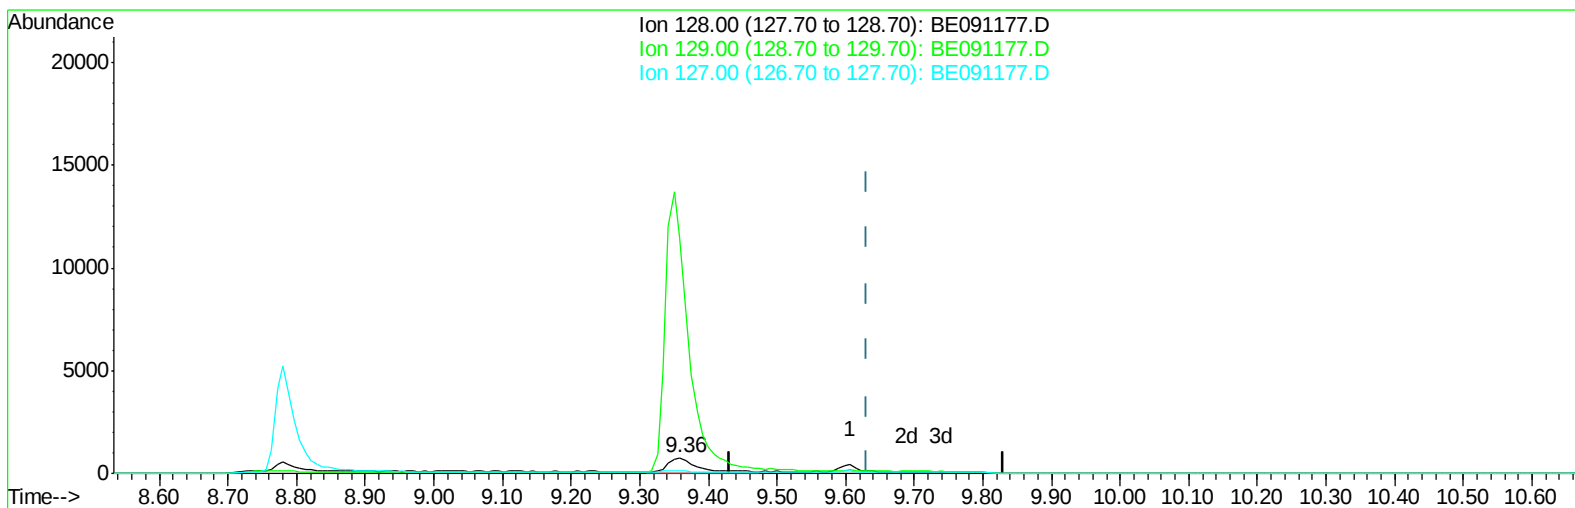

TIC: BE091177.D

(5) Naphthalene

9.358min (-0.273) 0.05ng/ul m

response 2556

Ion	Exp%	Act%
128.00	100	100
129.00	12.30	1501.05#
127.00	13.40	14.51
0.00	0.00	0.00