

Data Path : Z:\HPCHEM1\BNA_E\Data\BE111615\
Data File : BE091179.D
Acq On : 16 Nov 2015 12:04
Operator : UM/NP
Sample : PB86600BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK00

Quant Time: Nov 17 15:50:27 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Quant Update : Mon Nov 16 04:54:02 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

mmdadoda
11/17/2015 5:54:22 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	4071	0.40	ng/ul	-0.05
4) Naphthalene-d8	9.56	136	20589	0.40	ng/ul	-0.03
8) Acenaphthene-d10	13.37	164	12833	0.40	ng/ul	-0.01
12) Phenanthrene-d10	16.09	188	33309m	0.40	ng/ul	-0.01
18) Chrysene-d12	20.24	240	54177	0.40	ng/ul	0.00
22) Perylene-d12	22.12	264	59111m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.01	96	27045	9.24	ng/uL	-0.08
6) 2-Methylnaphthalene-d10	11.09	152	6755	0.24	ng/ul	0.00
16) Fluoranthene-d10	18.08	212	18749	0.20	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\Data\BE111615\
 Data File : BE091179.D
 Acq On : 16 Nov 2015 12:04
 Operator : UM/NP
 Sample : PB86600B1.
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK00

Quant Time: Nov 17 15:49:46 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 16 04:54:02 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mmdadoda
 11/17/2015 5:54:22 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	4071	0.40	ng/ul	-0.05
4) Naphthalene-d8	9.56	136	20589	0.40	ng/ul	-0.03
8) Acenaphthene-d10	13.37	164	12833	0.40	ng/ul	-0.01
12) Phenanthrene-d10	16.09	188	33309m	0.40	ng/ul	-0.01
18) Chrysene-d12	20.24	240	54177	0.40	ng/ul	0.00
22) Perylene-d12	22.12	264	59111m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.01	96	27045	9.24	ng/uL	-0.08
6) 2-Methylnaphthalene-d10	11.09	152	6755	0.24	ng/ul	0.00
16) Fluoranthene-d10	18.08	212	18749	0.20	ng/ul	0.00
Target Compounds						
3) 1,4-Dioxane	3.12	88	119	0.04	ng/ul#	29
11) Fluorene	14.36	166	2924	0.05	ng/ul#	9

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U21
 11/17/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE111615\
 Data File : BE091179.D
 Acq On : 16 Nov 2015 12:04
 Operator : UM/NP
 Sample : PB86600BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK00

Quant Time: Nov 17 15:49:08 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Mon Nov 16 04:54:02 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mmdadoda
 11/17/2015 5:54:22 PM

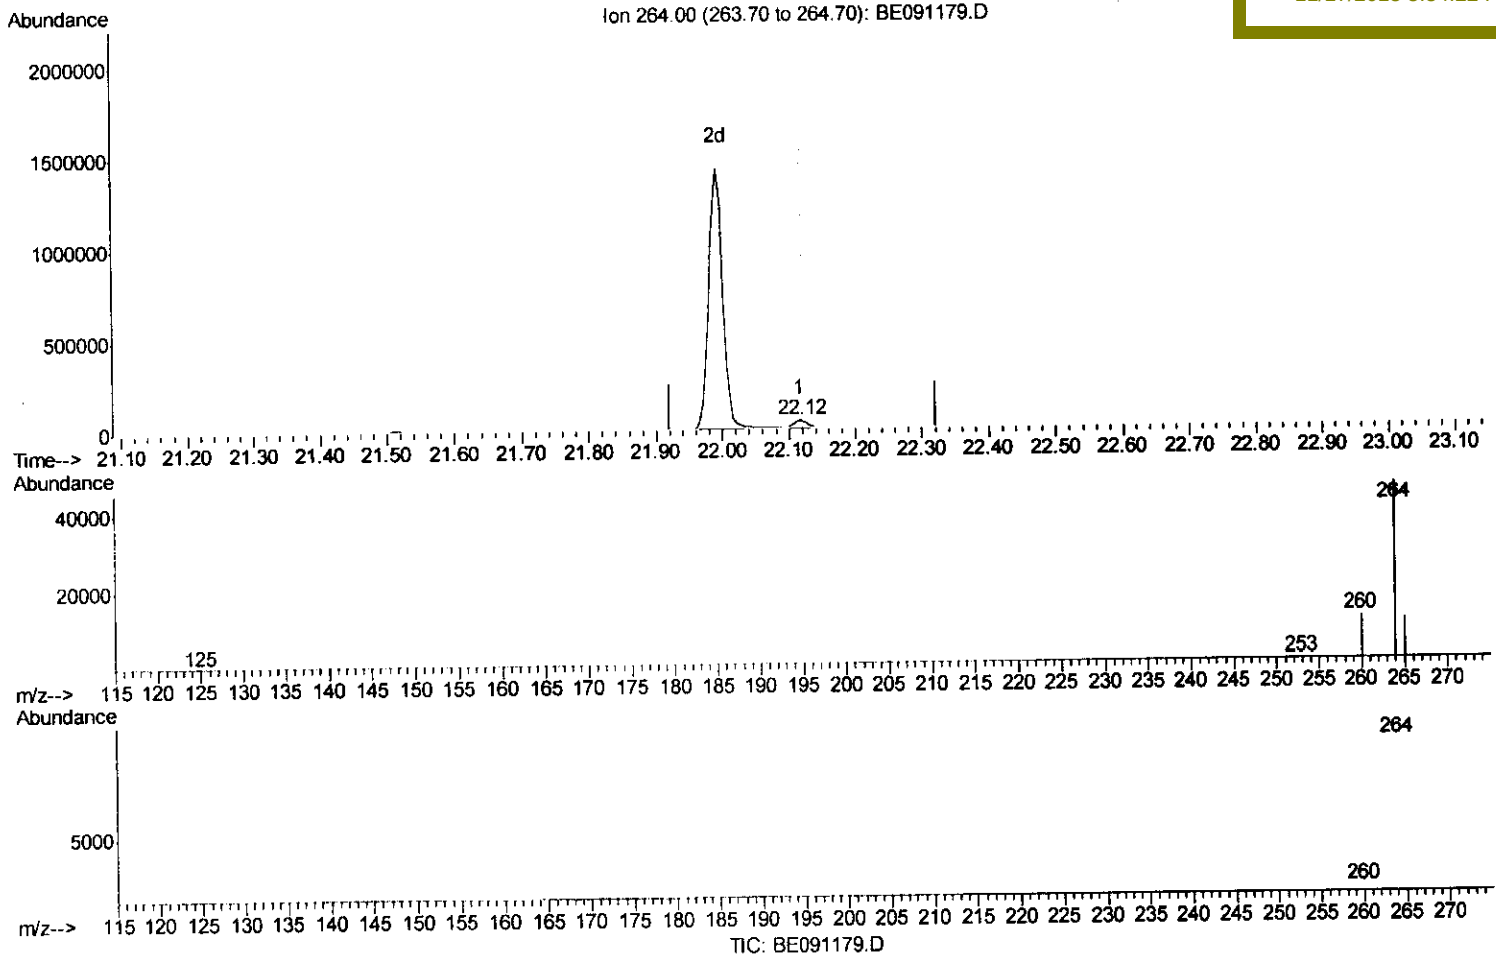

(22) Perylene-d12 (I)

22.116min (-0.006) 0.40ng/ul m

response 59111

Ion	Exp%	Act%
264.00	100	100
260.00	28.90	24.77
265.00	34.70	23.22#
0.00	0.00	0.00

U.m
 11 112 115

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE111615\
 Data File : BE091179.D
 Acq On : 16 Nov 2015 12:04
 Operator : UM/NP
 Sample : PB86600BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK00

Quant Time: Nov 17 15:48:00 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Mon Nov 16 04:54:02 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mmdadoda
 11/17/2015 5:54:22 PM

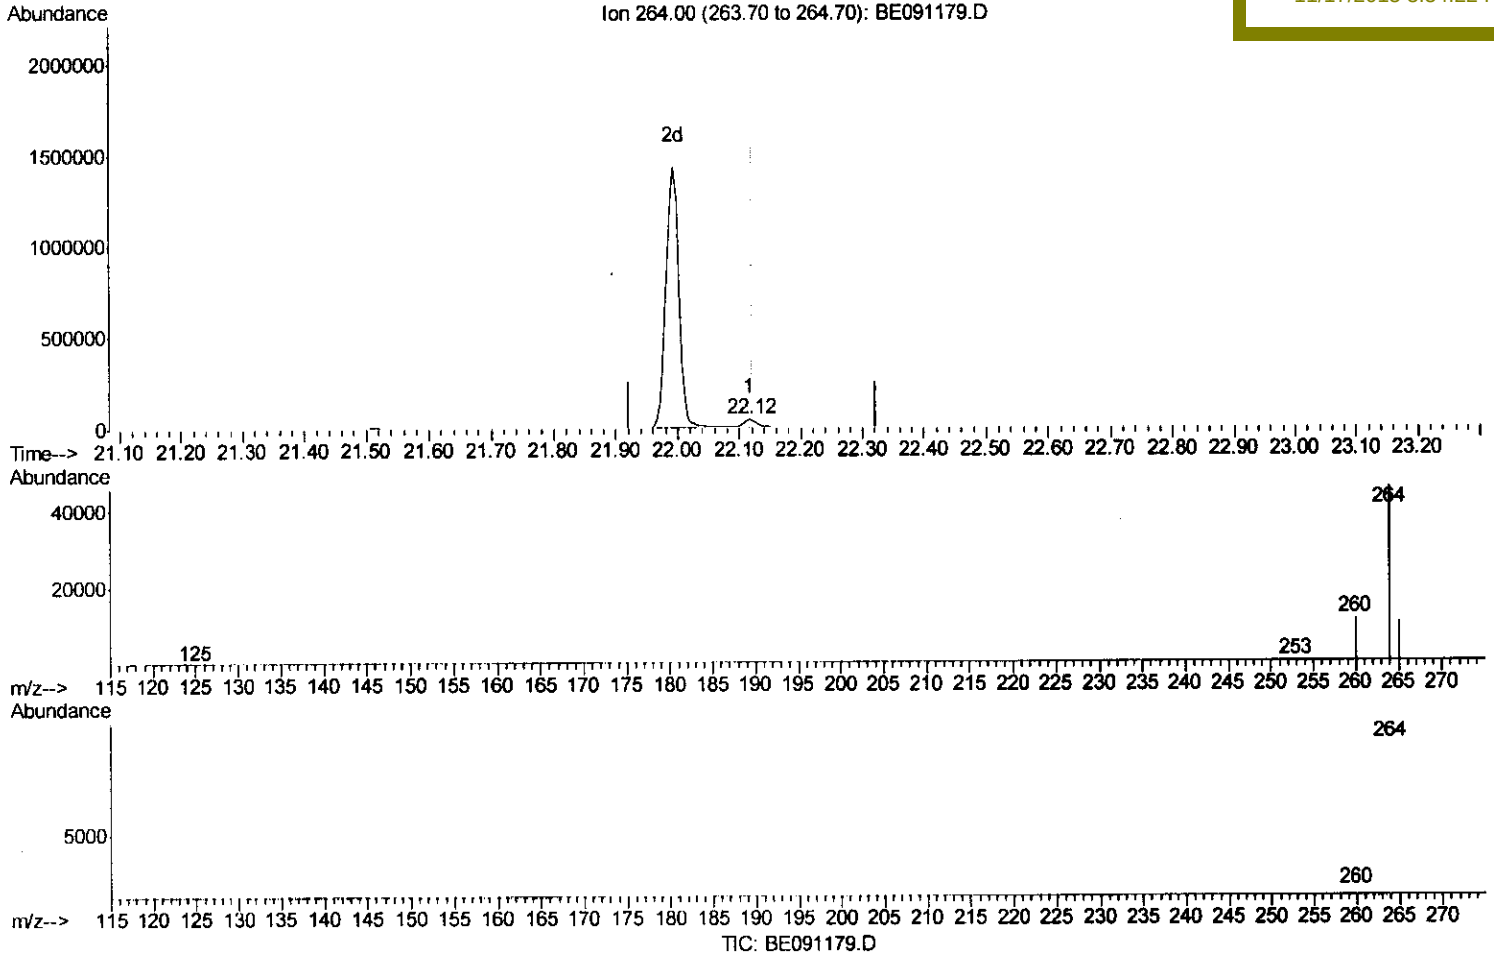

(22) Perylene-d12 (I)

22.116min (-0.006) 0.40ng/ul

response 81023

Ion	Exp%	Act%
264.00	100	100
260.00	28.90	24.77
265.00	34.70	23.22#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE111615\
 Data File : BE091179.D
 Acq On : 16 Nov 2015 12:04
 Operator : UM/NP
 Sample : PB86600BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK00

Quant Time: Nov 17 10:32:26 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 16 04:54:02 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mmdadoda
 11/17/2015 5:54:22 PM

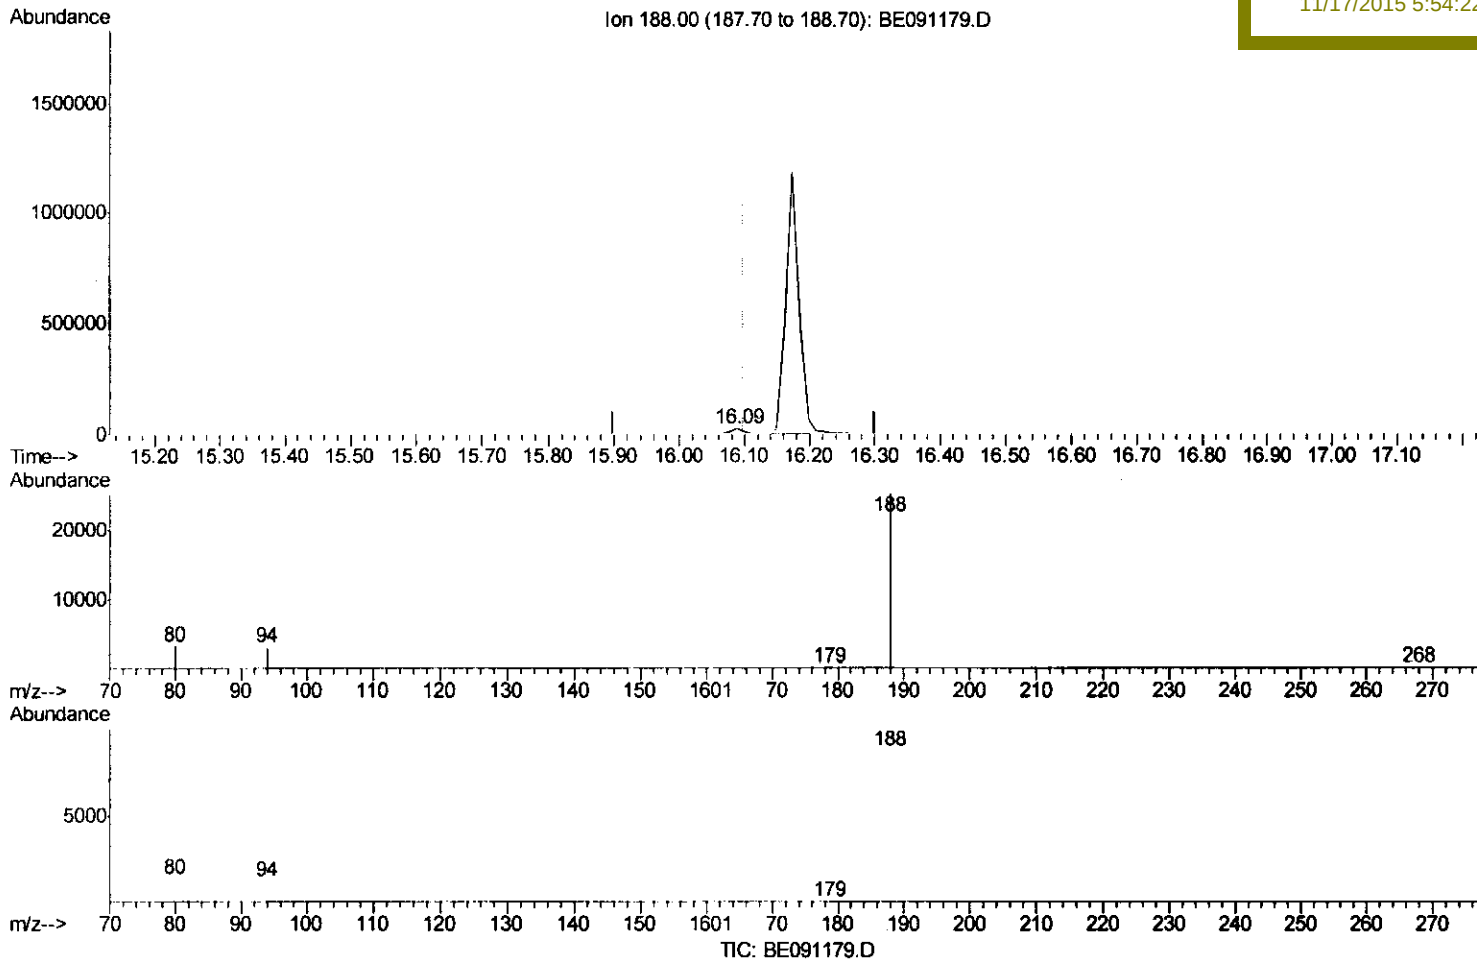

(12) Phenanthrene-d10 (I)

16.088min (-0.011) 0.40ng/ul m

response 33309

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	12.19#
80.00	8.90	13.04#
0.00	0.00	0.00

0.21
 11/12/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE111615\
 Data File : BE091179.D
 Acq On : 16 Nov 2015 12:04
 Operator : UM/NP
 Sample : PH86600BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK00

Quant Time: Nov 17 10:32:26 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Mon Nov 16 04:54:02 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mmdadoda
 11/17/2015 5:54:22 PM

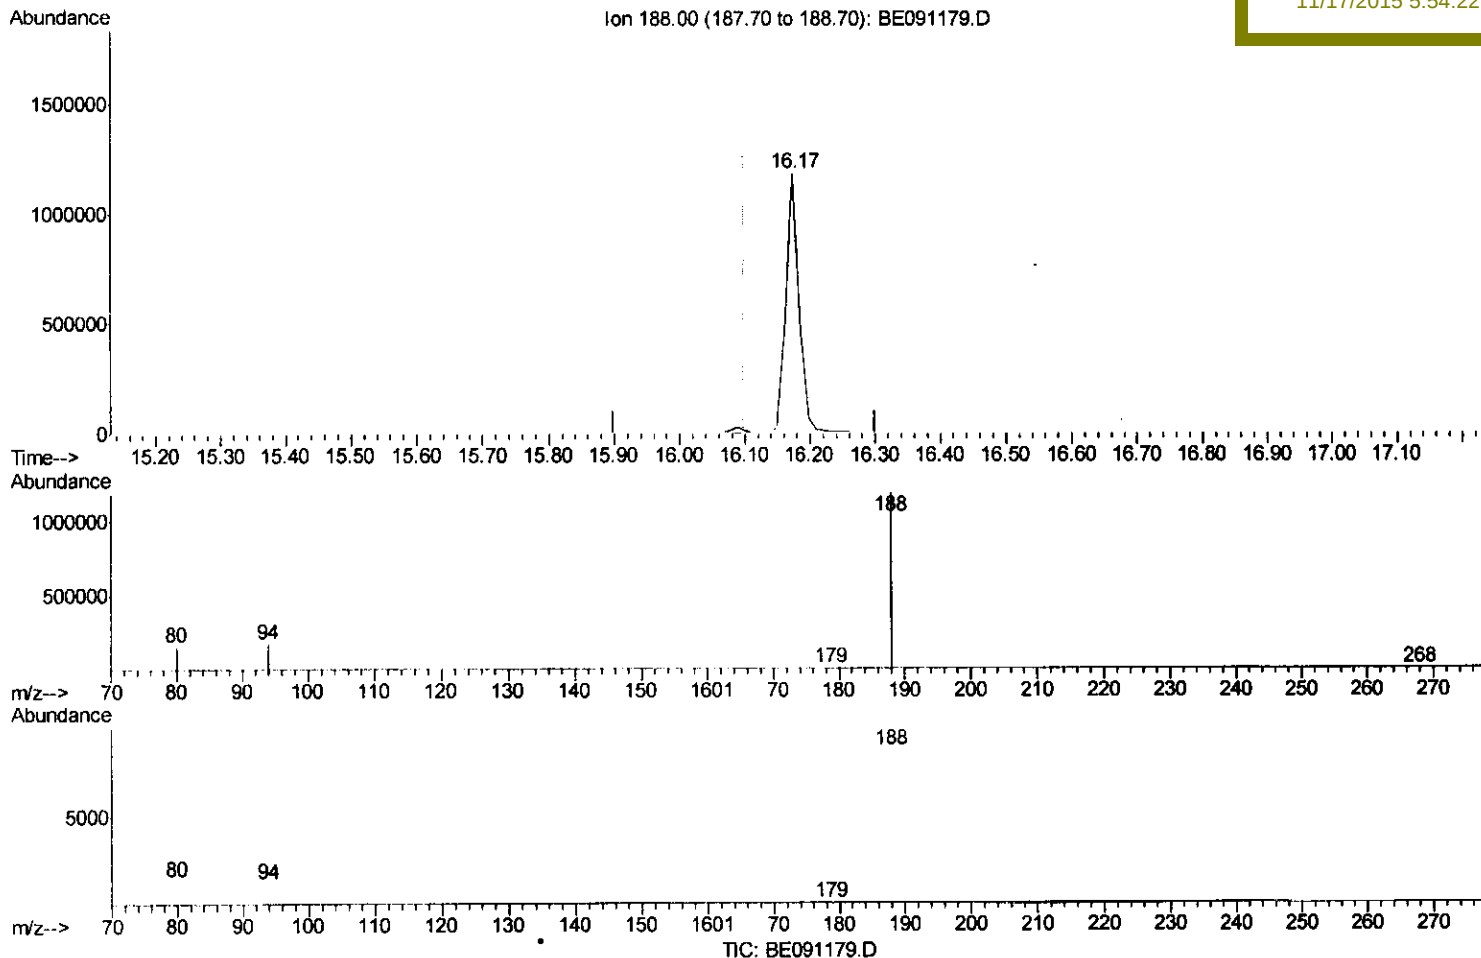

(12) Phenanthrene-d10 (I)

16.173min (+0.073) 0.40ng/ul

response 1655766

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	14.66#
80.00	8.90	13.36#
0.00	0.00	0.00