

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111615\
 Data File : BE091183.D
 Acq On : 16 Nov 2015 14:30
 Operator : UM/NP
 Sample : G4309-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 D9KQ1

Manual Integrations
 APPROVED

mmdadoda
 11/17/2015 5:54:38 PM

Quant Time: Nov 17 16:15:32 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 16 04:54:02 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	4049	0.40	ng/ul	-0.05
4) Naphthalene-d8	9.56	136	20287	0.40	ng/ul	-0.03
8) Acenaphthene-d10	13.37	164	12055	0.40	ng/ul	-0.01
12) Phenanthrene-d10	16.09	188	30720m	0.40	ng/ul	-0.01
18) Chrysene-d12	20.23	240	49732	0.40	ng/ul	0.00
22) Perylene-d12	22.12	264	41908m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.02	96	18964	6.51	ng/uL	-0.07
6) 2-Methylnaphthalene-d10	11.08	152	6149	0.22	ng/ul	0.00
16) Fluoranthene-d10	18.08	212	19590	0.23	ng/ul	0.00
Target Compounds						
5) Naphthalene	9.60	128	3357	0.07	ng/ul#	Ovalue 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE111615\
Data File : BE091183.D
Acq On : 16 Nov 2015 14:30
Operator : UM/NP
Sample : G4309-10
Misc :
ALS Vial : 16 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
D9KQ1

Manual Integrations
APPROVED

mmdadoda
11/17/2015 5:54:38 PM

Quant Time: Nov 17 16:15:32 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 16 04:54:02 2015
Response via : Initial Calibration

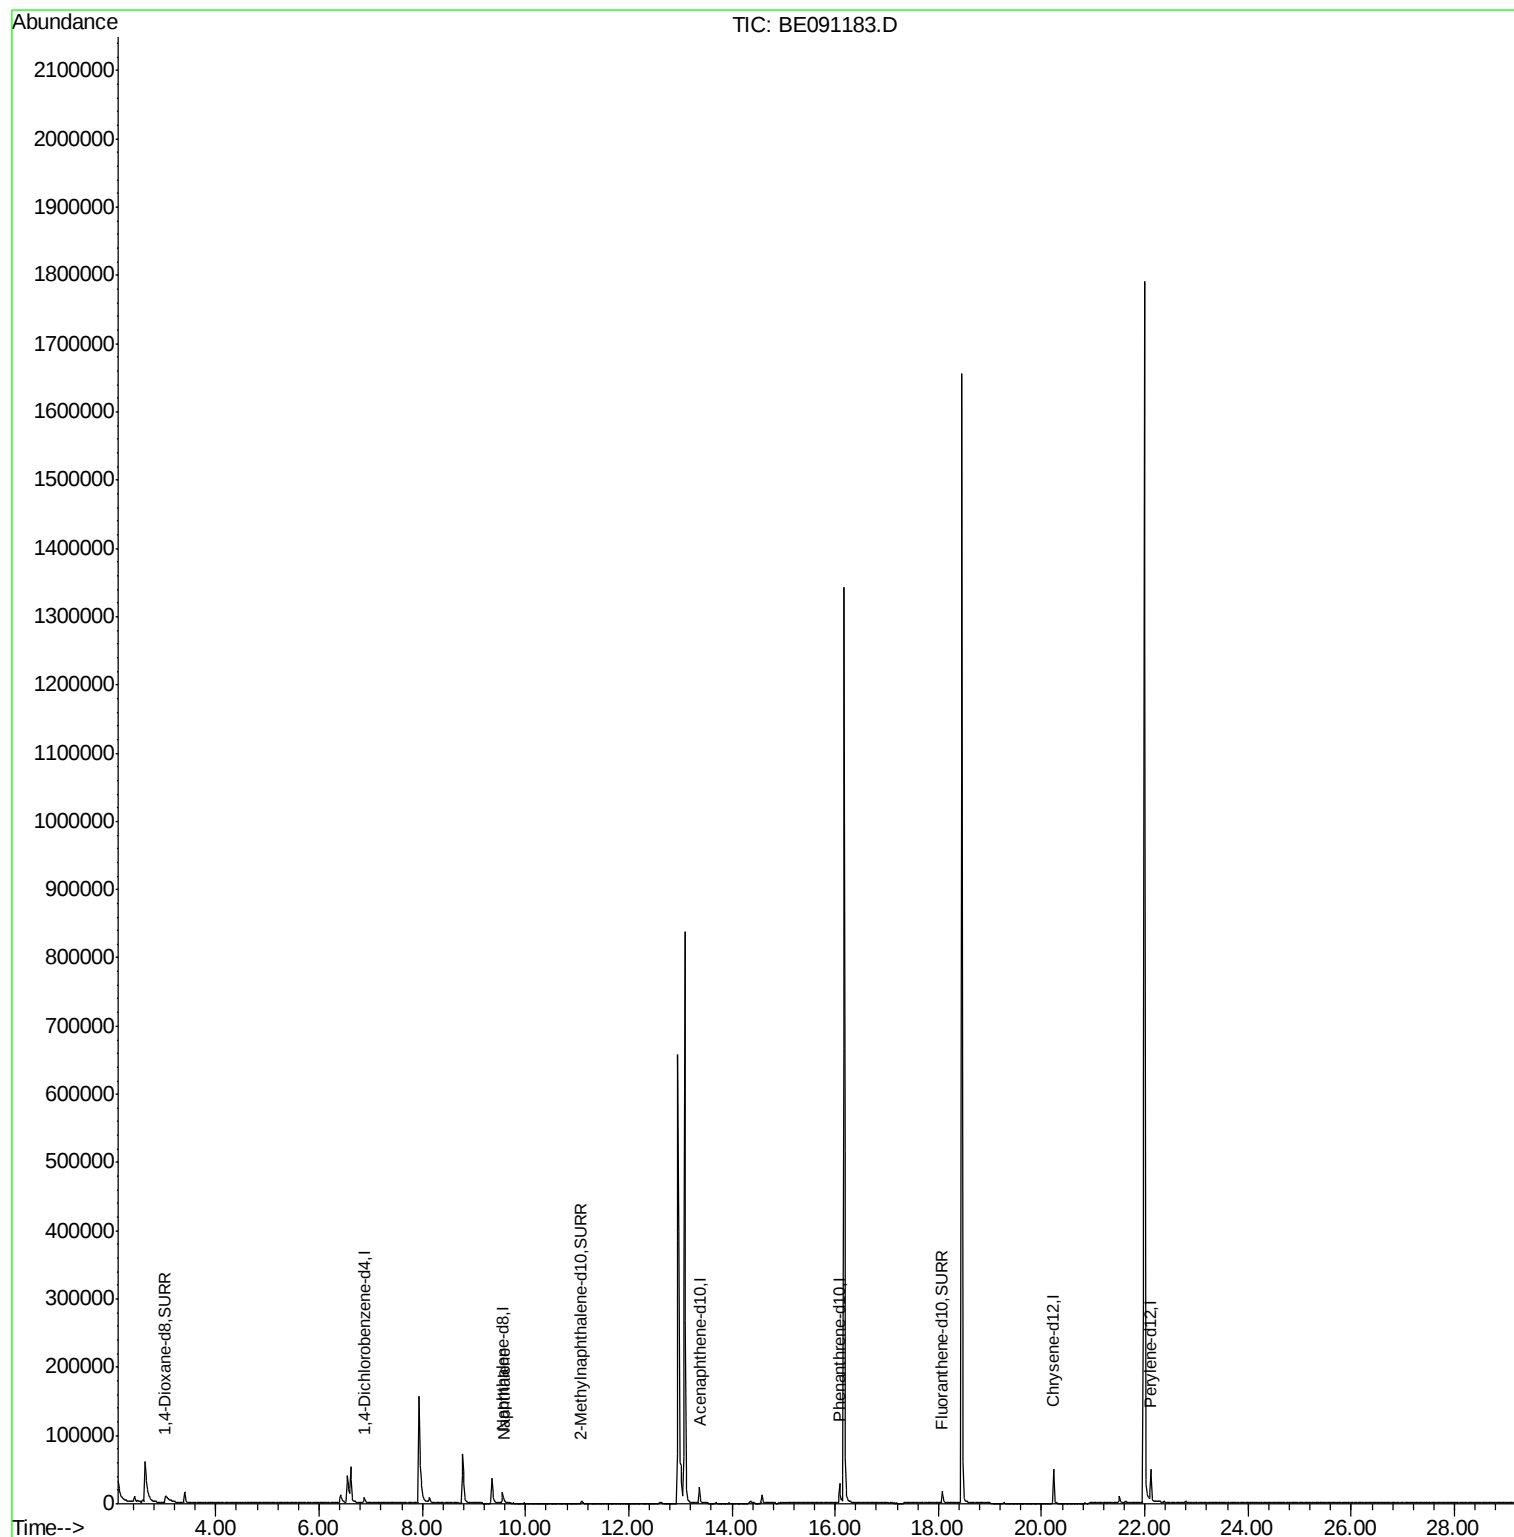

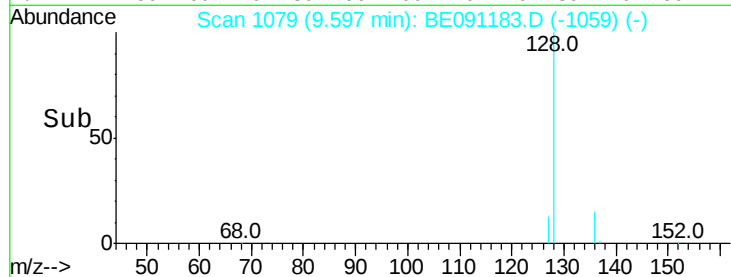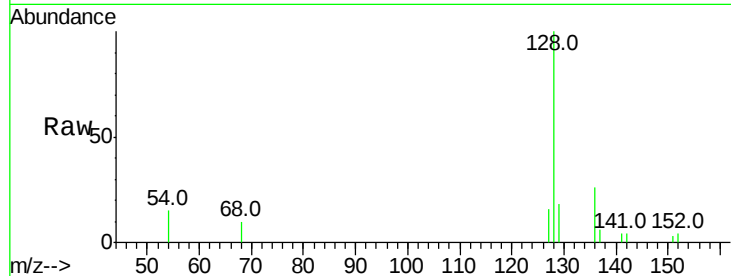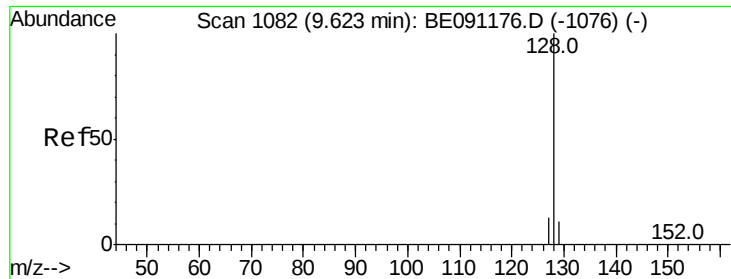

#5

Naphthalene

Concen: 0.07 ng/ul

RT: 9.60 min Scan# 1079

Delta R.T. -0.03 min

Lab File: BE091183.D

Acq: 16 Nov 2015 14:30

Tot Ion:	128	Resp:	3357
Ion Ratio	Lower	Upper	
128	100		
129	18.3	9.8	14.8#
127	16.0	10.7	16.1

Instrument :

BNA_E

ClientSampleId :

D9KQ1

Manual Integrations
APPROVED

mmdadoda
11/17/2015 5:54:38 PM

