


1,4-Dioxane

Response Ratio

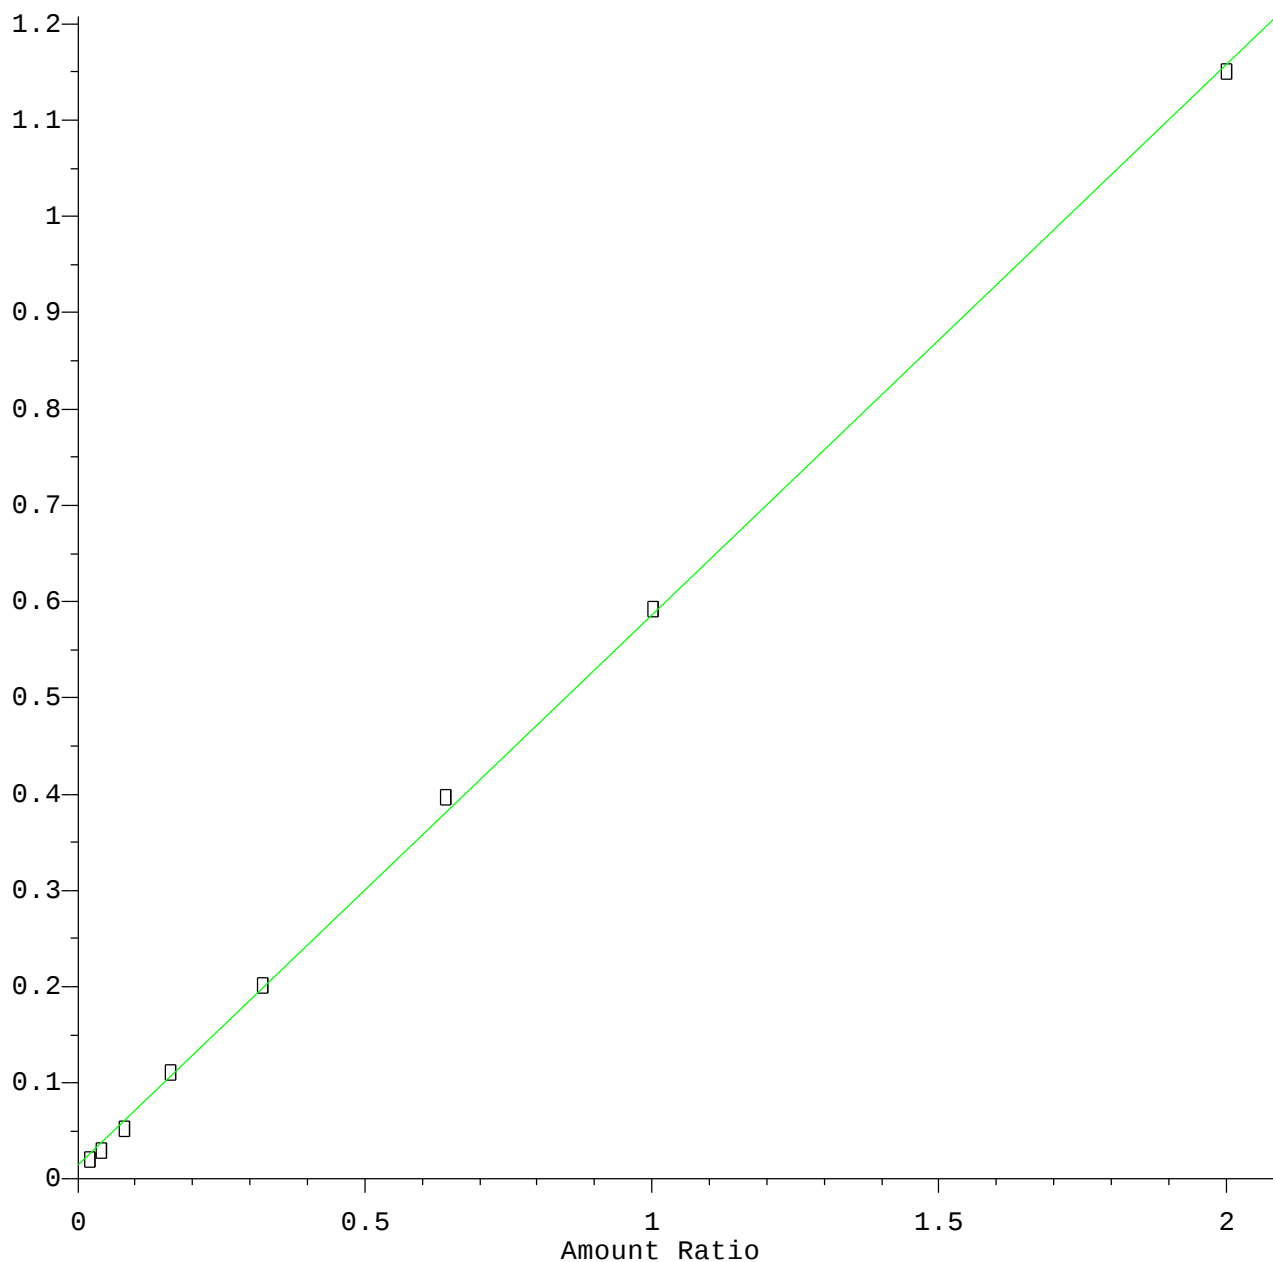


Resp Ratio = $5.72 \times 10^{-1} \times \text{Amt} + 1.40 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111616.M
Calibration Table Last Updated: Wed Nov 16 15:43:18 2016


n-Nitrosodimethylamine

Response Ratio

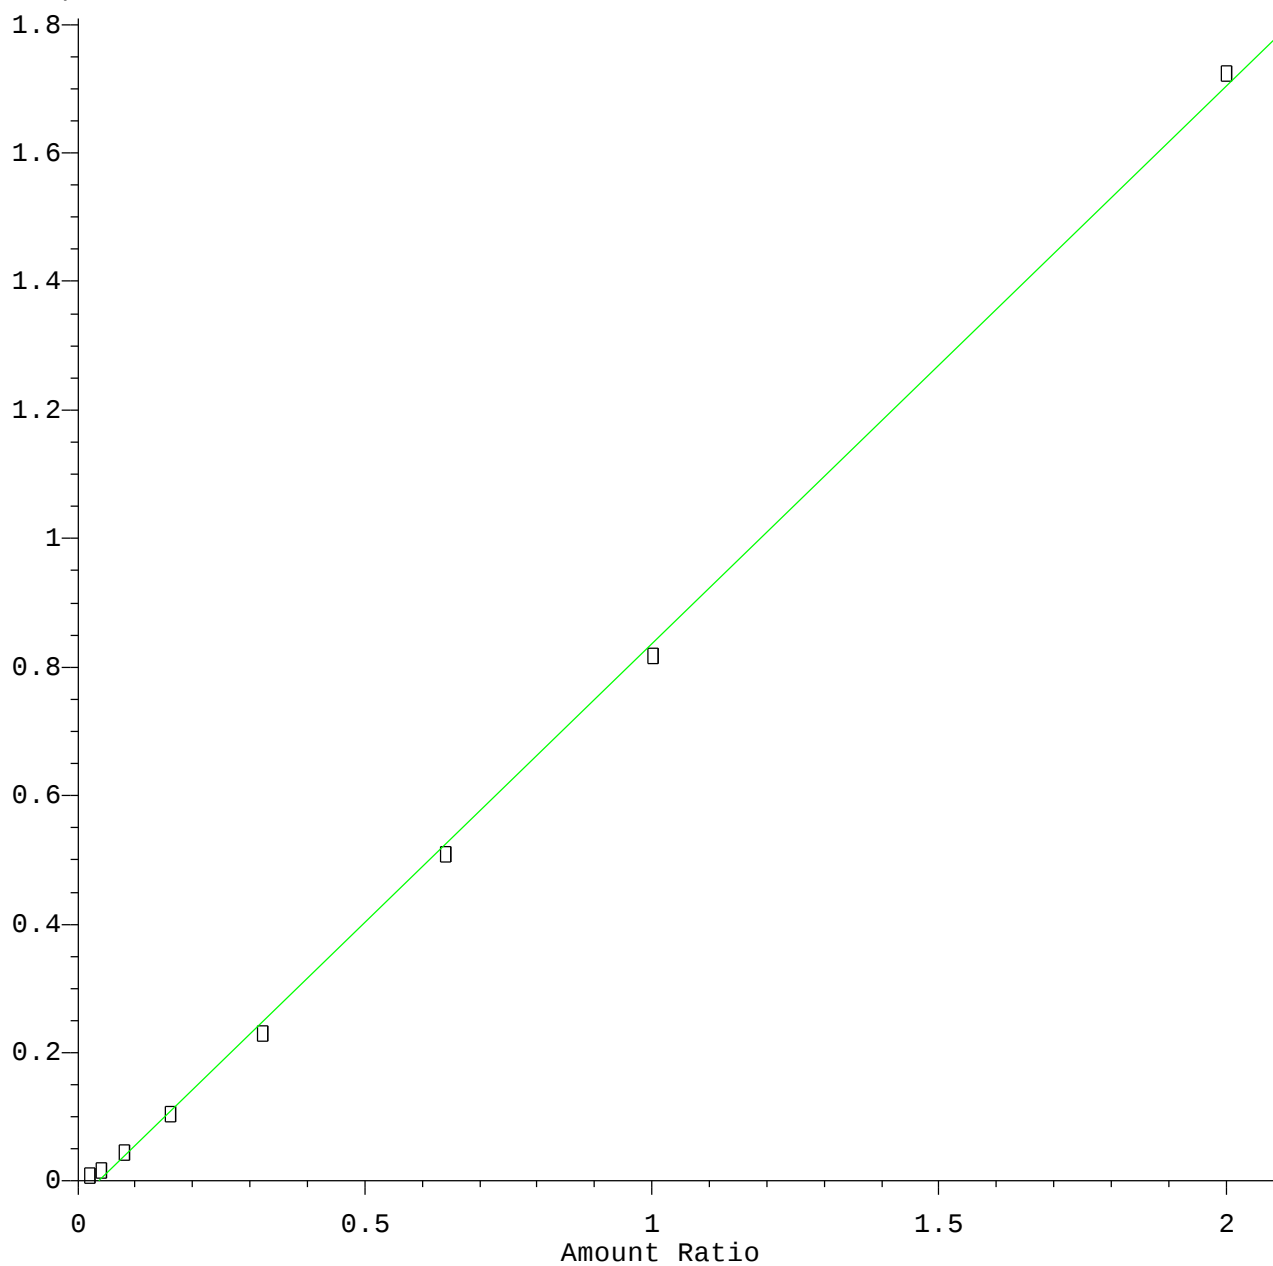

Resp Ratio = $8.68 \times 10^{-1} \times \text{Amt} - 3.09 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111616.M
Calibration Table Last Updated: Wed Nov 16 15:43:18 2016

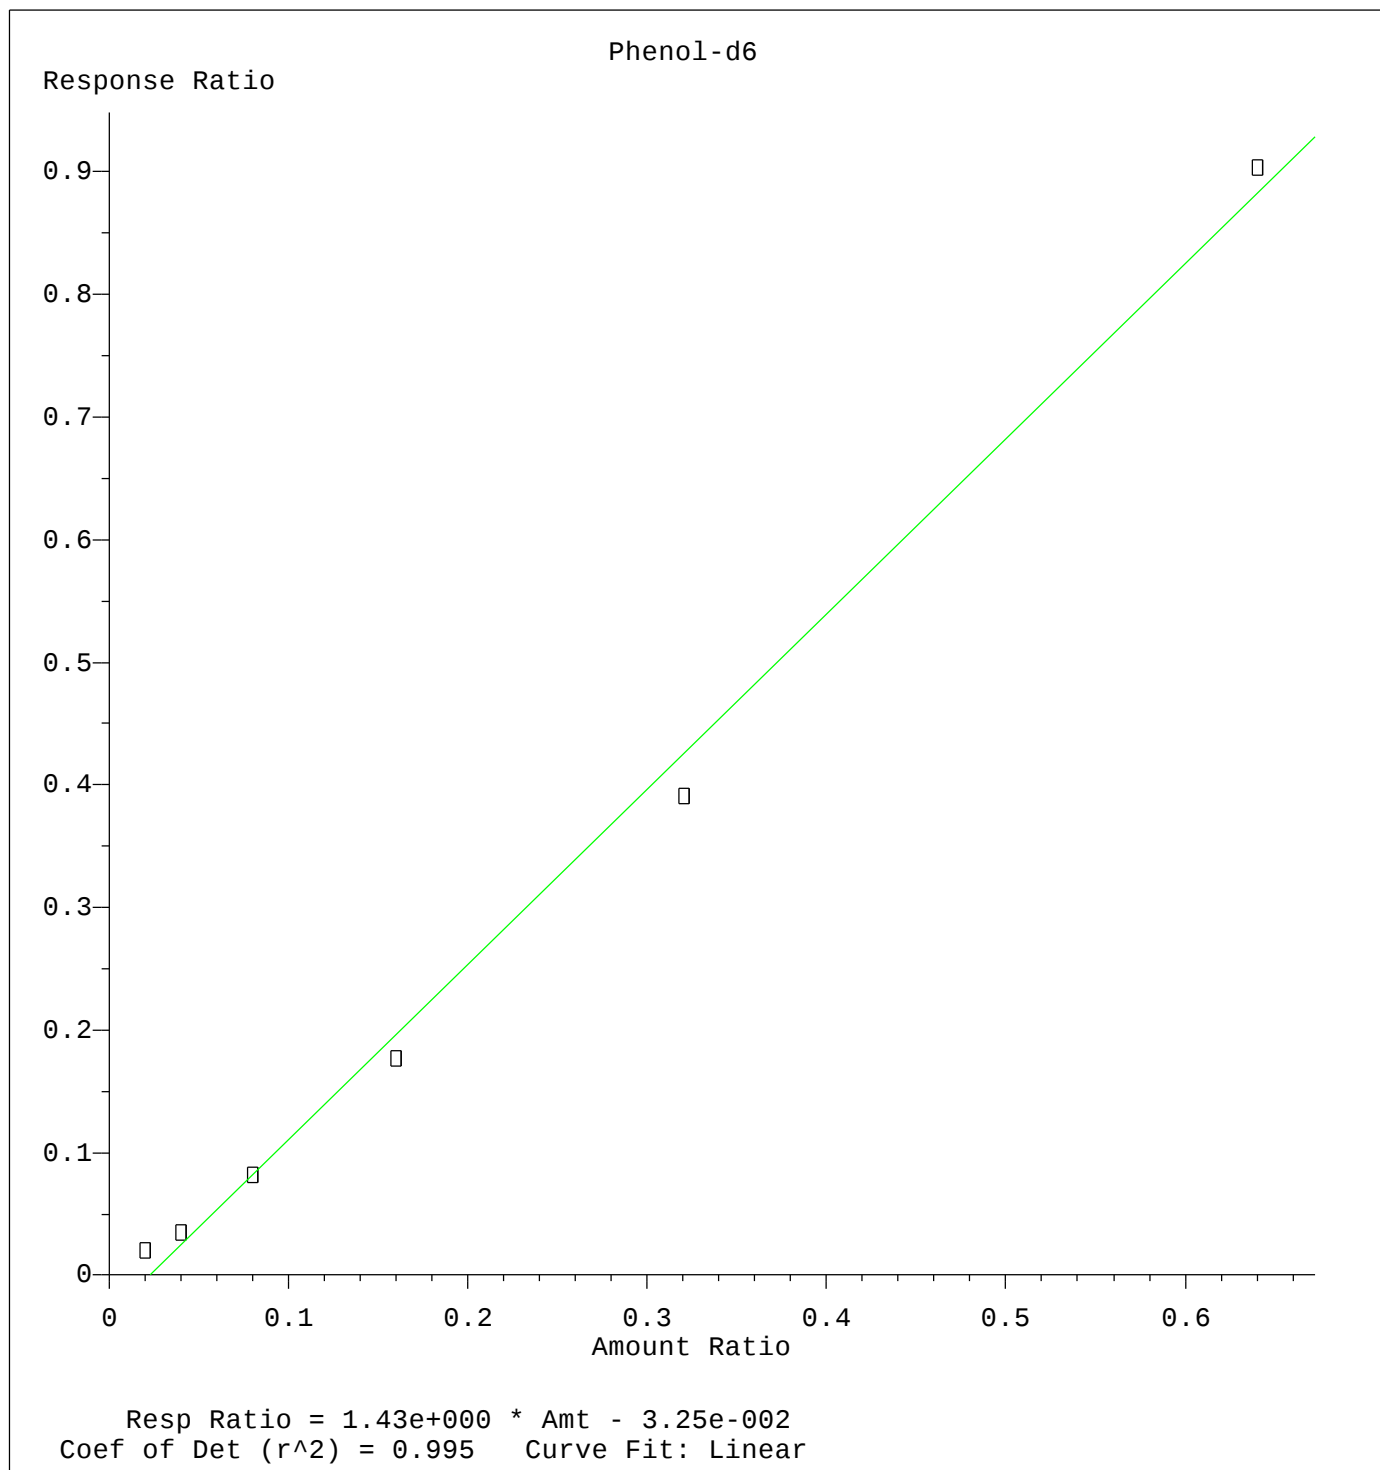

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111616.M
Calibration Table Last Updated: Wed Nov 16 15:43:18 2016


bis(2-Chloroethyl)ether

Response Ratio

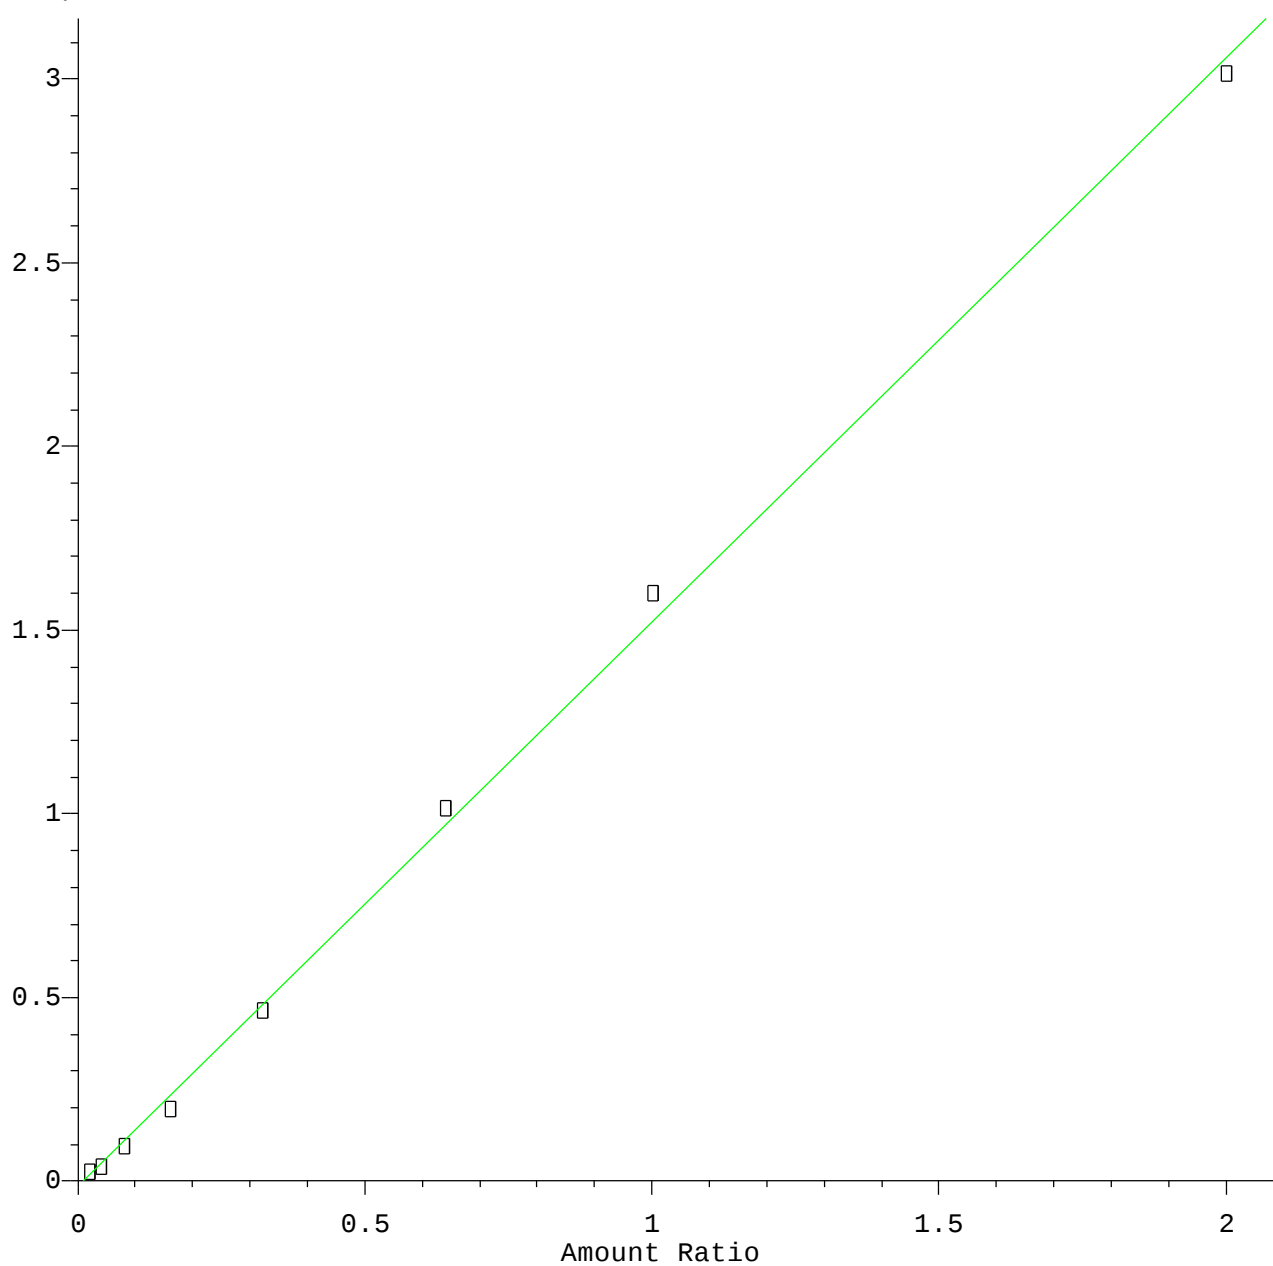


Resp Ratio = 1.54e+000 * Amt - 1.22e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111616.M
Calibration Table Last Updated: Wed Nov 16 15:43:18 2016

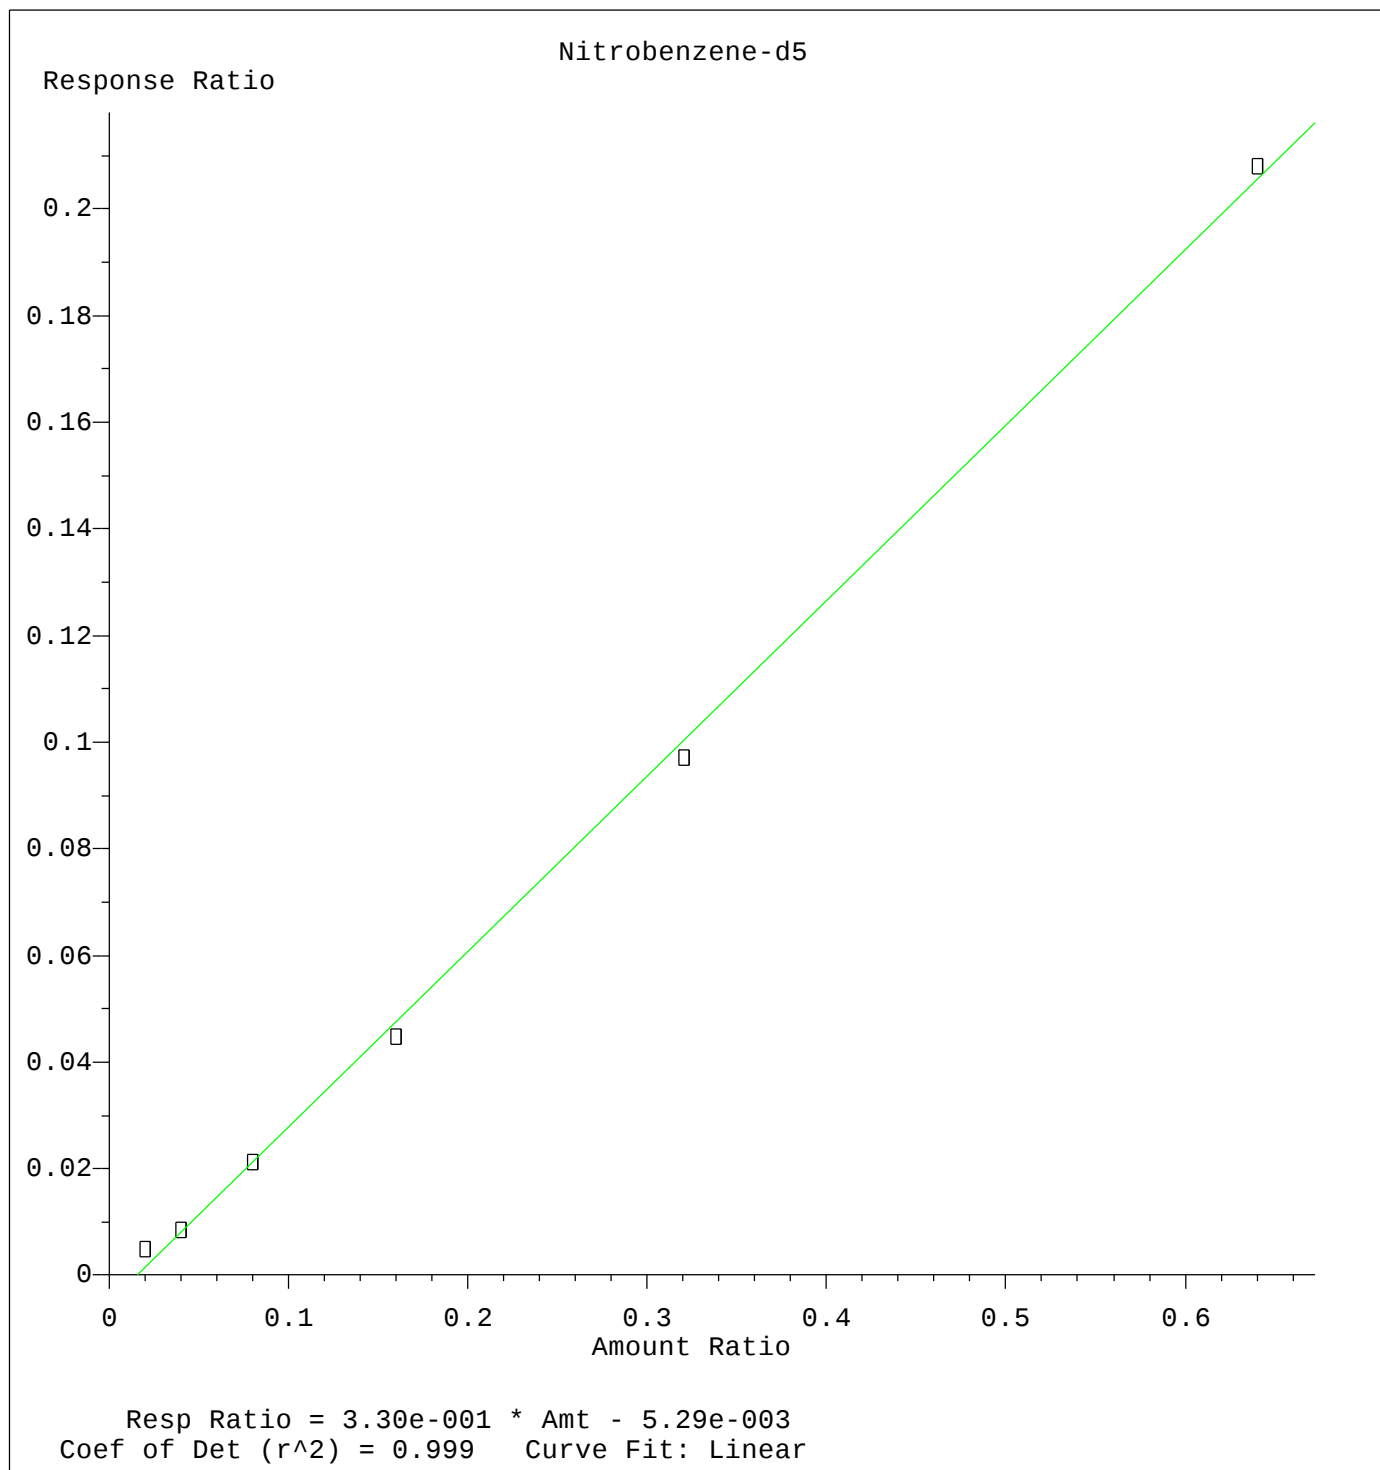


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111616.M
Calibration Table Last Updated: Wed Nov 16 15:43:18 2016

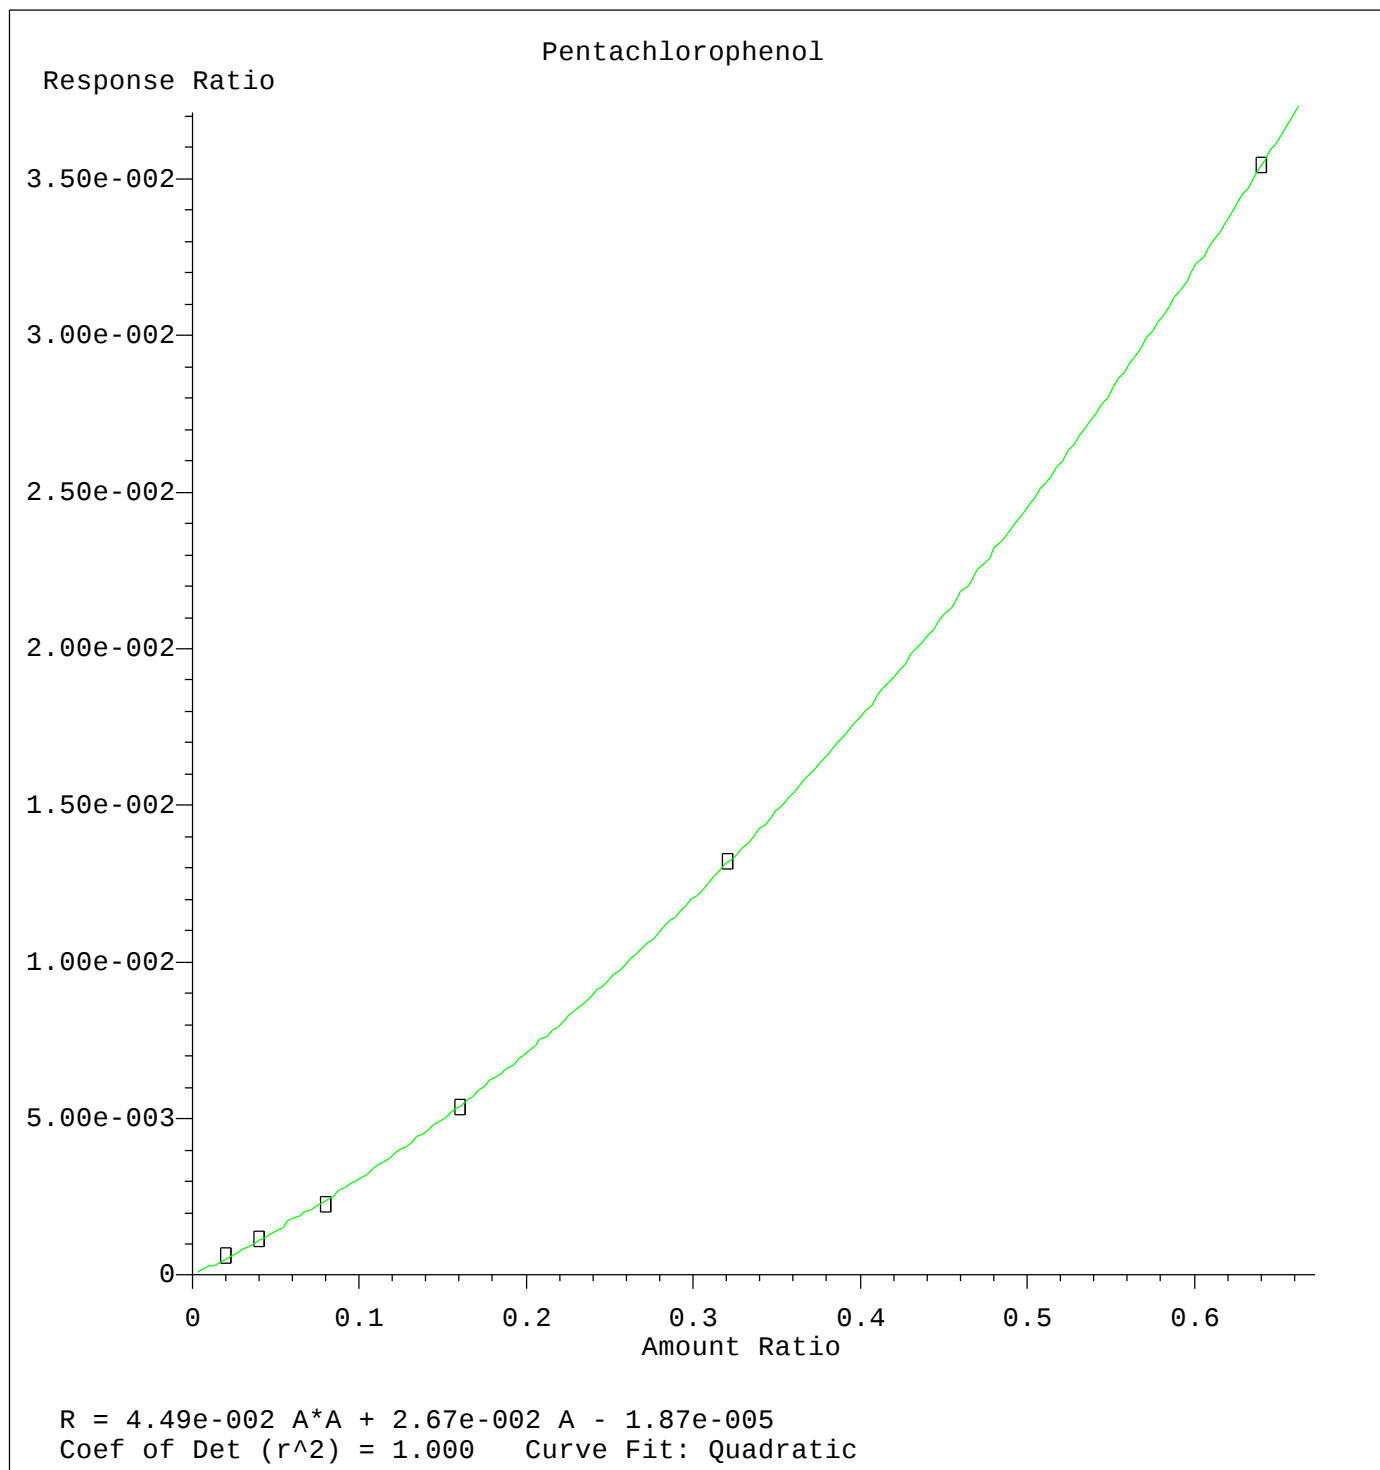

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111616.M
Calibration Table Last Updated: Wed Nov 16 15:43:18 2016

Benzo(a)anthracene


Response Ratio

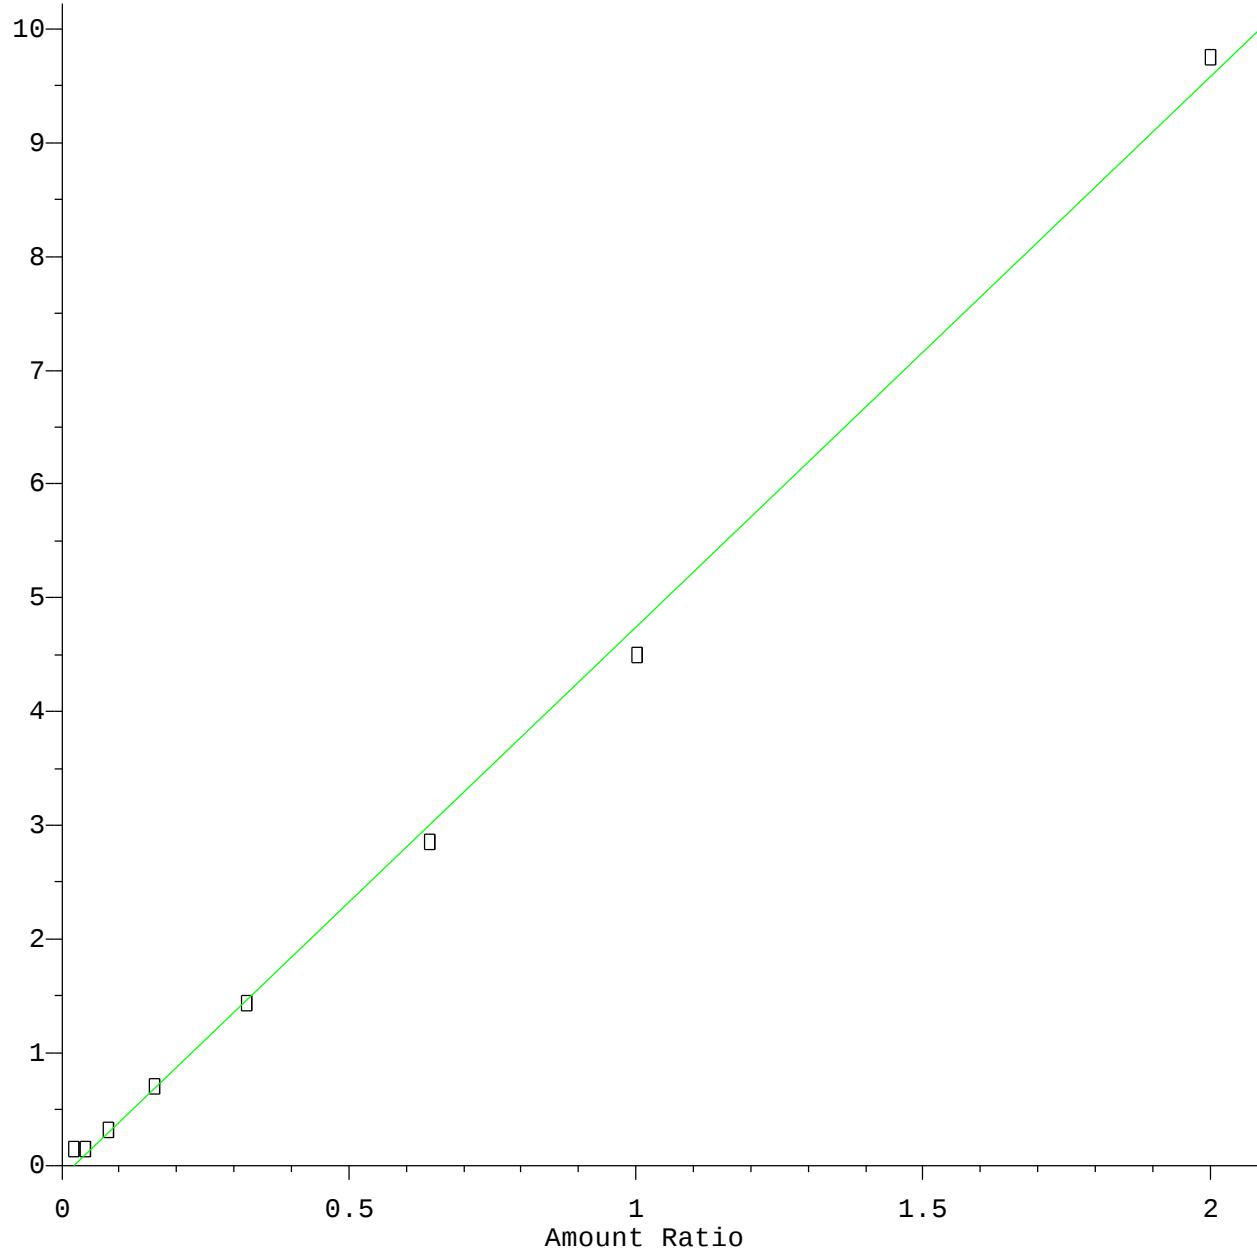

Resp Ratio = 4.84×10^0 * Amt - 9.73×10^{-2}
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111616.M
Calibration Table Last Updated: Wed Nov 16 15:43:18 2016

Bis(2-ethylhexyl)phthalate

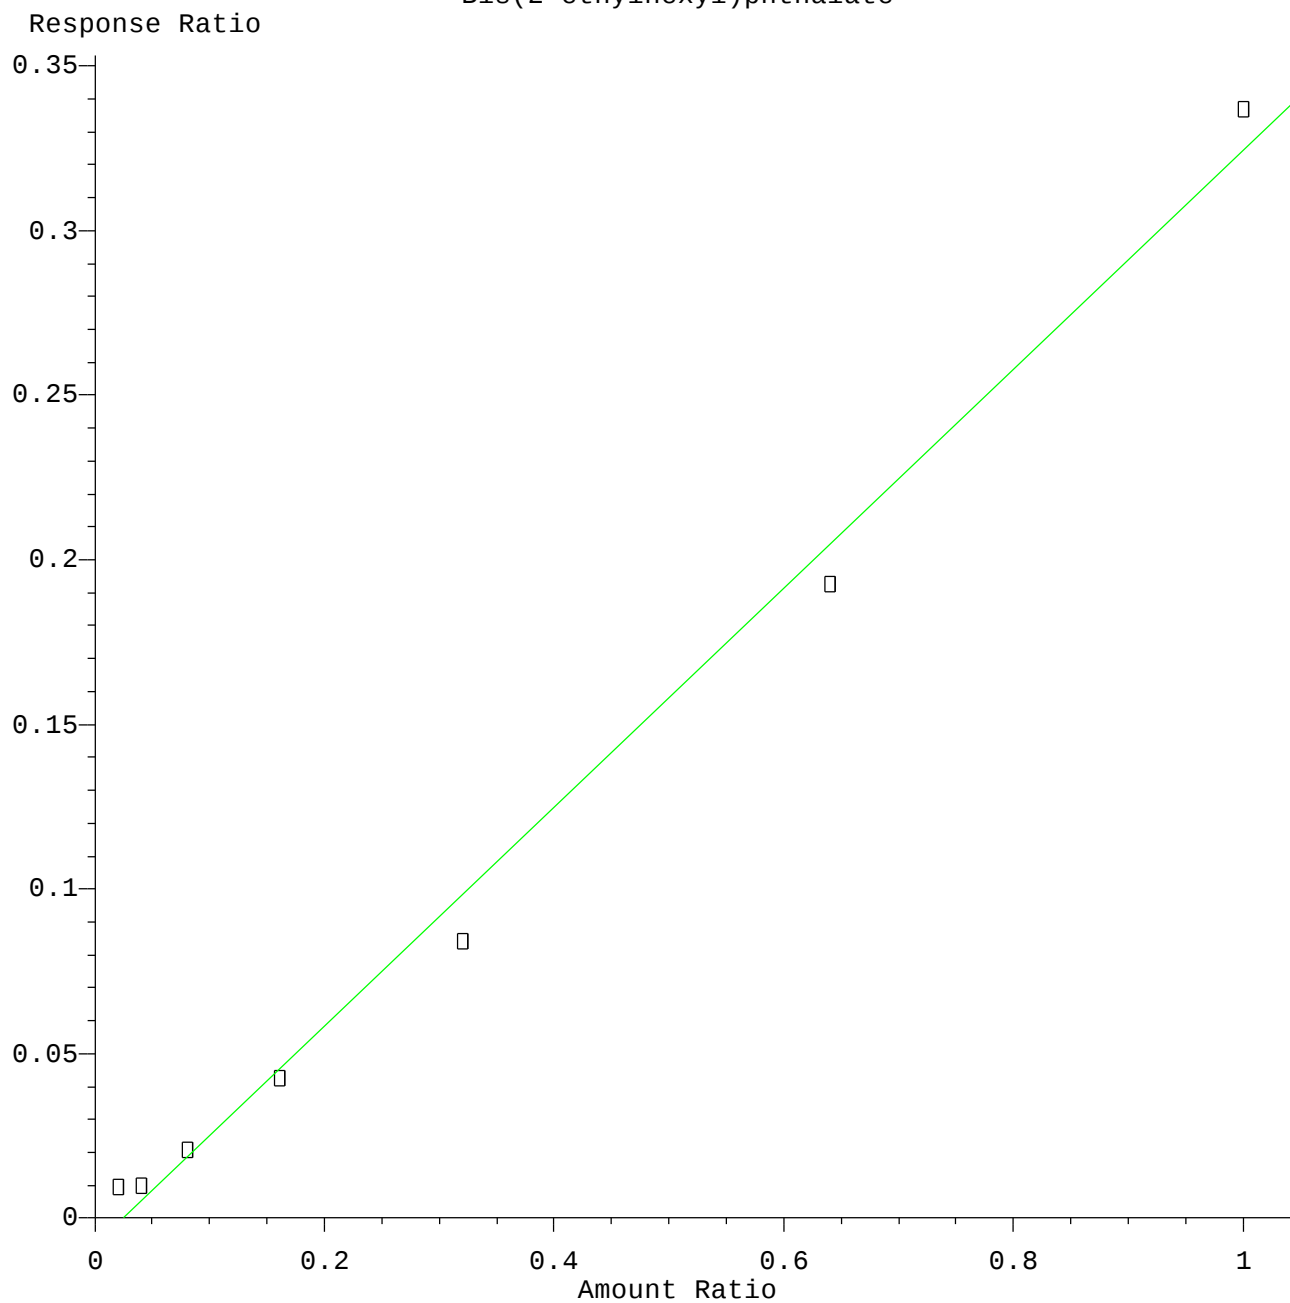


Resp Ratio = $3.32 \times 10^{-1} \times \text{Amt} - 8.00 \times 10^{-3}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111616.M
Calibration Table Last Updated: Wed Nov 16 15:43:18 2016

Indeno(1,2,3-cd)pyrene

Response Ratio

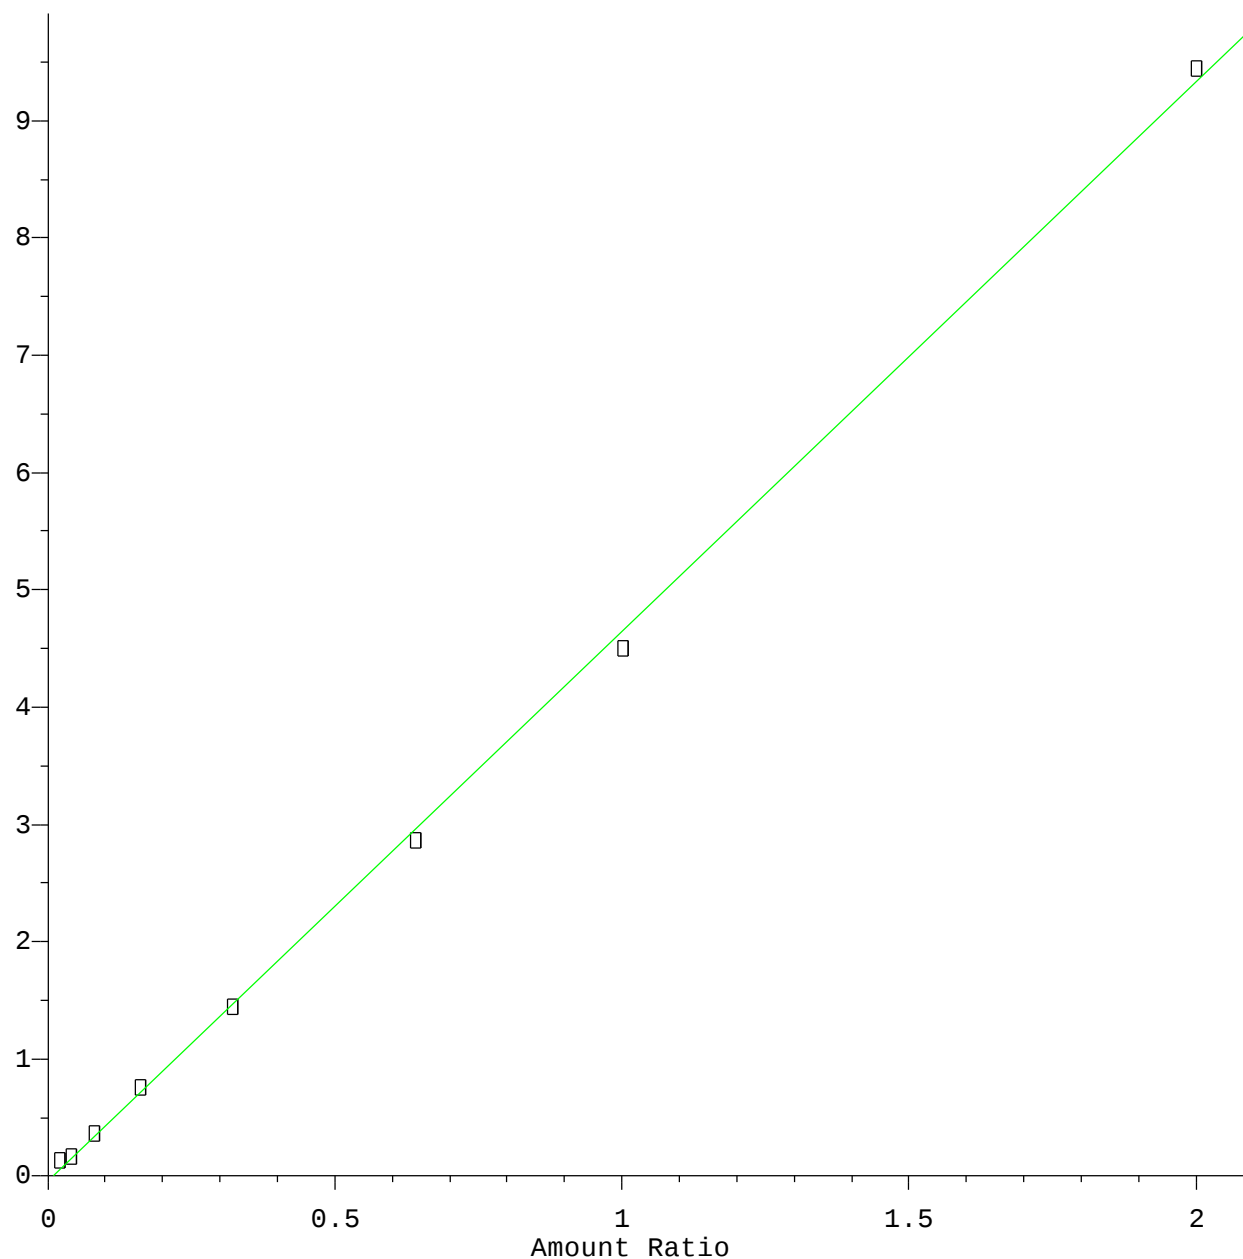

Resp Ratio = 4.69×10^0 * Amt - 4.30×10^{-2}
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111616.M
Calibration Table Last Updated: Wed Nov 16 15:43:18 2016