
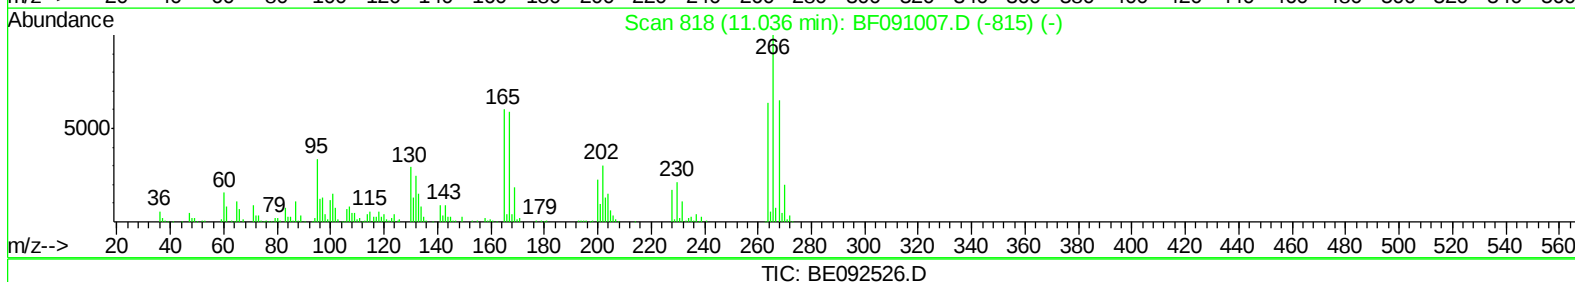
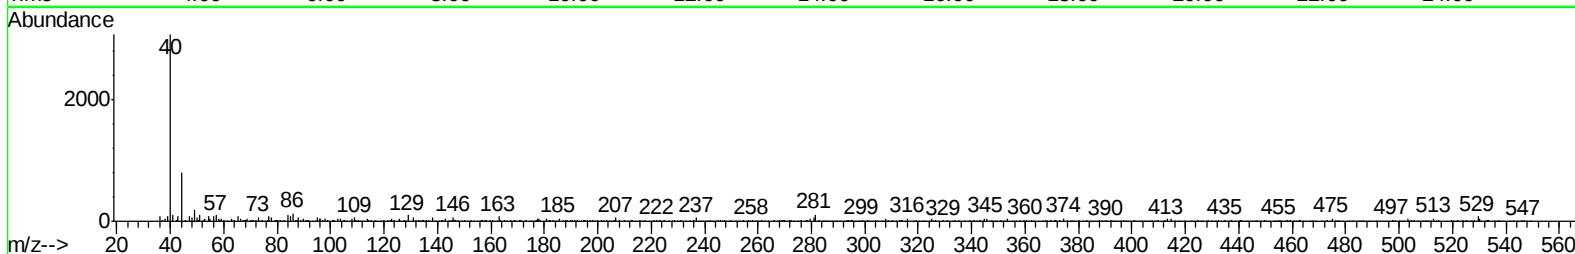


Data Path : Z:\HPCHEM1\BNA_E\Data\BE111616\
Data File : BE092526.D
Acq On : 16 Nov 2016 9:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 08:01:34 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

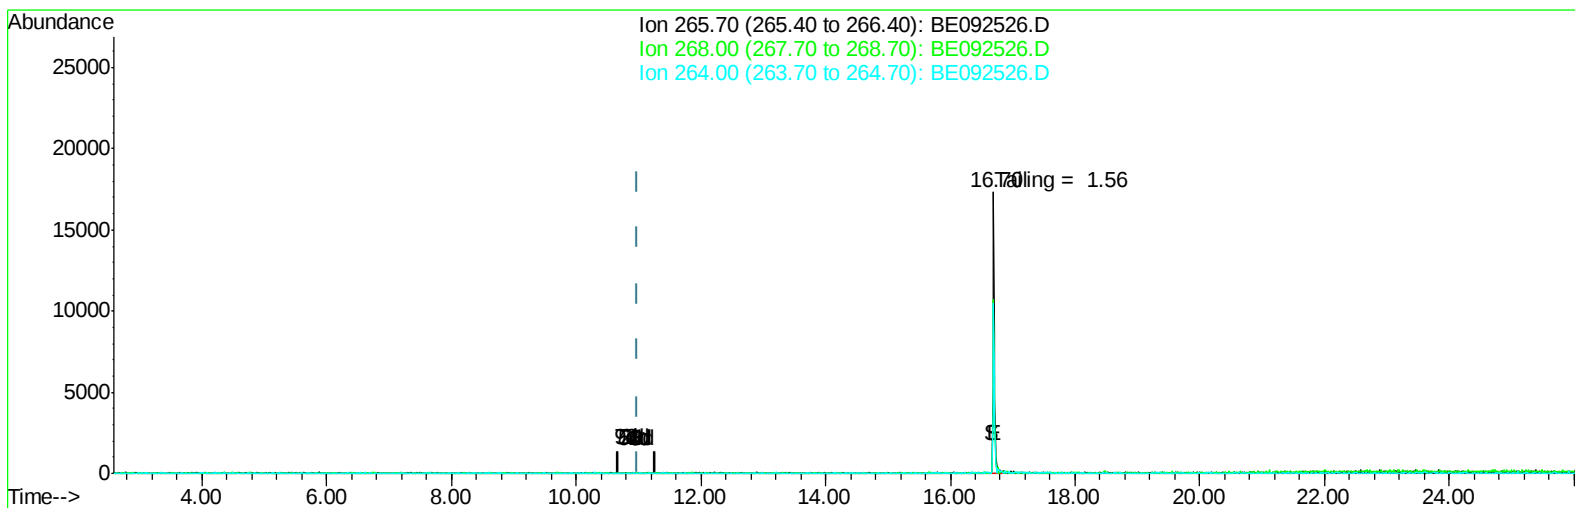




TIC: BE092526.D

(69) Pentachlorophenol (C)
10.949min (-0.042) 123.49ng
response 32

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	92.59#
264.00	63.90	22.22#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE111616\
Data File : BE092526.D
Acq On : 16 Nov 2016 9:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 08:01:34 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

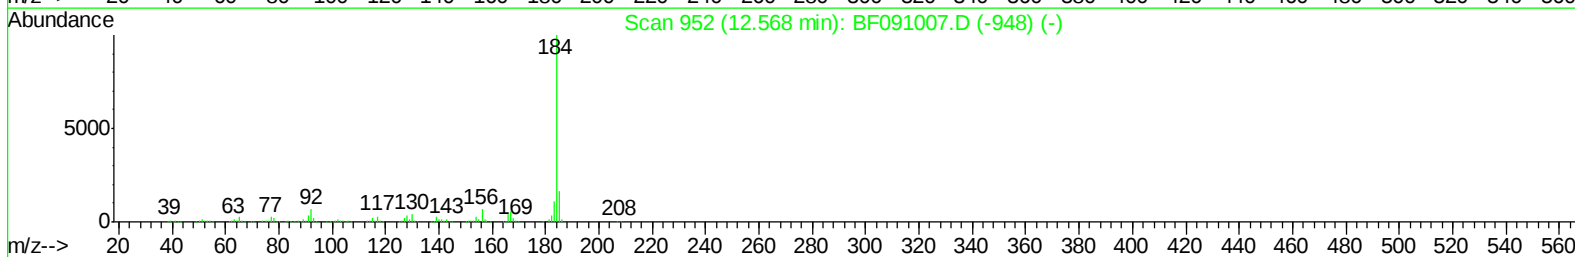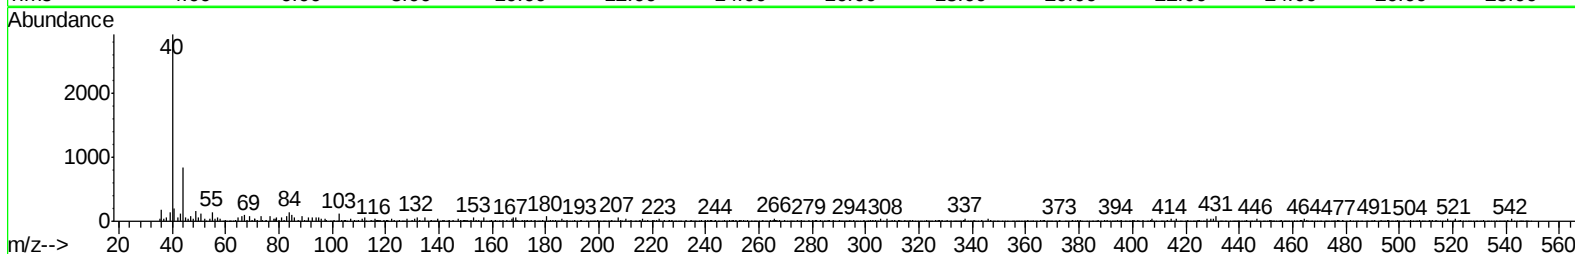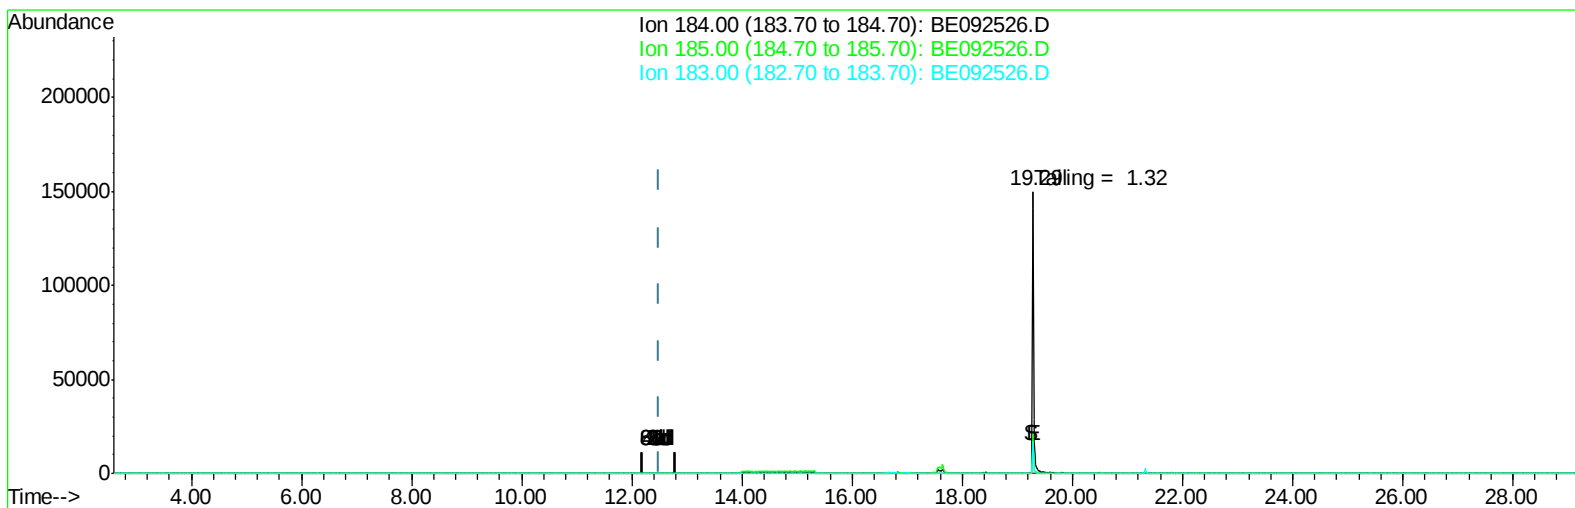

TIC: BE092526.D

(76) Benzidine

12.459min (-0.052) 40.87ng

response 21

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	2.94#
183.00	10.90	120.59#
0.00	0.00	0.00