
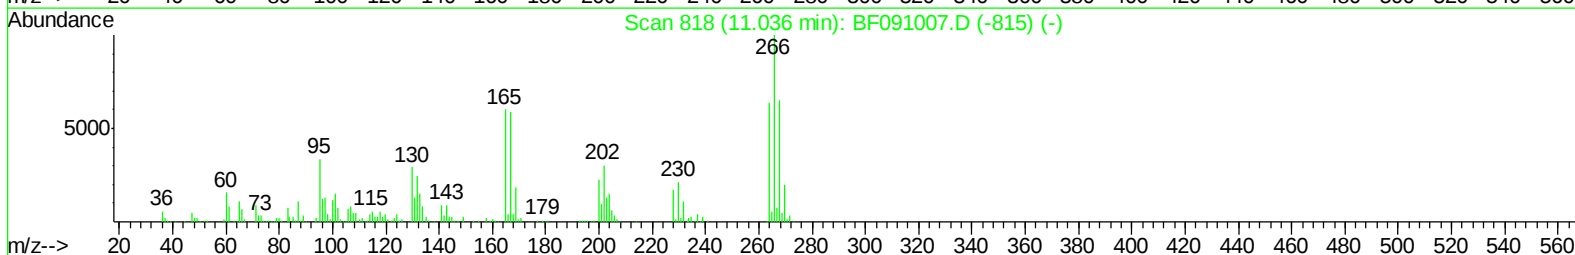
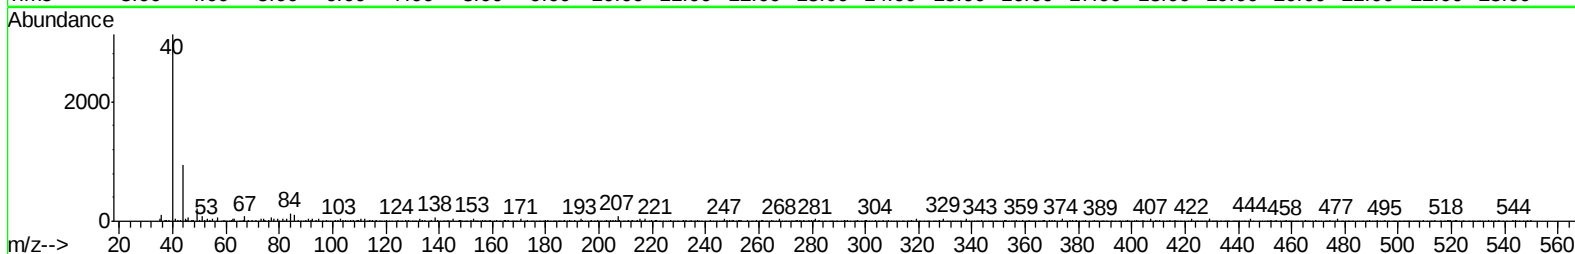


Data Path : Z:\HPCHEM1\BNA_E\Data\BE111616\
Data File : BE092537.D
Acq On : 16 Nov 2016 16:37
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 08:02:56 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

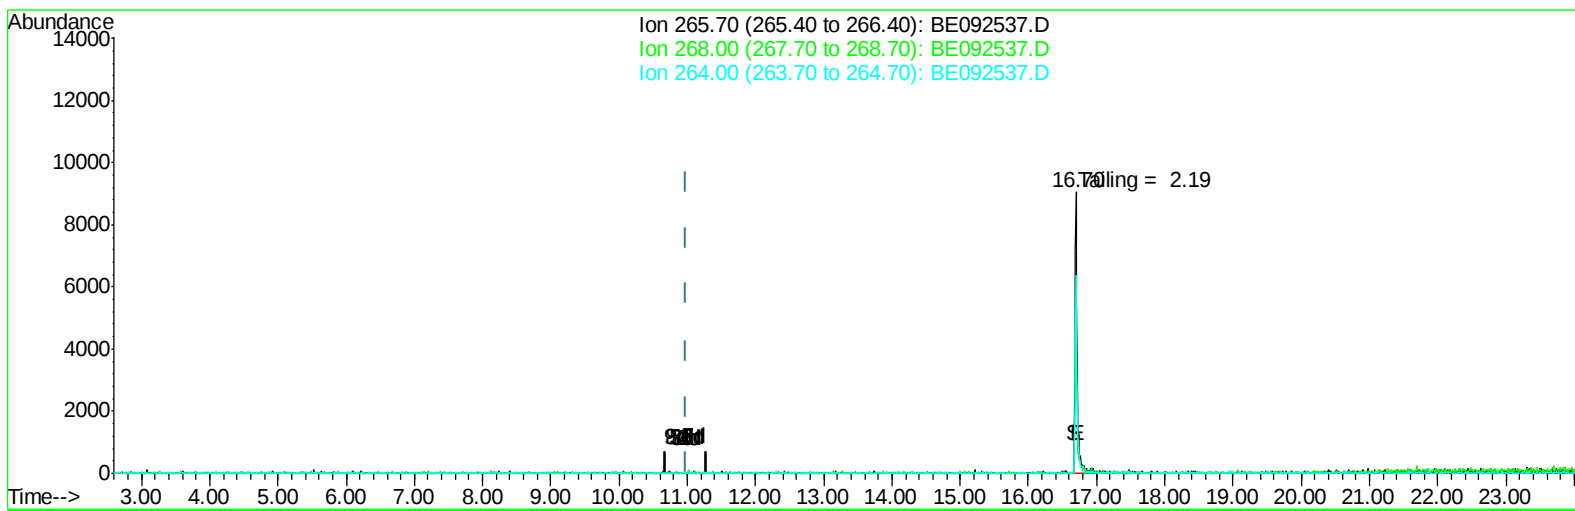




TIC: BE092537.D

(69) Pentachlorophenol (C)
10.990min (-0.000) 157.45ng
response 8

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	411.11#
264.00	63.90	77.78#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE111616\
 Data File : BE092537.D
 Acq On : 16 Nov 2016 16:37
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 08:02:56 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 08 12:59:29 2016
 Response via : Initial Calibration

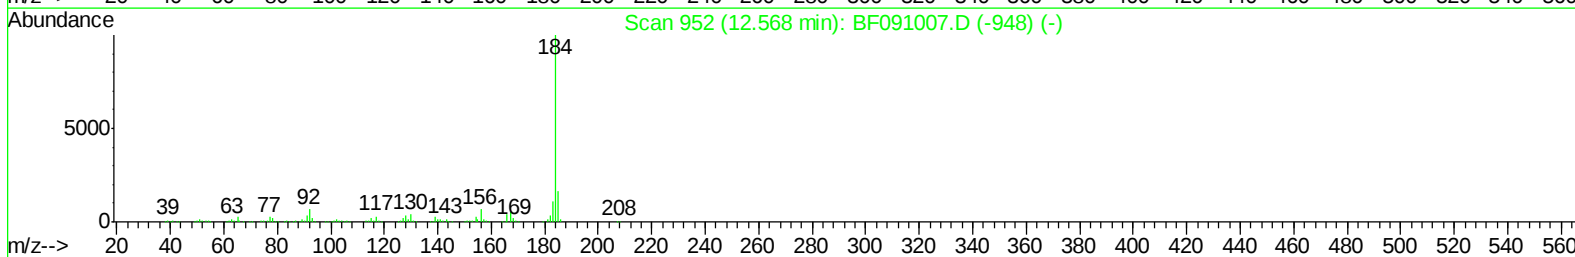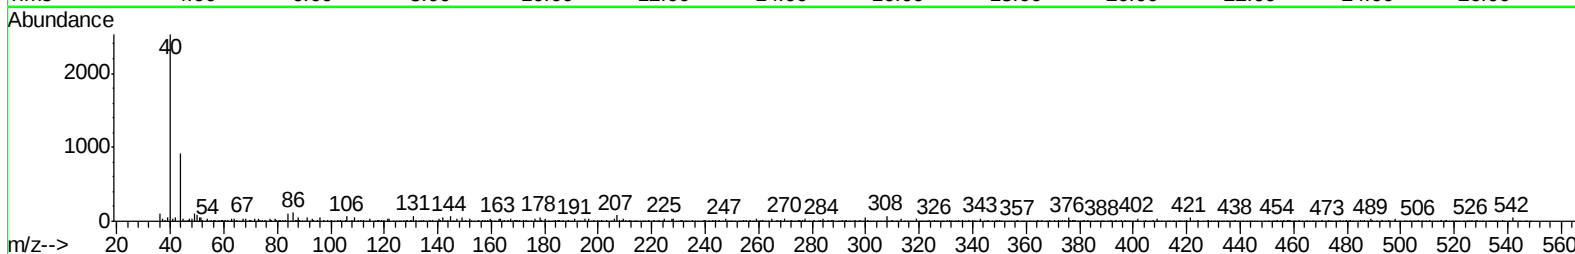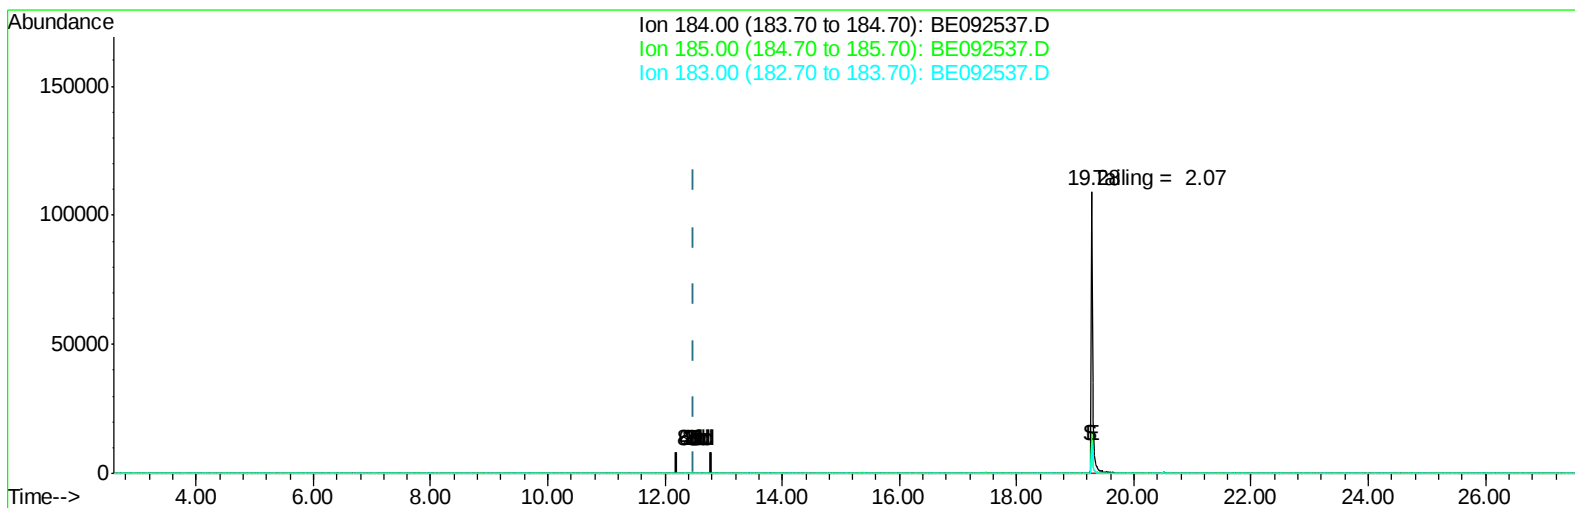

TIC: BE092537.D

(76) Benzidine

12.547min (+0.037) 4.40ng

response 6

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	228.57#
183.00	10.90	57.14#
0.00	0.00	0.00