

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111616\
 Data File : BE092541.D
 Acq On : 16 Nov 2016 19:42
 Operator : UM/SJ
 Sample : H5636-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 CPS043041

Quant Time: Nov 17 04:59:27 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE111616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 15:43:18 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	7647	5.00	ng	-0.02
7) Naphthalene-d8	10.93	136	34059	5.00	ng	0.00
12) Acenaphthene-d10	14.80	164	23755	5.00	ng	0.00
18) Phenanthrene-d10	17.56	188	53087	5.00	ng	0.00
24) Chrysene-d12	21.72	240	79441	5.00	ng	0.00
31) Perylene-d12	24.08	264	68226	5.00	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.66	112	6314	4.89	ng	-0.02
5) Phenol-d6	7.31	99	5046	2.42	ng	-0.04
8) Nitrobenzene-d5	9.34	82	9916	4.49	ng	-0.02
13) 2,4,6-Tribromophenol	16.30	330	5716	10.73	ng	-0.01
14) 2-Fluorobiphenyl	13.42	172	26903	4.65	ng	-0.01
26) Terphenyl-d14	20.16	244	50281	5.54	ng	-0.02
Target Compounds						
29) Bis(2-ethylhexyl)phthalate	21.61	149	1884	0.48	ng	Qvalue # 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111616\
Data File : BE092541.D
Acq On : 16 Nov 2016 19:42
Operator : UM/SJ
Sample : H5636-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
CPS043041

Quant Time: Nov 17 04:59:27 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE111616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 15:43:18 2016
Response via : Initial Calibration

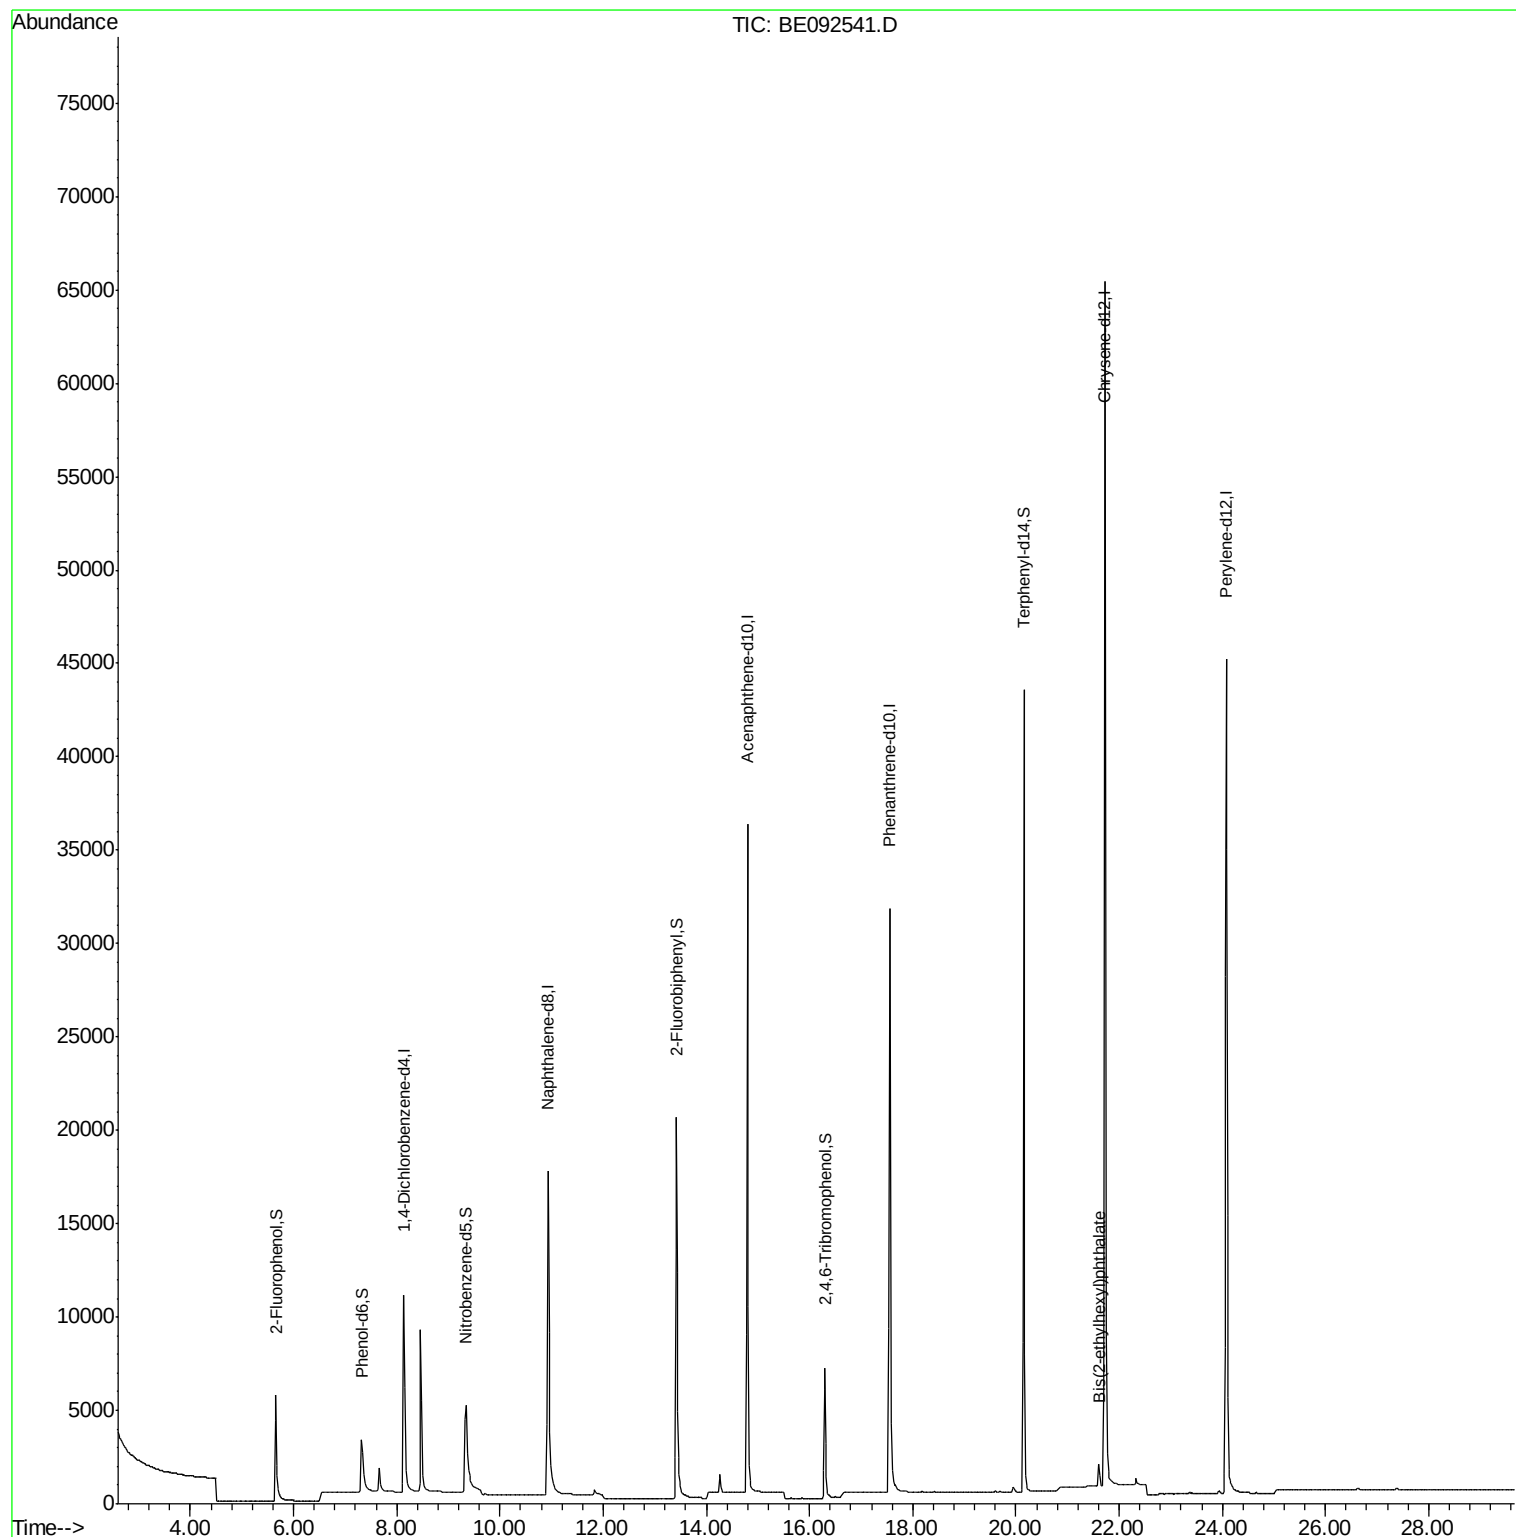

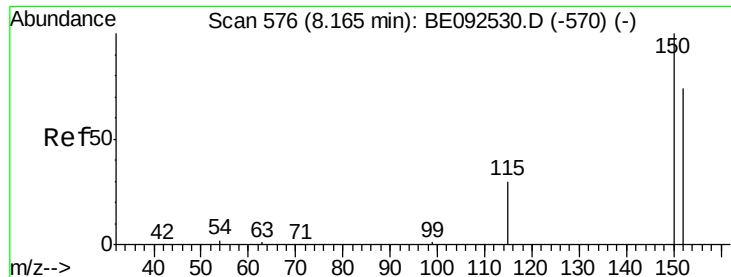

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.14 min Scan# 575

Delta R.T. -0.02 min

Lab File: BE092541.D

Acq: 16 Nov 2016 19:42

Instrument :

BNA_E

ClientSampleId :

CPS043041


Tot Ion:152 Resp: 7647

Ion Ratio Lower Upper

152 100

150 181.1 106.0 159.0#




115 88.0 31.2 46.8#

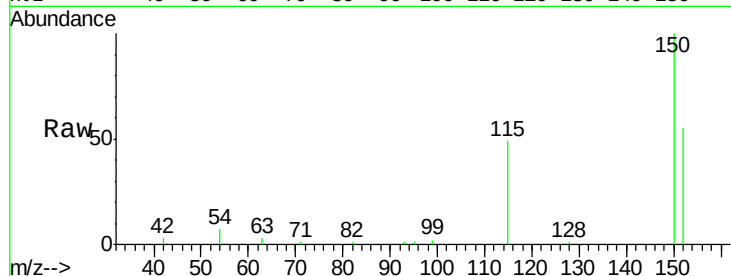

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

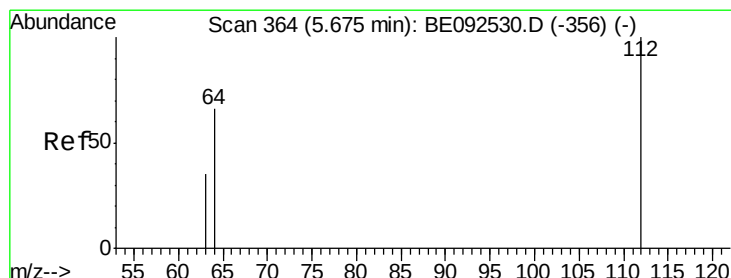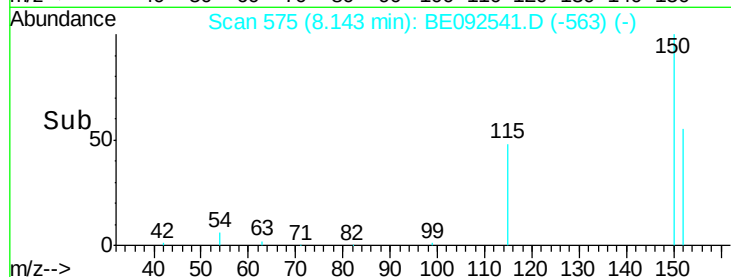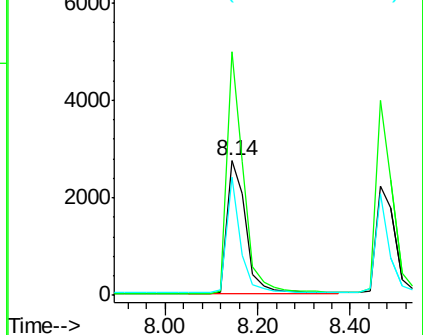

#4

2-Fluorophenol

Concen: 4.89 ng

RT: 5.66 min Scan# 361

Delta R.T. -0.02 min

Lab File: BE092541.D

Acq: 16 Nov 2016 19:42


Tgt Ion:112 Resp: 6314

Ion Ratio Lower Upper

112 100

64 68.1 53.5 80.3



63 36.5 27.9 41.9

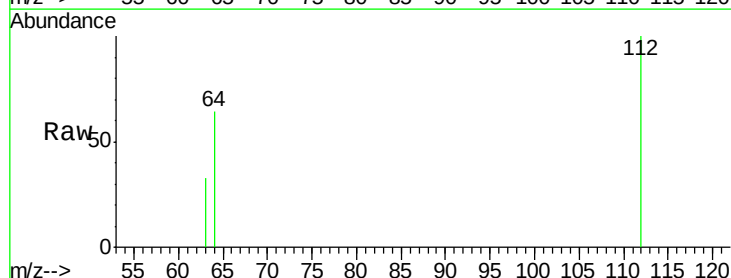


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

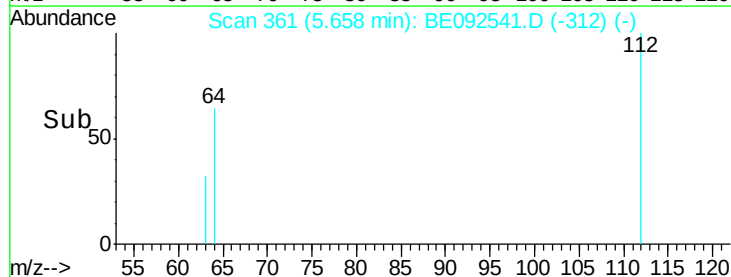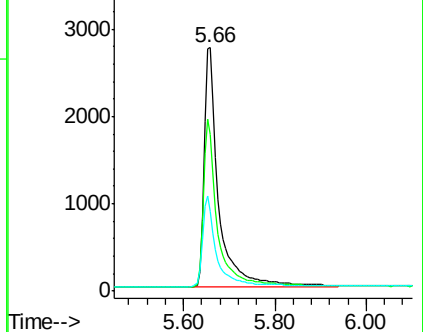

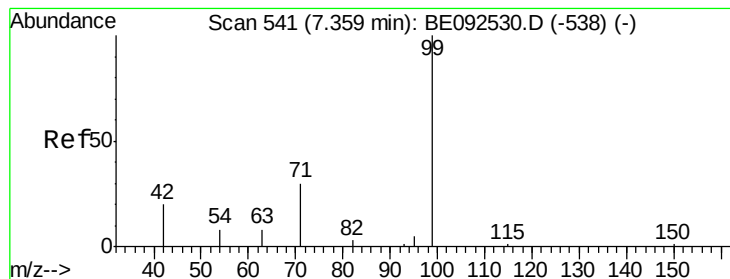

#5

Phenol-d6

Concen: 2.42 ng

RT: 7.31 min Scan# 539

Delta R.T. -0.04 min

Lab File: BE092541.D

Acq: 16 Nov 2016 19:42

Instrument :

BNA_E

ClientSampleId :

CPS043041


Tot Ion: 99 Resp: 5046

Ion Ratio Lower Upper

99 100

42 26.5 16.0 24.0#




71 36.9 30.6 45.8

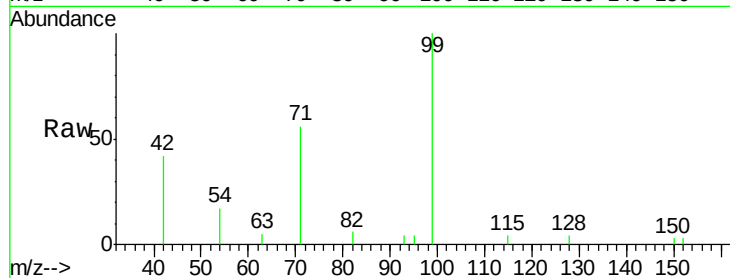

Abundance Ion 99.00 (98.70 to 99.70): BE092530.D (-538) (-)

Ion 42.00 (41.70 to 42.70): BE092530.D (-538) (-)

Ion 71.00 (70.70 to 71.70): BE092530.D (-538) (-)

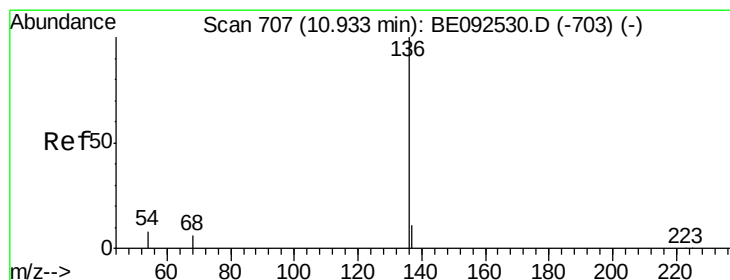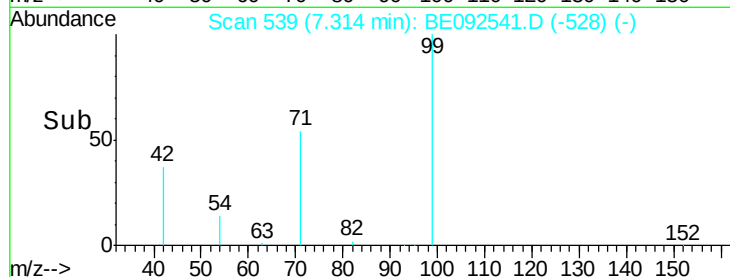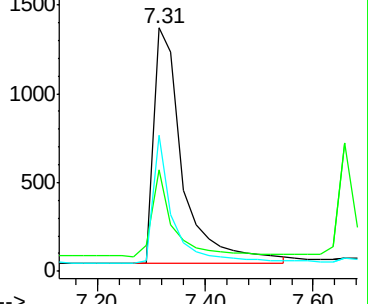

#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.93 min Scan# 707

Delta R.T. -0.00 min

Lab File: BE092541.D

Acq: 16 Nov 2016 19:42

Tgt Ion: 136 Resp: 34059


Ion Ratio Lower Upper

136 100

137 10.9 8.2 12.4

54 9.4 9.6 14.4#

68 6.6 6.7 10.1#


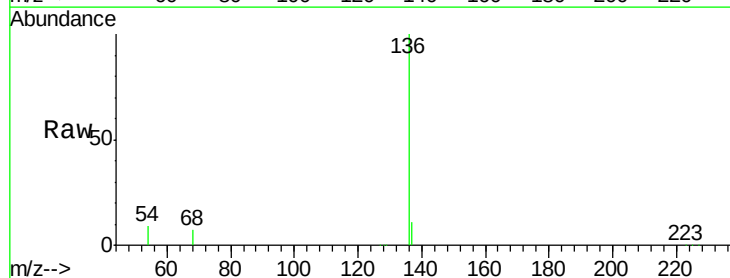



Abundance Ion 136.00 (135.70 to 136.70): BE092530.D (-703) (-)

Ion 137.00 (136.70 to 137.70): BE092530.D (-703) (-)

Ion 54.00 (53.70 to 54.70): BE092530.D (-703) (-)

Ion 68.00 (67.70 to 68.70): BE092530.D (-703) (-)

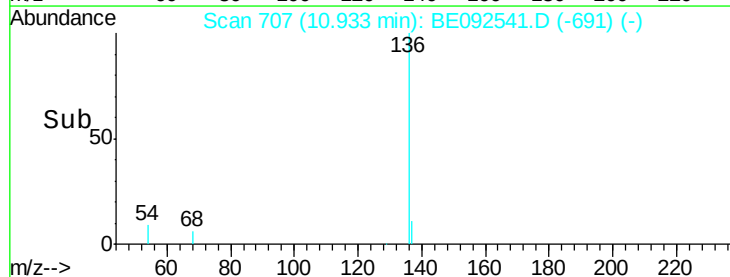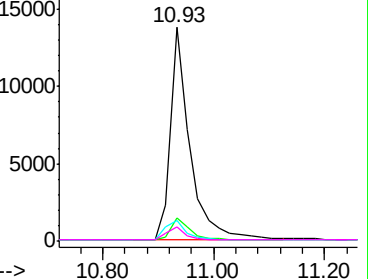

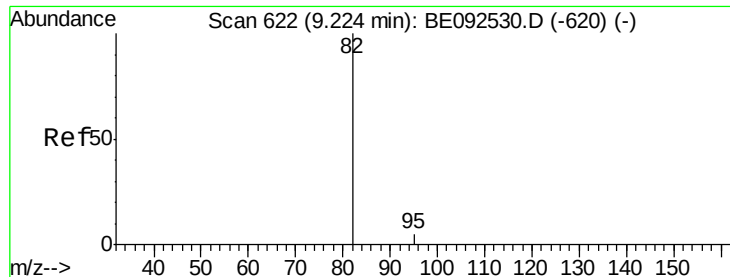

#8

Nitrobenzene-d5

Concen: 4.49 ng

RT: 9.34 min Scan# 627

Delta R.T. -0.02 min

Lab File: BE092541.D

Acq: 16 Nov 2016 19:42

Instrument :

BNA_E

ClientSampleId :

CPS043041


Tot Ion: 82 Resp: 9916

Ion Ratio Lower Upper

82 100

128 45.7 39.0 58.4




54 50.2 44.8 67.2

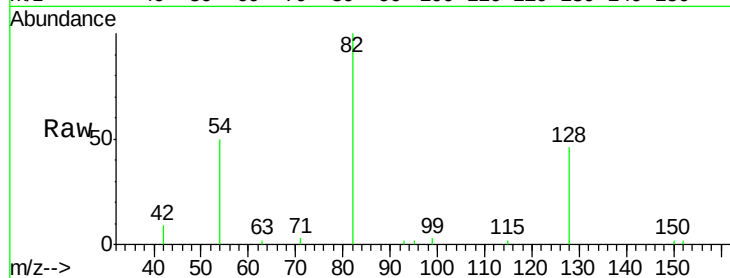

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

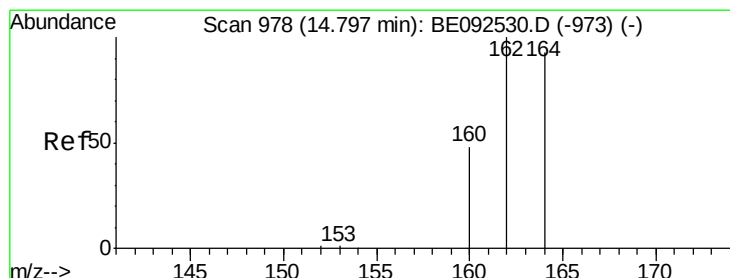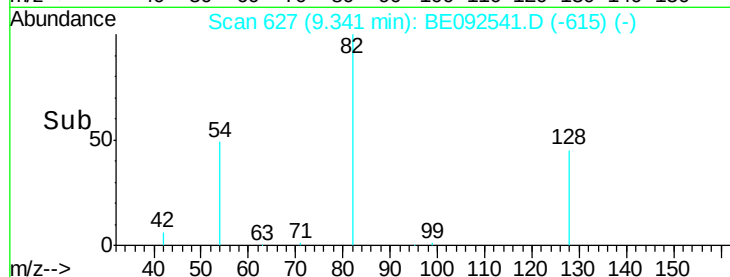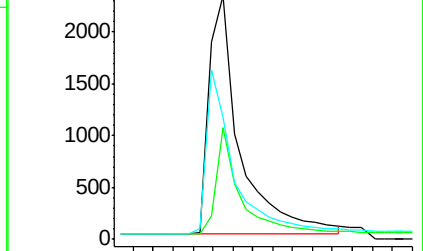

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.80 min Scan# 979

Delta R.T. 0.00 min

Lab File: BE092541.D

Acq: 16 Nov 2016 19:42


Tgt Ion: 164 Resp: 23755

Ion Ratio Lower Upper

164 100

162 100.0 71.4 107.0



160 43.4 27.4 41.2#

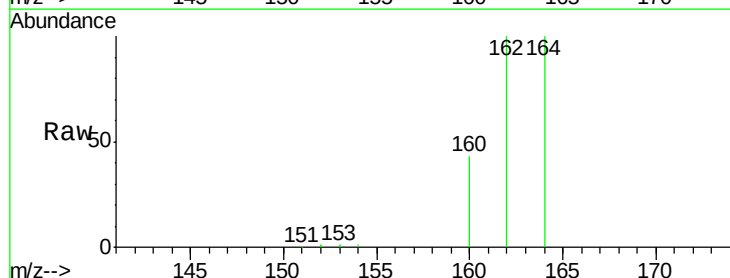


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



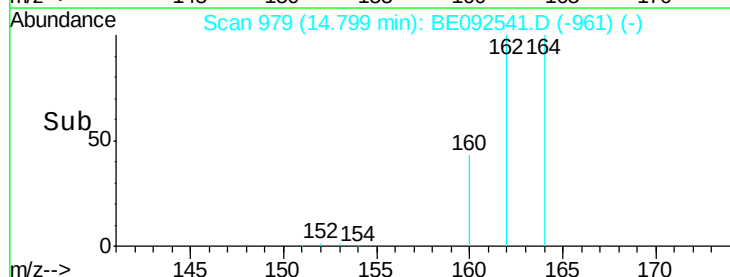
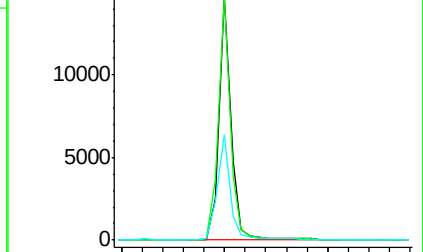


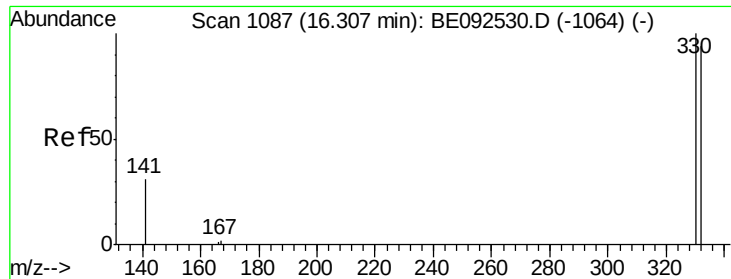

#13
 2,4,6-Tribromophenol
 Concen: 10.73 ng
 RT: 16.30 min Scan# 1087
 Delta R.T. -0.01 min
 Lab File: BE092541.D
 Acq: 16 Nov 2016 19:42




Instrument :
 BNA_E
 ClientSampleId :
 CPS043041


Tot Ion:330 Resp: 5716
 Ion Ratio Lower Upper
 330 100
 332 97.1 75.4 113.0
 141 43.8 31.0 46.6

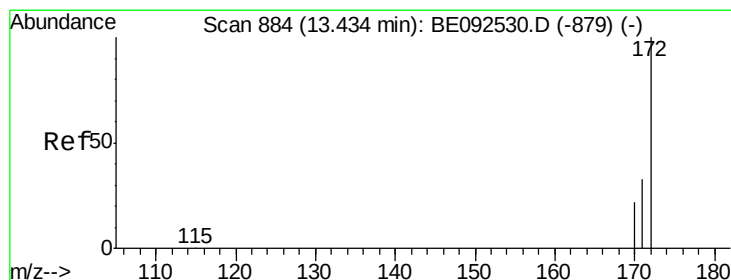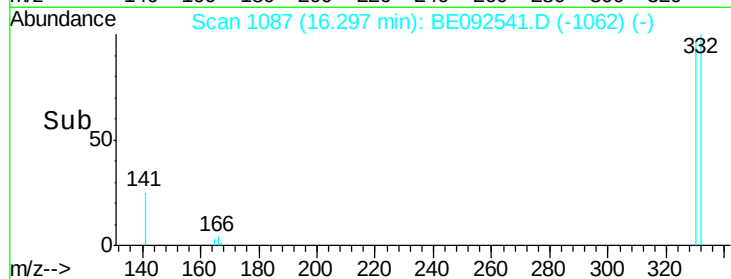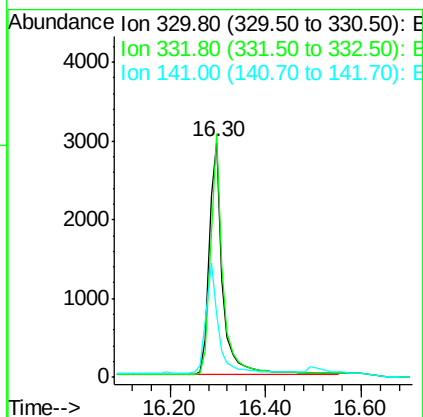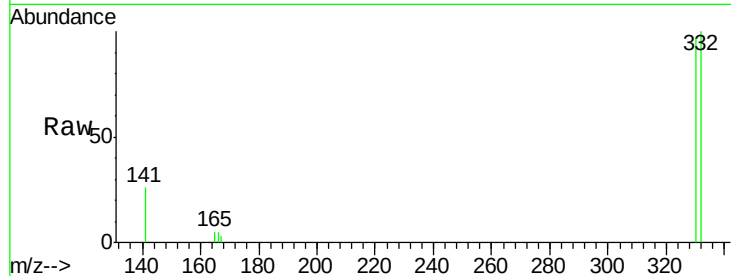

#14
 2-Fluorobiphenyl
 Concen: 4.65 ng
 RT: 13.42 min Scan# 883
 Delta R.T. -0.01 min
 Lab File: BE092541.D
 Acq: 16 Nov 2016 19:42

Tgt Ion:172 Resp: 26903
 Ion Ratio Lower Upper
 172 100
 171 33.4 30.1 45.1
 170 22.1 21.8 32.6

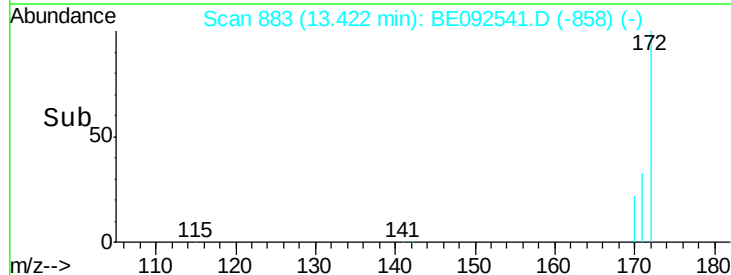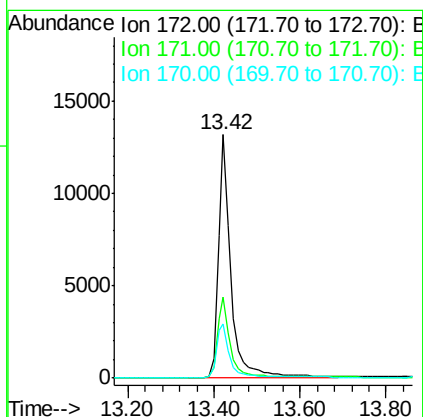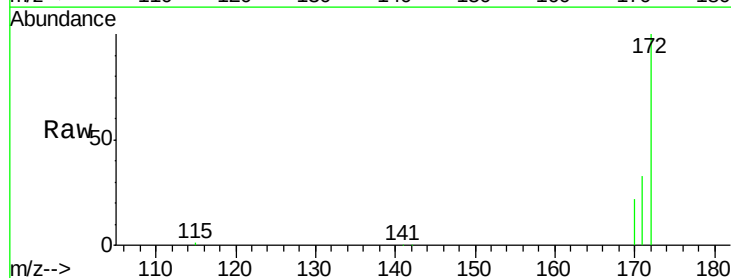

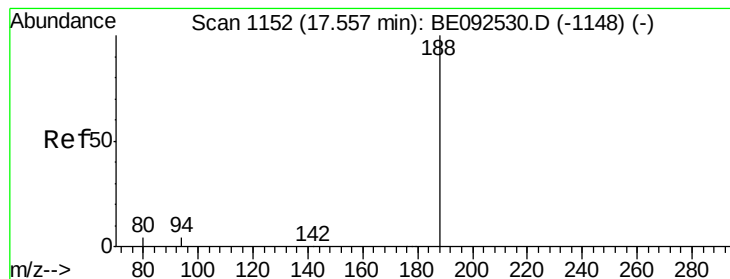

#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.56 min Scan# 1153

Delta R.T. -0.00 min

Lab File: BE092541.D

Acq: 16 Nov 2016 19:42

Instrument :

BNA_E

ClientSampleId :

CPS043041


Tot Ion:188 Resp: 53087

Ion Ratio Lower Upper

188 100

94 5.3 3.2 4.8#




80 4.8 2.6 3.8#

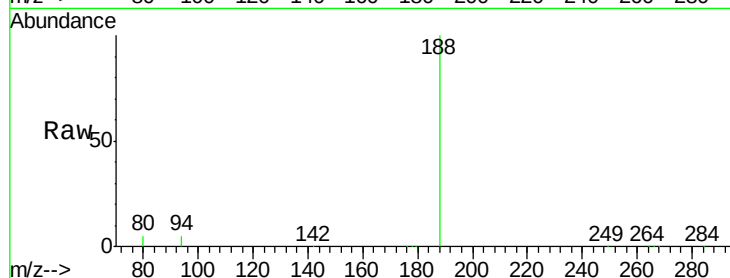

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

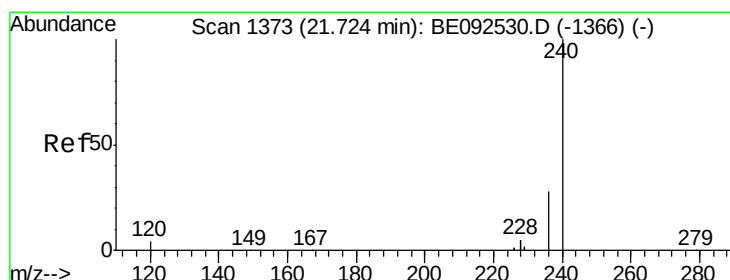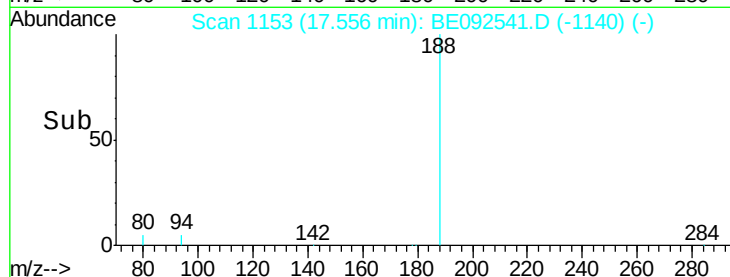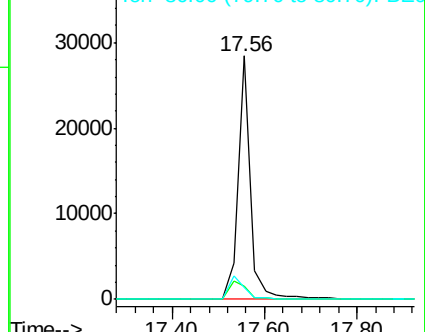

#24

Chrysene-d12

Concen: 5.00 ng

RT: 21.72 min Scan# 1374

Delta R.T. -0.00 min

Lab File: BE092541.D

Acq: 16 Nov 2016 19:42


Tgt Ion:240 Resp: 79441

Ion Ratio Lower Upper

240 100

120 2.9 2.6 4.0



236 27.9 24.6 37.0

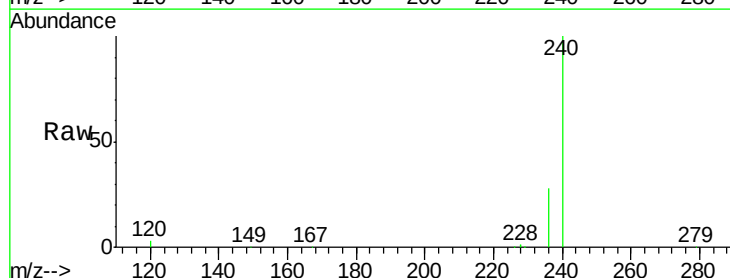


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



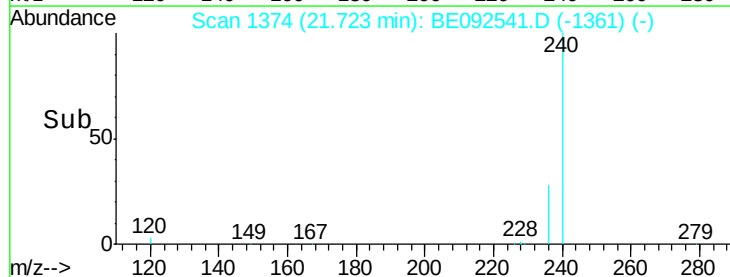
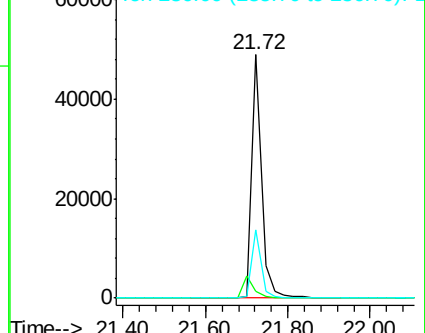


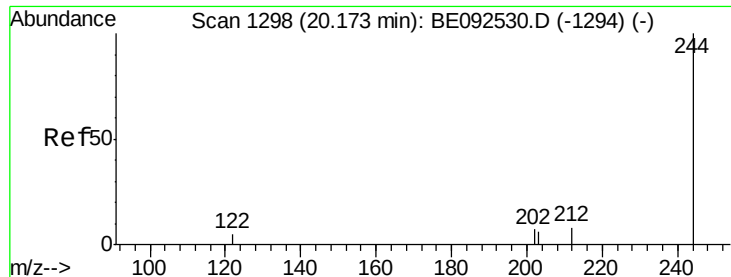

#26
 Terphenyl-d14
 Concen: 5.54 ng
 RT: 20.16 min Scan# 1298
 Delta R.T. -0.02 min
 Lab File: BE092541.D
 Acq: 16 Nov 2016 19:42




Instrument :
 BNA_E
 ClientSampleID :
 CPS043041




Tot Ion:244 Resp: 50281
 Ion Ratio Lower Upper
 244 100
 212 8.3 6.7 10.1
 122 4.9 3.6 5.4

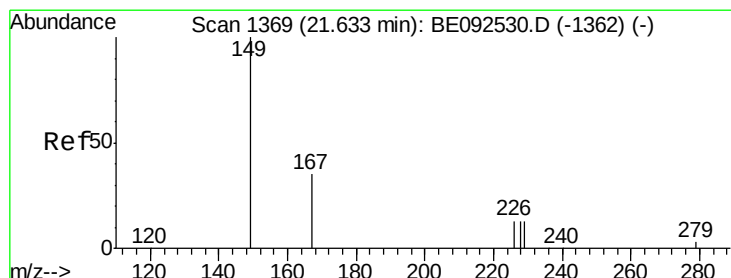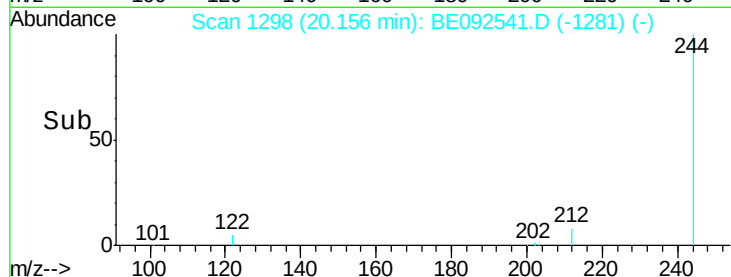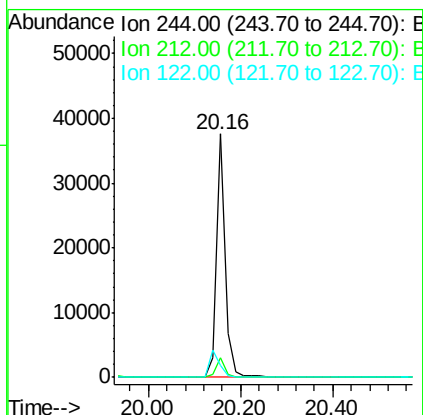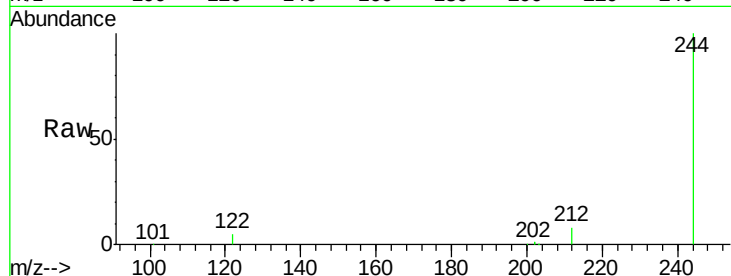

#29
 Bis(2-ethylhexyl)phthalate
 Concen: 0.48 ng
 RT: 21.61 min Scan# 1369
 Delta R.T. -0.02 min
 Lab File: BE092541.D
 Acq: 16 Nov 2016 19:42

Tgt Ion:149 Resp: 1884
 Ion Ratio Lower Upper
 149 100
 167 23.2 16.0 24.0
 279 0.0 16.0 24.0#

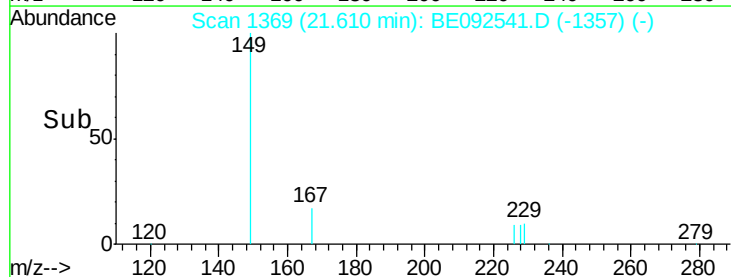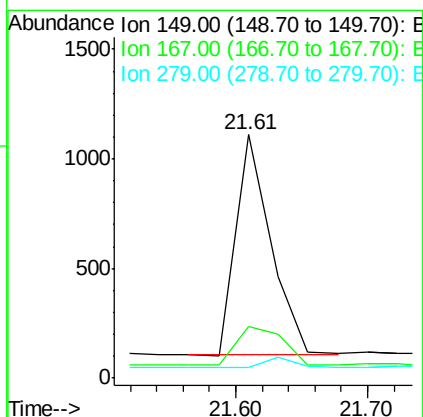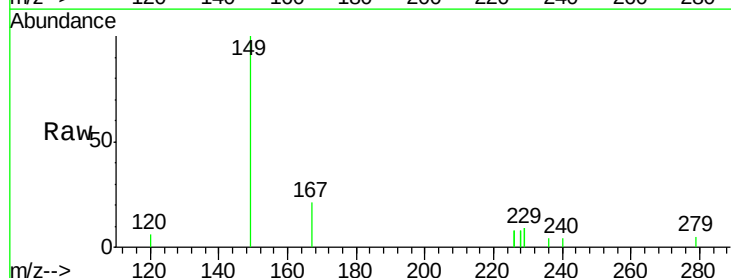

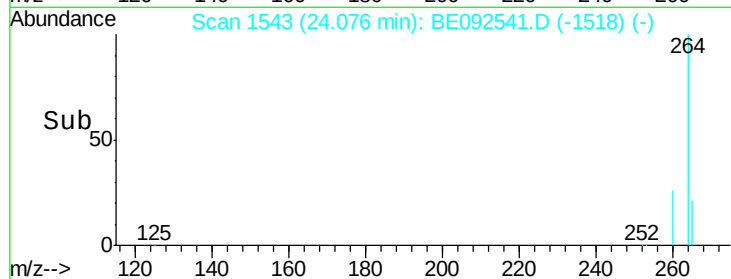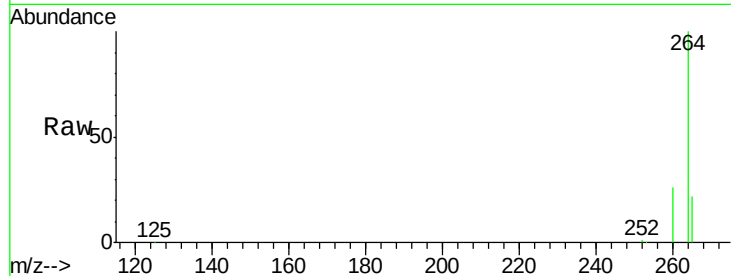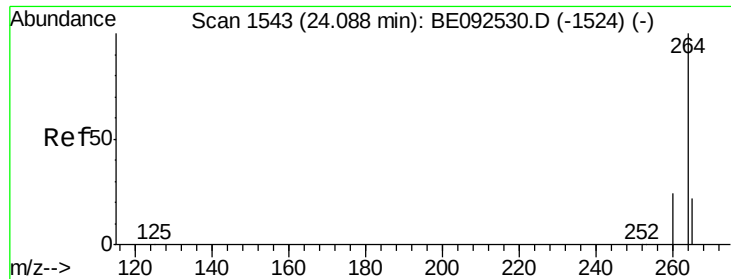

#31

Pervlene-d12

Concen: 5.00 ng

RT: 24.08 min Scan# 1543

Delta R.T. -0.01 min

Lab File: BE092541.D

Acq: 16 Nov 2016 19:42

Instrument :

BNA_E

ClientSampleId :

CPS043041

Tot Ion: 264 Resp: 68226

Ion Ratio Lower Upper

264 100

260 25.7 20.1 30.1

265 21.6 17.9 26.9

