


Data Path : Z:\HPCHEM1\BNA E\DATA\BE111616\
 Data File : BE092526.D
 Acq On : 16 Nov 2016 9:06
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 16 15:43:18 2016

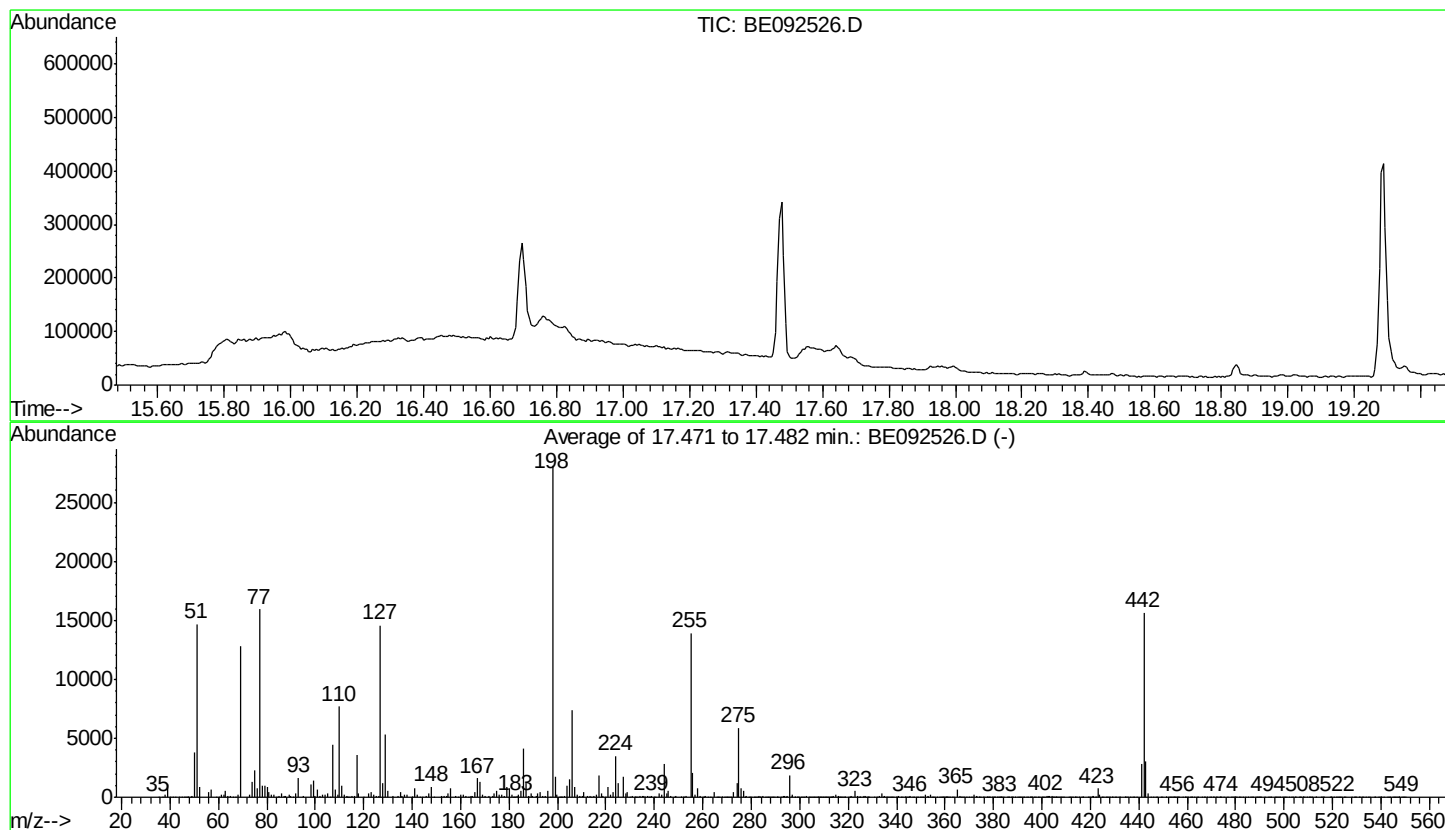

AutoFind: Scans 2533, 2534, 2535; Background Corrected with Scan 2524

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.1	14650	PASS
68	69	0.00	2	1.9	246	PASS
69	198	0.00	100	45.5	12795	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.7	14544	PASS
197	198	0.00	2	0.1	28	PASS
198	198	100	100	100.0	28106	PASS
199	198	5	9	6.1	1707	PASS
275	198	10	60	20.8	5860	PASS
365	198	1	100	2.4	664	PASS
441	442	0.01	24	17.8	2787	PASS
442	198	50	100	55.8	15677	PASS
443	442	15	24	19.5	3053	PASS