
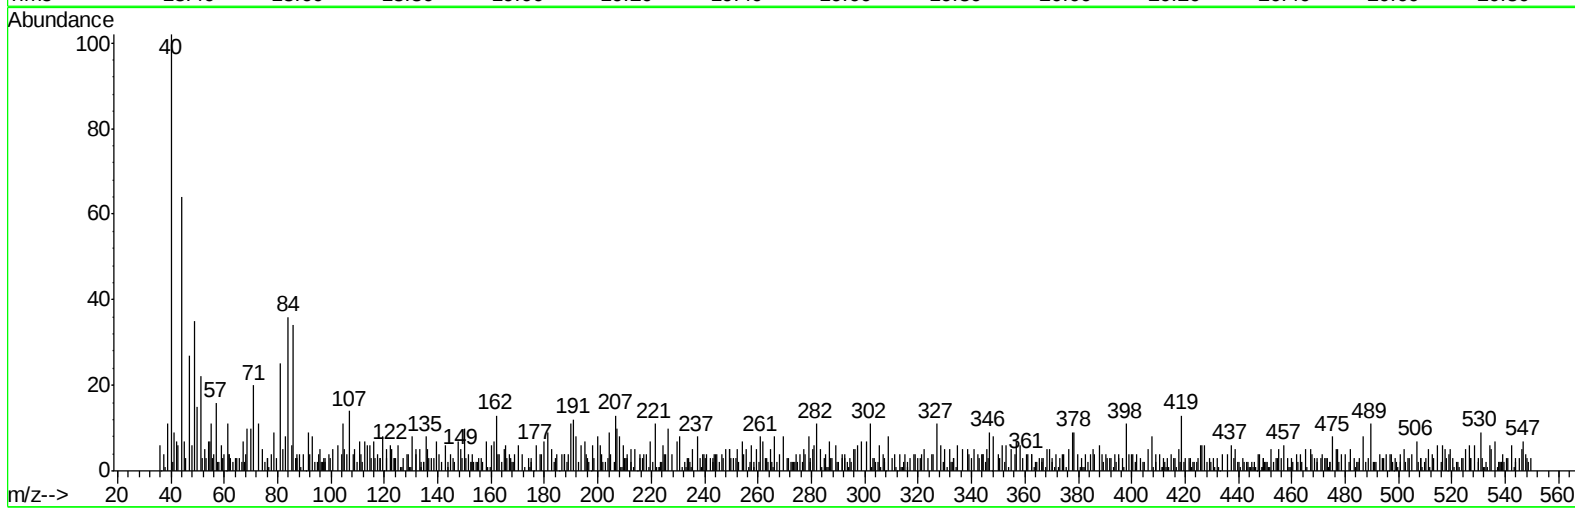


Data Path : Z:\HPCHEM1\BNA E\DATA\BE111617\
Data File : BE094817.D
Acq On : 15 Nov 2017 16:34
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 03:04:14 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 13:27:38 2017
Response via : Initial Calibration

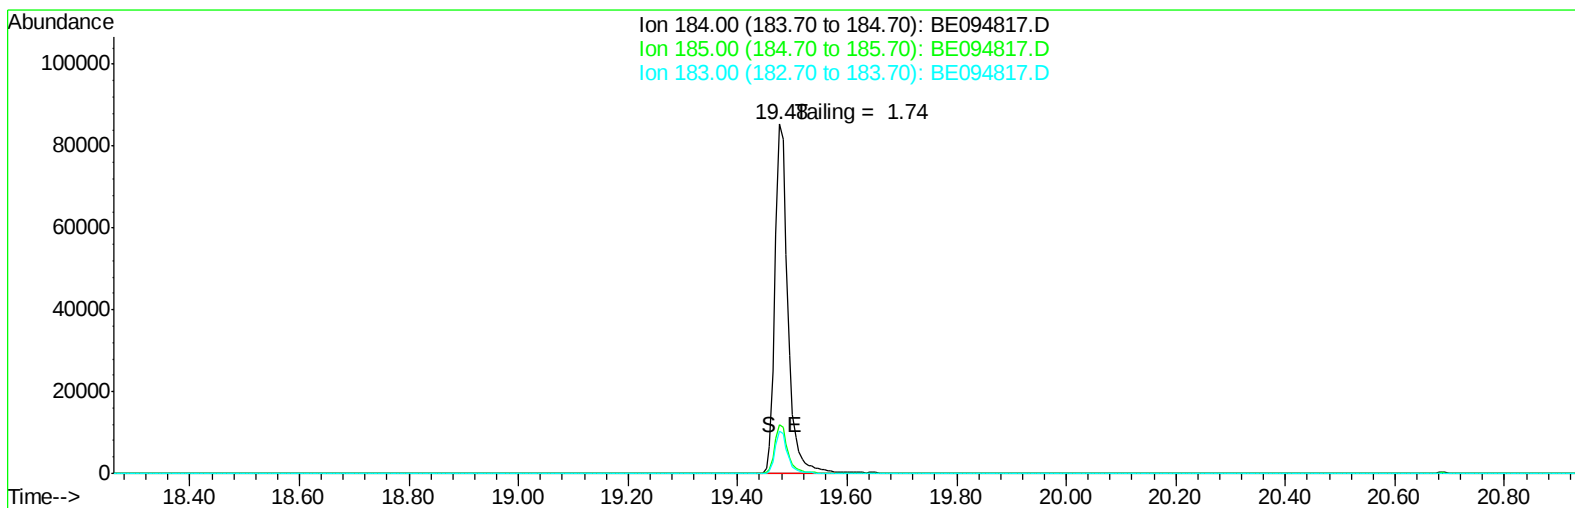

TIC: BE094817.D

(76) Benzidine



12.643min (-0.102) 42.81ng

response 12

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	0.00#
183.00	11.60	100.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111617\
Data File : BE094817.D
Acq On : 15 Nov 2017 16:34
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 03:04:14 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 13:27:38 2017
Response via : Initial Calibration

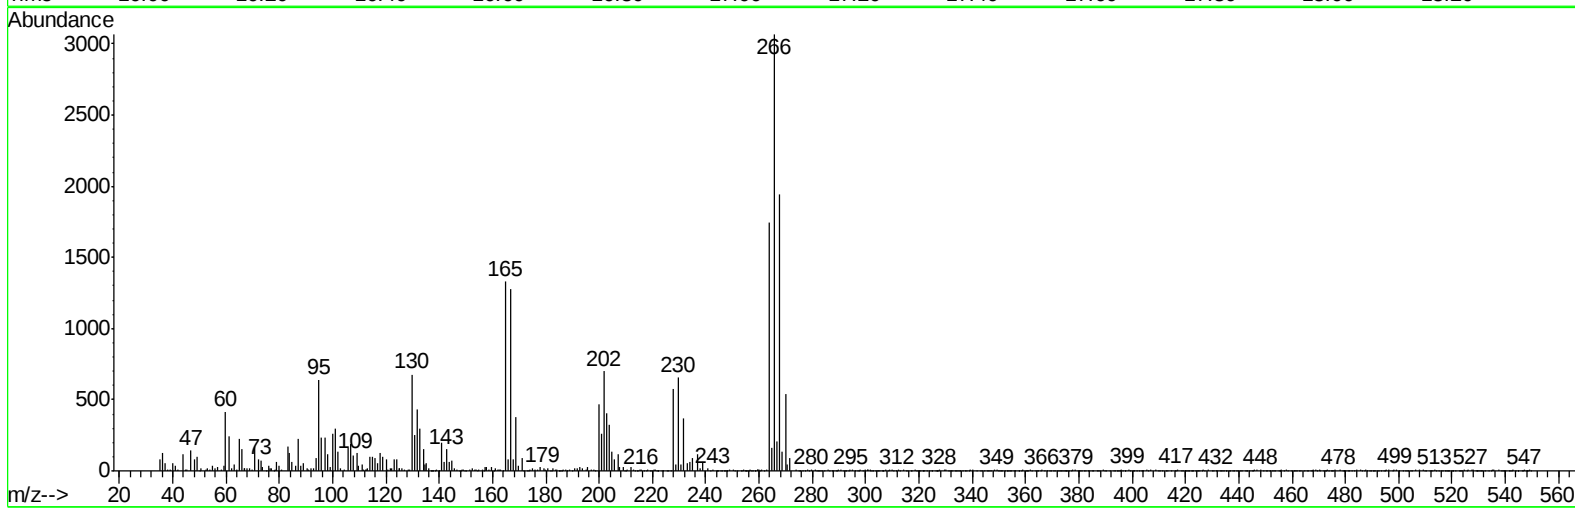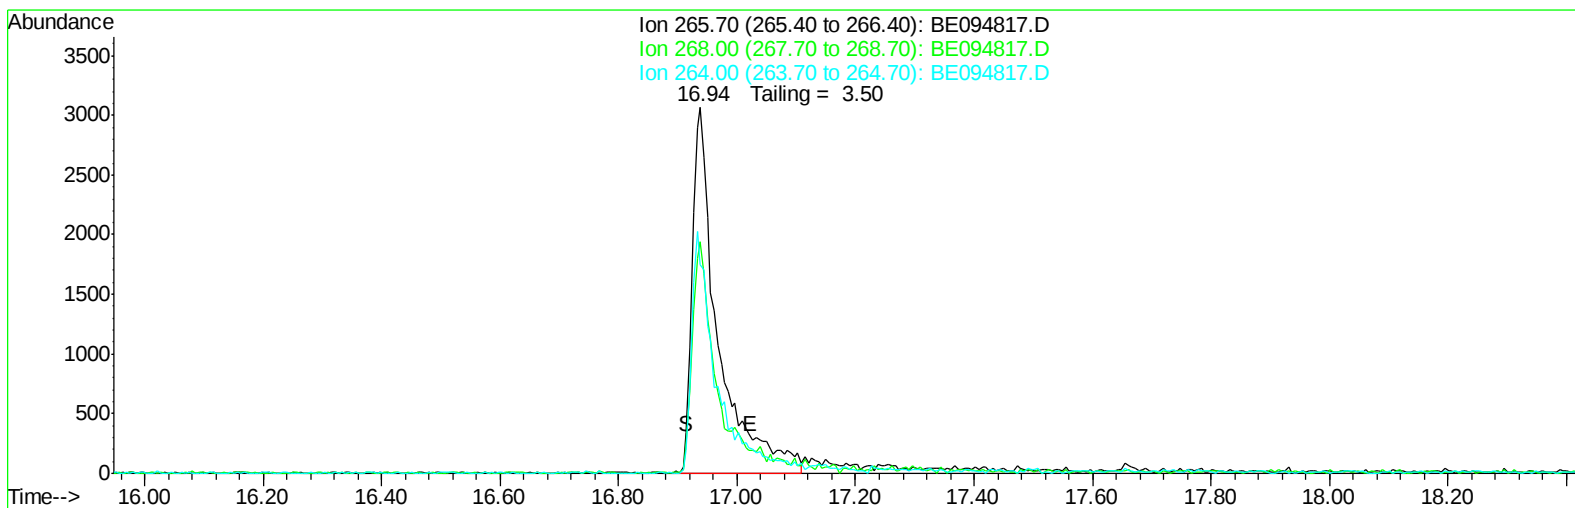

TIC: BE094817.D

(69) Pentachlorophenol (C)

16.938min (+5.729) 72611.00ng m

response 9340

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.38
264.00	61.90	56.83
0.00	0.00	0.00