


Data Path : Z:\HPCHEM1\BNA_E\Data\BE111617\
 Data File : BE094817.D
 Acq On : 15 Nov 2017 16:34
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 23 22:40:47 2017

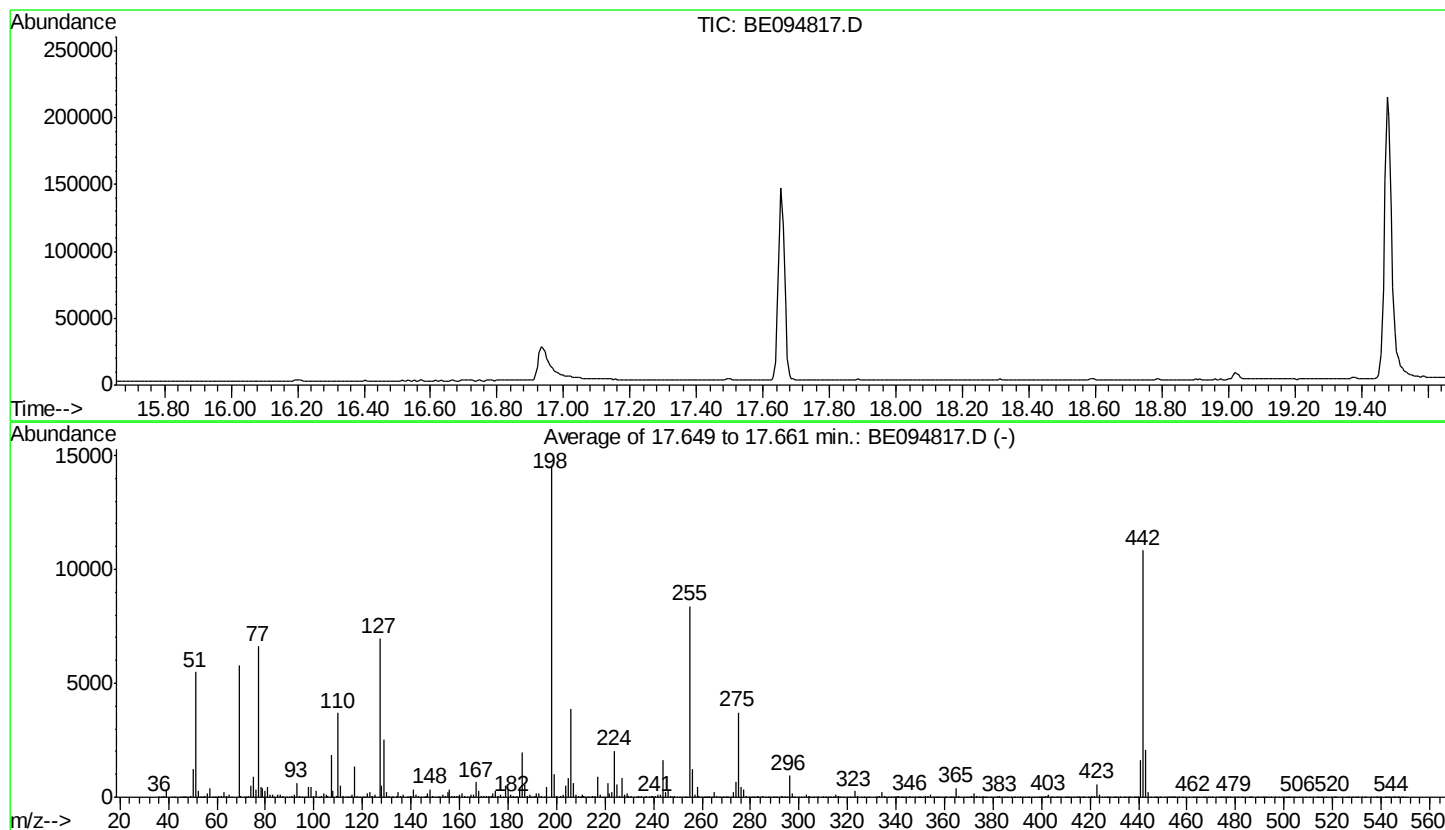

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	5479	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.7	5777	PASS
70	69	0.00	2	0.6	37	PASS
127	198	10	80	47.7	6939	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14548	PASS
199	198	5	9	6.9	998	PASS
275	198	10	60	25.5	3708	PASS
365	198	1	100	2.9	421	PASS
441	442	0.01	24	15.2	1645	PASS
442	198	50	100	74.4	10826	PASS
443	442	15	24	19.0	2056	PASS