

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111715\
 Data File : BE091196.D
 Acq On : 17 Nov 2015 10:02
 Operator : UM/NP
 Sample : G4309-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 18 03:29:22 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 18 03:27:44 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	4099	0.40	ng/ul	-0.03
4) Naphthalene-d8	9.56	136	20834	0.40	ng/ul	-0.02
8) Acenaphthene-d10	13.37	164	12224	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.17	188	1675333	0.40	ng/ul	0.09
18) Chrysene-d12	20.23	240	60145	0.40	ng/ul	0.00
22) Perylene-d12	22.11	264	72715	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.00	96	19341	6.56	ng/uL	-0.03
6) 2-Methylnaphthalene-d10	11.08	152	6458	0.23	ng/ul	0.00
16) Fluoranthene-d10	18.08	212	23550	0.00	ng/ul	0.00
Target Compounds						
25) Benzo(a)pyrene	21.99	252	9138	0.04	ng/ul#	Ovalue 34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111715\
Data File : BE091196.D
Acq On : 17 Nov 2015 10:02
Operator : UM/NP
Sample : G4309-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 18 03:29:22 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 18 03:27:44 2015
Response via : Initial Calibration

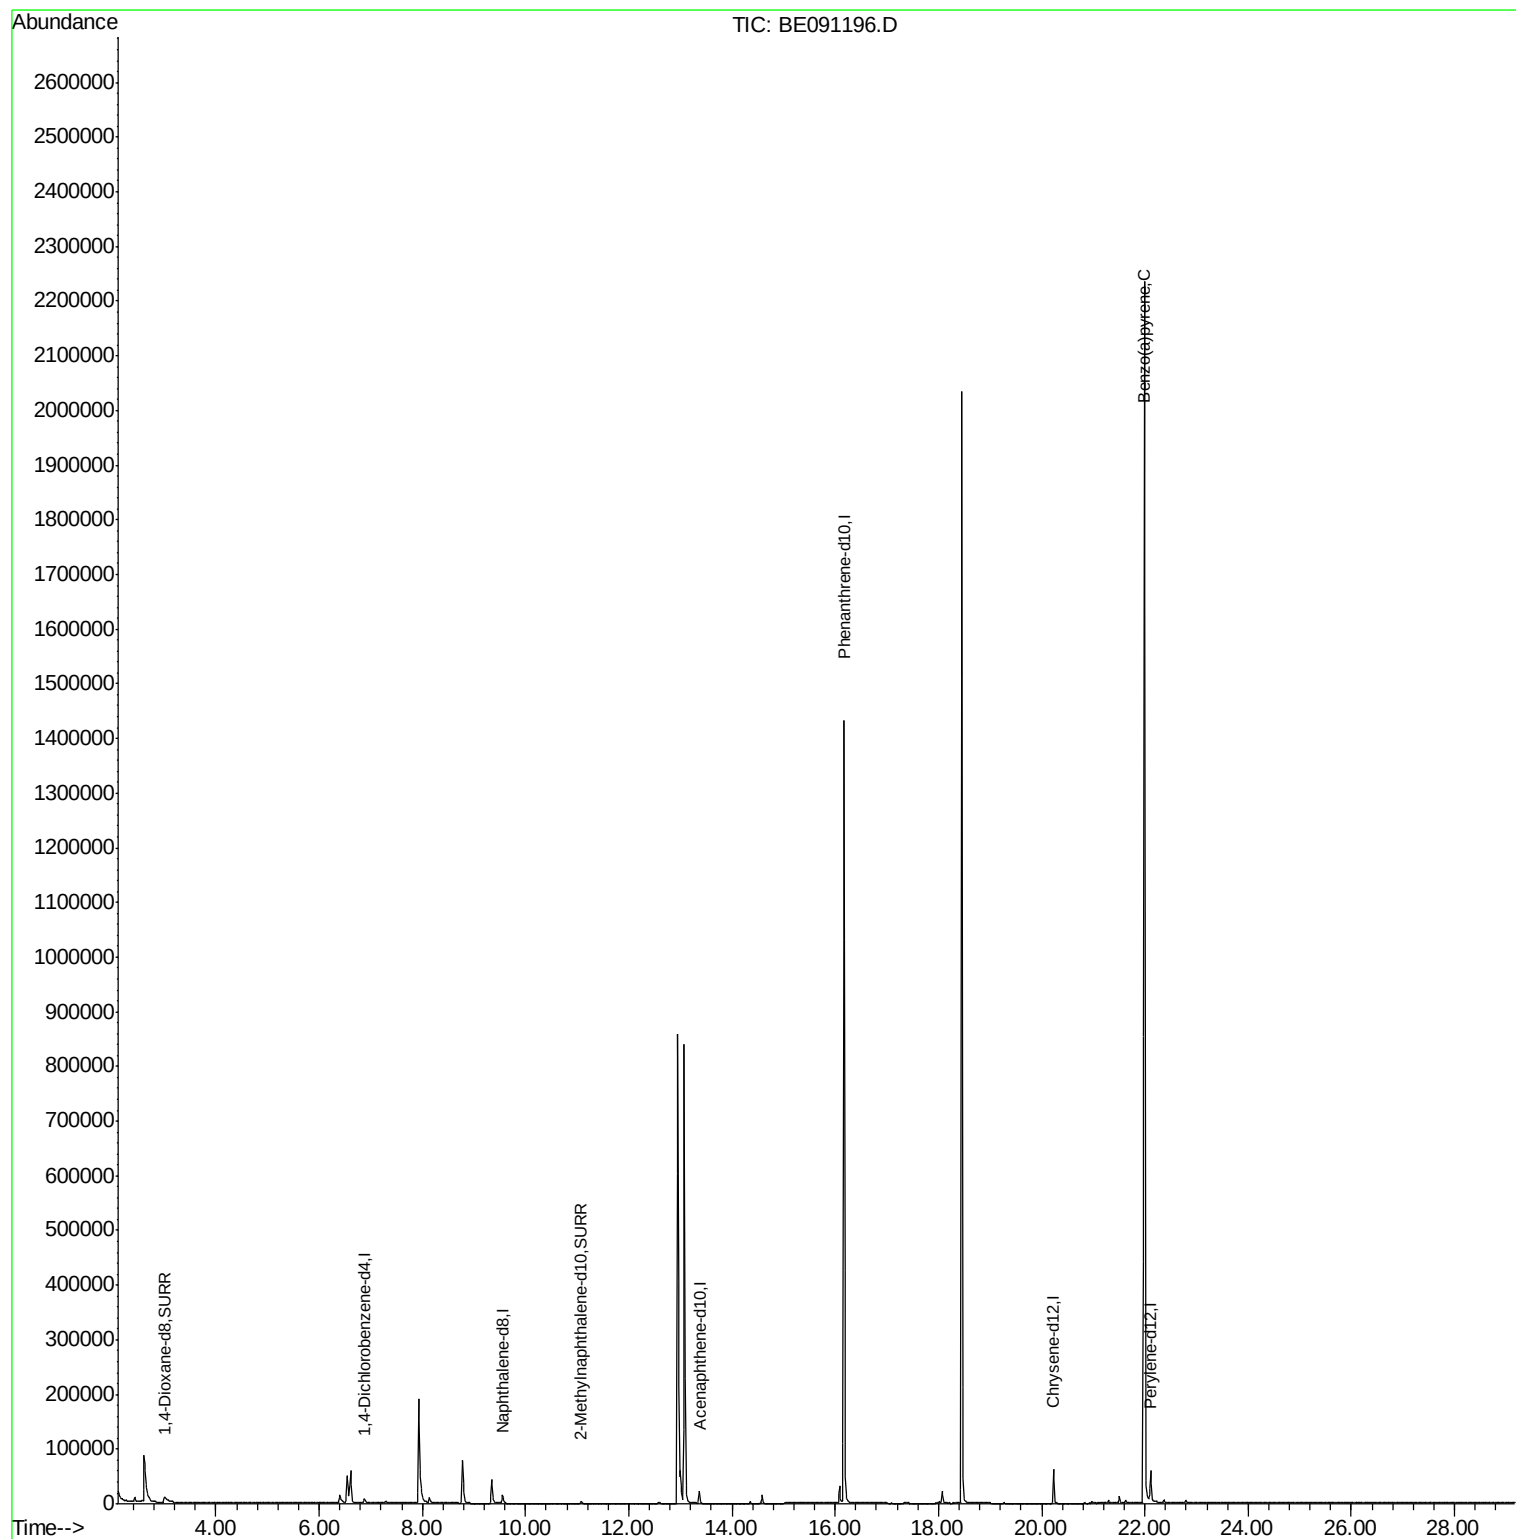

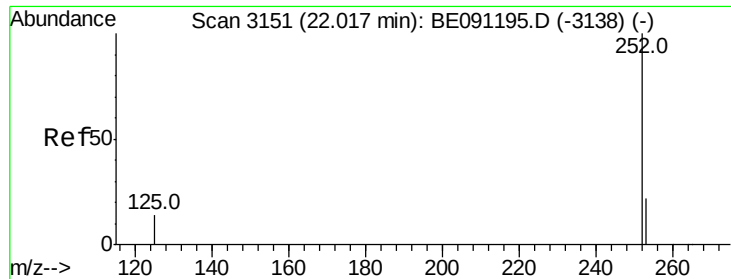

#25

Benzo(a)pyrene

Concen: 0.04 ng/ul

RT: 21.99 min Scan# 3145

Delta R.T. -0.03 min

Lab File: BE091196.D

Acq: 17 Nov 2015 10:02

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 9138

Ion Ratio Lower Upper

252 100

253 38.3 21.8 32.8#

125 76.8 14.5 21.7#

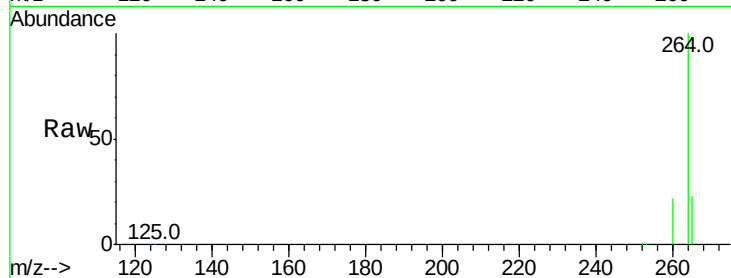

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

