

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111715\
 Data File : BE091197.D
 Acq On : 17 Nov 2015 10:38
 Operator : UM/NP
 Sample : G4309-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 18 03:29:26 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 18 03:27:44 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	3766	0.40	ng/ul	-0.02
4) Naphthalene-d8	9.57	136	18922	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.37	164	11179	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.17	188	1314542	0.40	ng/ul	0.09
18) Chrysene-d12	20.23	240	73855	0.40	ng/ul	0.00
22) Perylene-d12	22.11	264	71432	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.08	96	3675	1.36	ng/uL	0.05
6) 2-Methylnaphthalene-d10	11.08	152	2914	0.11	ng/ul	0.00
16) Fluoranthene-d10	18.07	212	19283	0.01	ng/ul	0.00
Target Compounds						
25) Benzo(a)pyrene	21.99	252	6895	0.03	ng/ul#	Ovalue 13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111715\
Data File : BE091197.D
Acq On : 17 Nov 2015 10:38
Operator : UM/NP
Sample : G4309-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 18 03:29:26 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 18 03:27:44 2015
Response via : Initial Calibration

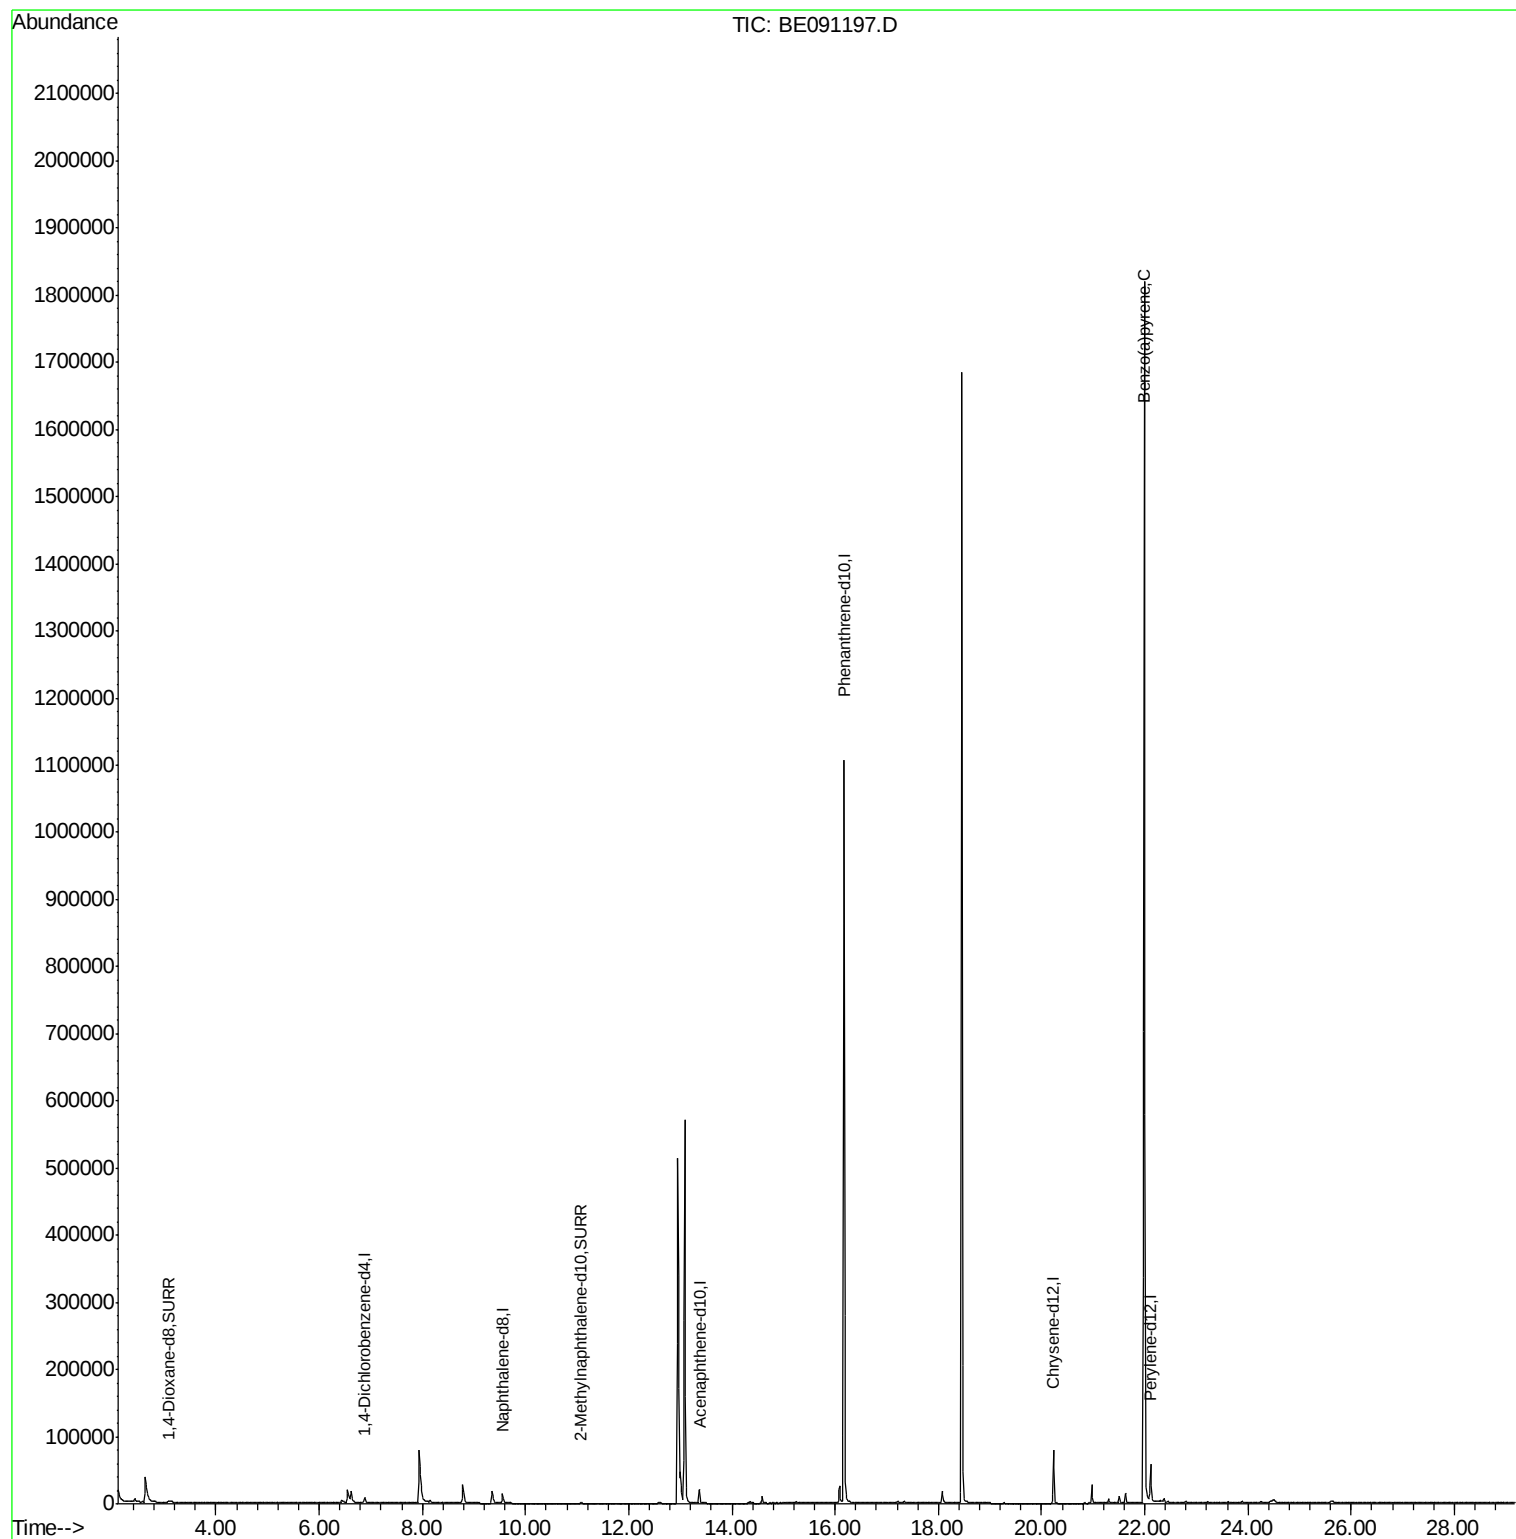

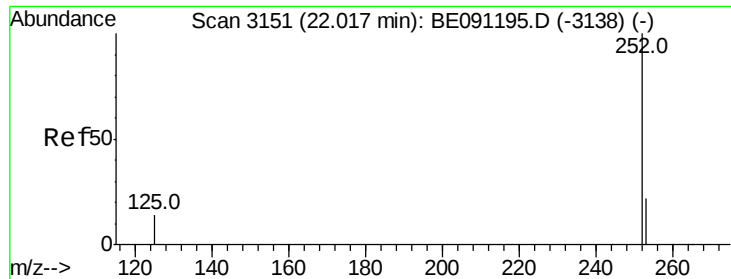

#25

Benzo(a)pyrene

Concen: 0.03 ng/ul

RT: 21.99 min Scan# 3145

Delta R.T. -0.03 min


Lab File: BE091197.D

Acq: 17 Nov 2015 10:38

Instrument :

BNA_E

ClientSampleId :

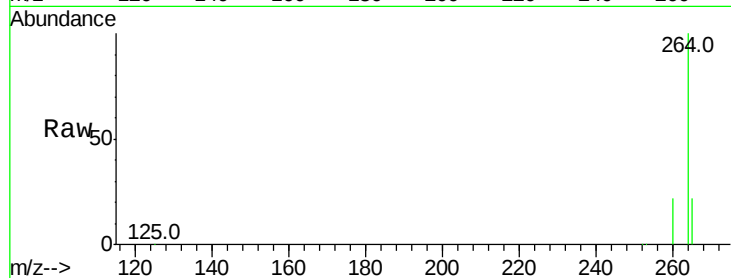

Tot Ion: 252 Resp: 6895

Ion Ratio Lower Upper

252 100

253 39.6 21.8 32.8#

125 98.8 14.5 21.7#

