

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111715\
 Data File : BE091200.D
 Acq On : 17 Nov 2015 12:29
 Operator : UM/NP
 Sample : G4309-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 18 03:29:41 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 18 03:27:44 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	3877	0.40	ng/ul	-0.03
4) Naphthalene-d8	9.56	136	20442	0.40	ng/ul	-0.02
8) Acenaphthene-d10	13.36	164	13110	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.17	188	1541873	0.40	ng/ul	0.09
18) Chrysene-d12	20.23	240	65852	0.40	ng/ul	0.00
22) Perylene-d12	22.11	264	76138	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.00	96	17657	6.33	ng/uL	-0.03
6) 2-Methylnaphthalene-d10	11.07	152	6783	0.24	ng/ul	0.00
16) Fluoranthene-d10	18.07	212	22911	0.01	ng/ul	0.00
Target Compounds						
25) Benzo(a)pyrene	21.99	252	8887	0.04	ng/ul#	Ovalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111715\
Data File : BE091200.D
Acq On : 17 Nov 2015 12:29
Operator : UM/NP
Sample : G4309-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 18 03:29:41 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 18 03:27:44 2015
Response via : Initial Calibration

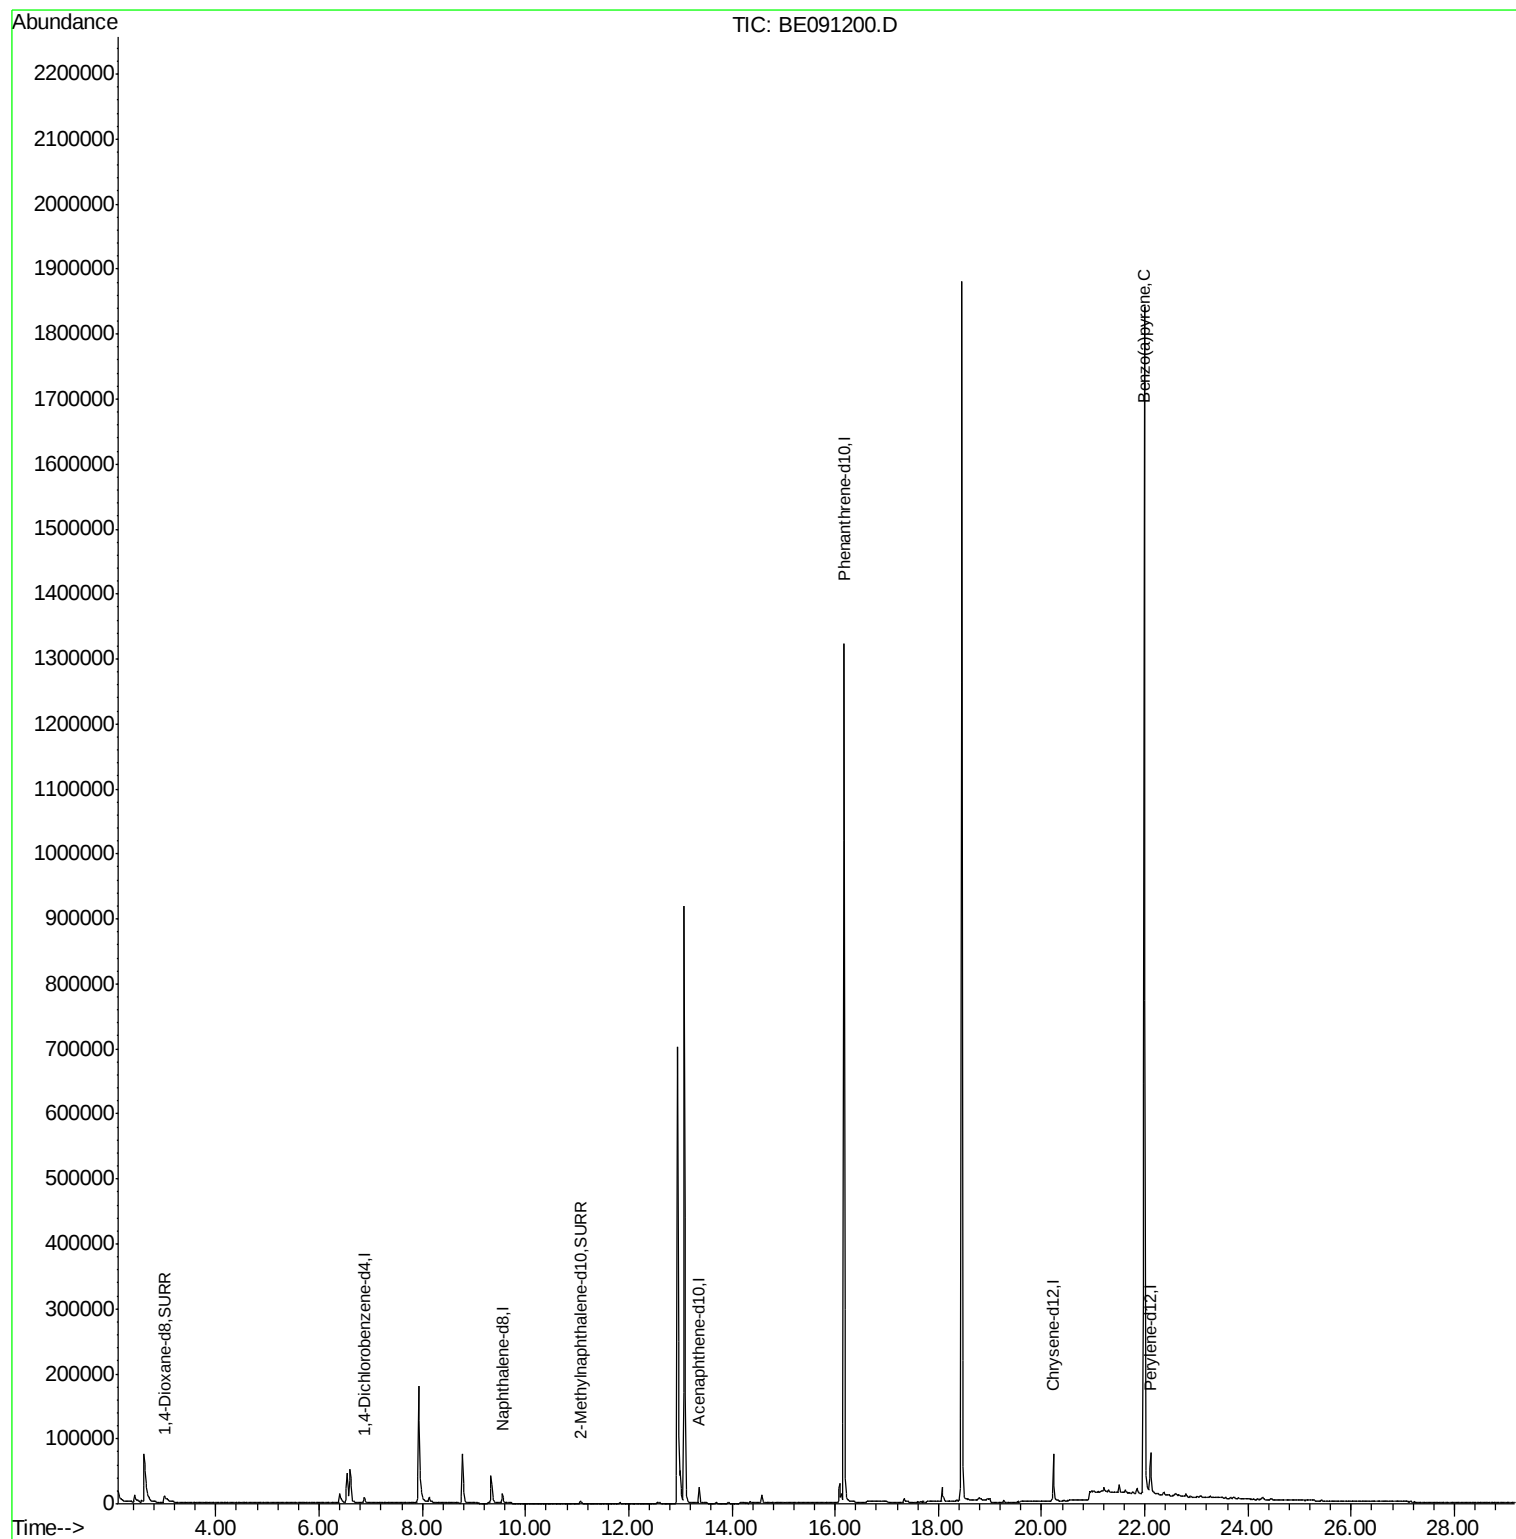

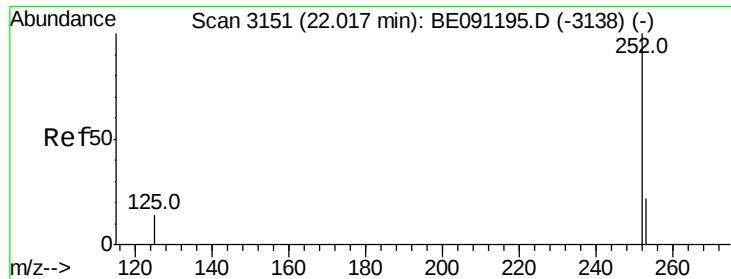

#25

Benzo(a)pyrene

Concen: 0.04 ng/ul

RT: 21.99 min Scan# 3145

Delta R.T. -0.03 min

Lab File: BE091200.D

Acq: 17 Nov 2015 12:29

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 8887

Ion Ratio Lower Upper

252 100

253 44.3 21.8 32.8#

125 267.8 14.5 21.7#

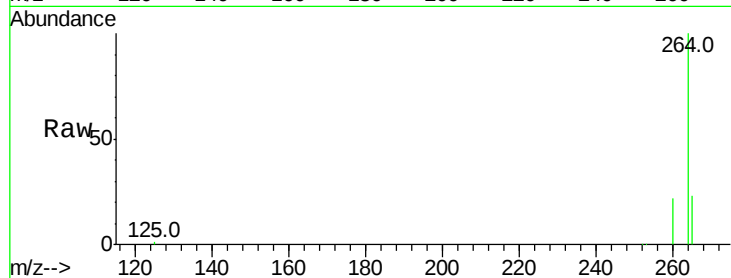

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

