

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111715\
 Data File : BE091202.D
 Acq On : 17 Nov 2015 13:40
 Operator : UM/NP
 Sample : G4309-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 D9KP2

Manual Integrations
 APPROVED

Mmdadoda
 11/19/2015 6:41:36 PM

Quant Time: Nov 19 11:51:51 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 18 03:27:44 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	3213	0.40	ng/ul	-0.03
4) Naphthalene-d8	9.55	136	16957	0.40	ng/ul	-0.03
8) Acenaphthene-d10	13.36	164	10818	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.09	188	28418m	0.40	ng/ul	0.00
18) Chrysene-d12	20.23	240	53528	0.40	ng/ul	0.00
22) Perylene-d12	22.11	264	45928m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.99	96	18440	7.98	ng/uL	-0.03
6) 2-Methylnaphthalene-d10	11.07	152	6617	0.29	ng/ul	0.00
16) Fluoranthene-d10	18.08	212	21662	0.27	ng/ul	0.00
Target Compounds						
5) Naphthalene	9.60	128	1716	0.04	ng/ul#	Qvalue 80

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111715\
Data File : BE091202.D
Acq On : 17 Nov 2015 13:40
Operator : UM/NP
Sample : G4309-19
Misc :
ALS Vial : 25 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
D9KP2

Manual Integrations
APPROVED

Mmdadoda
11/19/2015 6:41:36 PM

Quant Time: Nov 19 11:51:51 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 18 03:27:44 2015
Response via : Initial Calibration

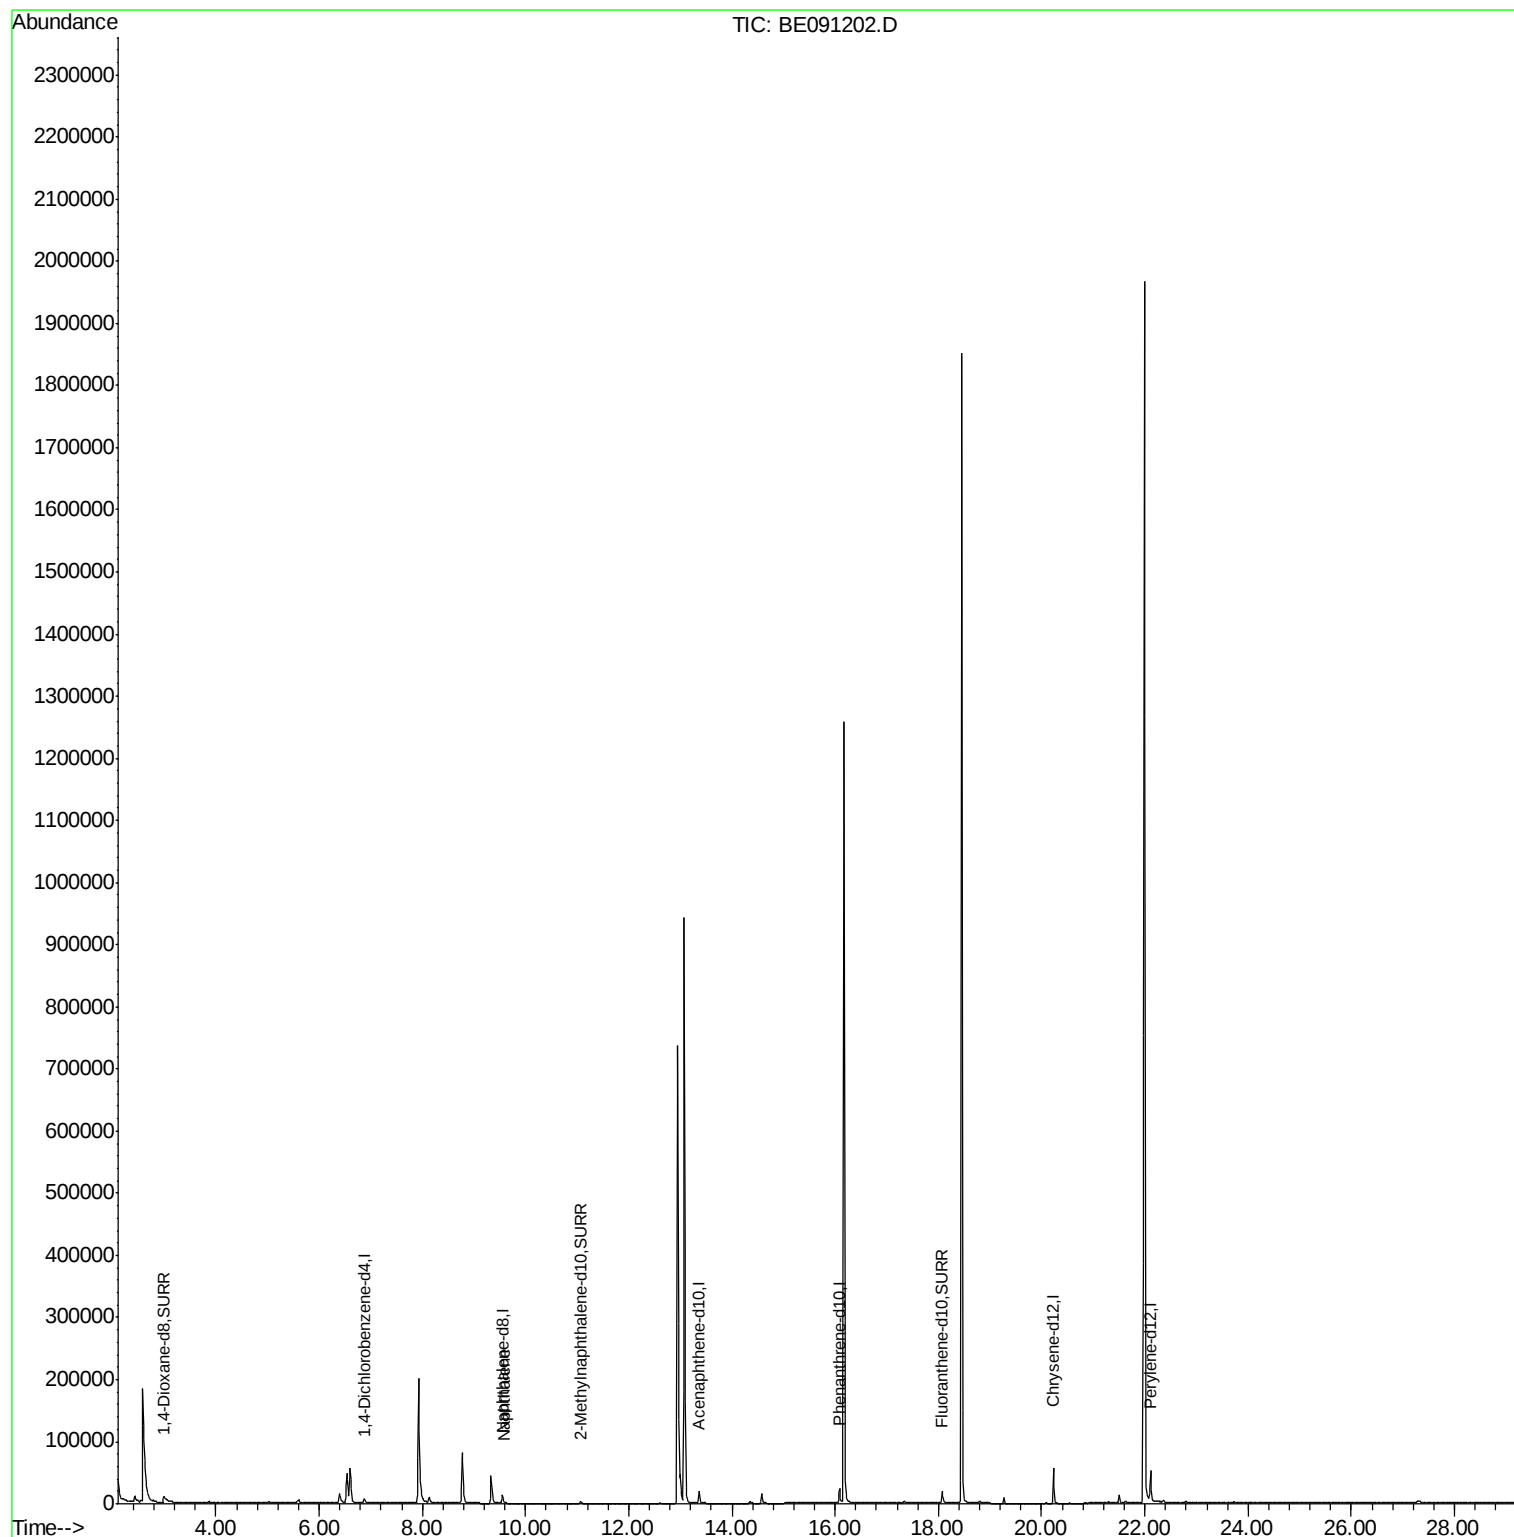

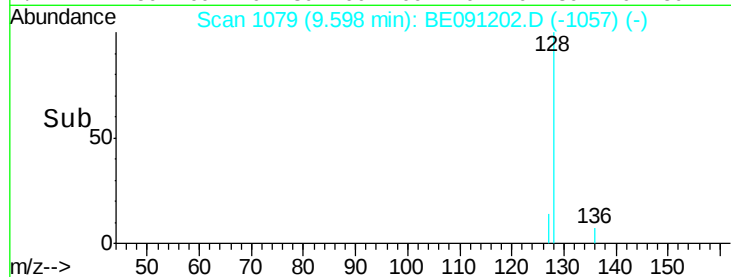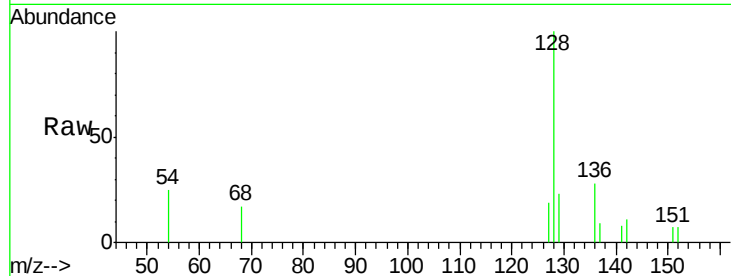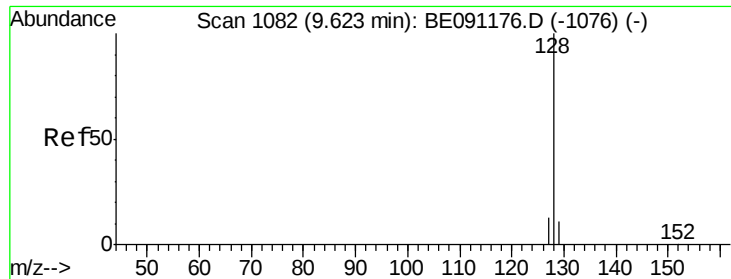

#5

Naphthalene

Concen: 0.04 ng/ul

RT: 9.60 min Scan# 1079

Delta R.T. -0.02 min

Lab File: BE091202.D

Acq: 17 Nov 2015 13:40

Tgt Ion:	128	Resp:	1716
Ion Ratio	Lower	Upper	
128	100		
129	22.5	9.8	14.8#
127	19.2	10.7	16.1#

Instrument :

BNA_E

ClientSampleId :

D9KP2

Manual Integrations
APPROVED

Mmdadoda
11/19/2015 6:41:36 PM

