


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE111715\
 Data File : BE091194.D
 Acq On : 17 Nov 2015 8:51
 Operator : UM/NP
 Sample : DFTPP79
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP79

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 19 04:25:56 2015

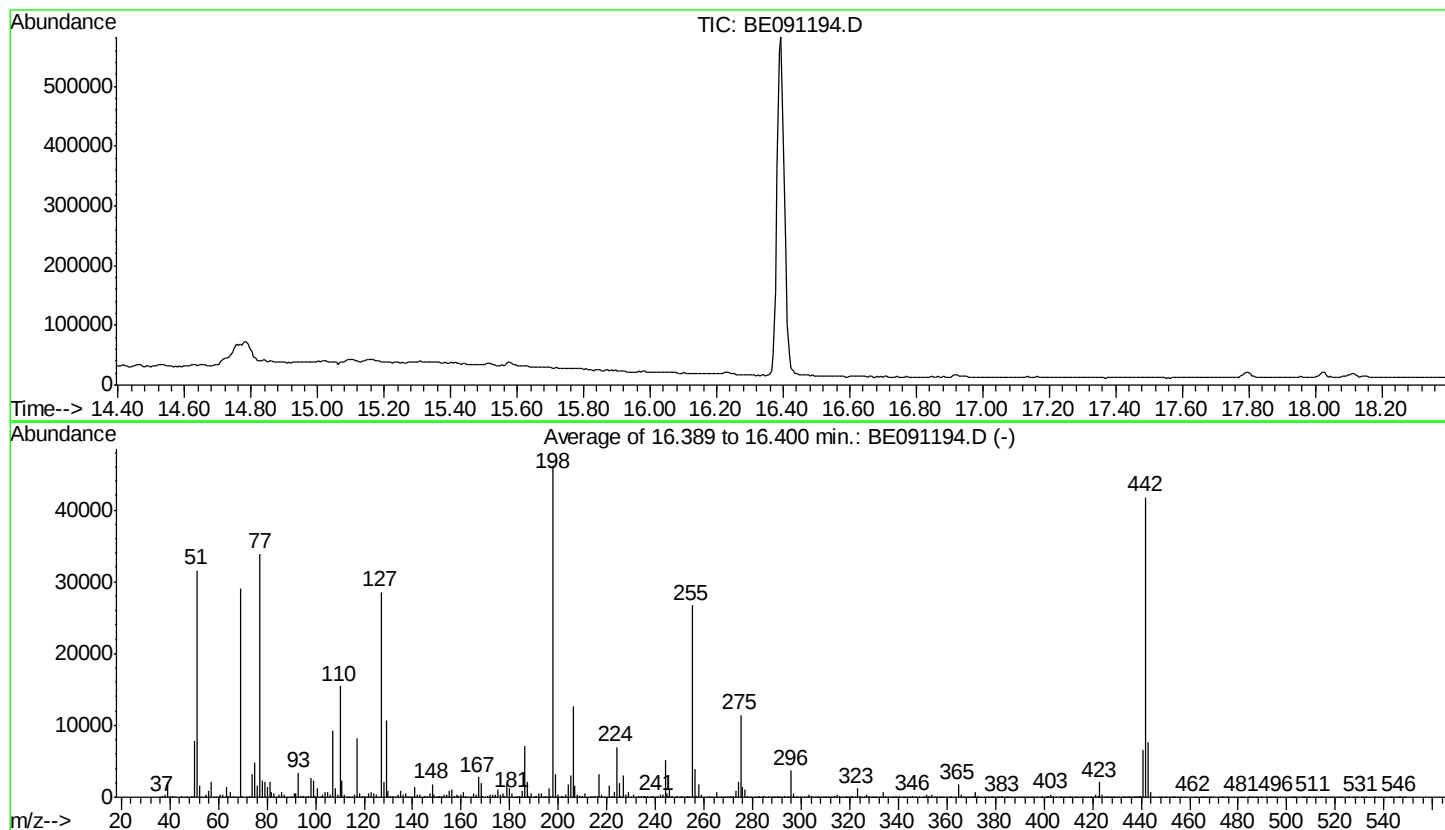

AutoFind: Scans 2349, 2350, 2351; Background Corrected with Scan 2342

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	68.5	31620	PASS
68	69	0.00	2	0.2	48	PASS
69	198	0.00	100	63.1	29118	PASS
70	69	0.00	2	0.7	206	PASS
127	198	10	80	61.9	28587	PASS
197	198	0.00	1	0.5	232	PASS
198	198	100	100	100.0	46160	PASS
199	198	5	9	7.1	3286	PASS
275	198	10	60	24.8	11441	PASS
365	198	1	100	3.9	1779	PASS
441	443	0.01	100	86.6	6606	PASS
442	198	50	100	90.4	41744	PASS
443	442	15	24	18.3	7625	PASS