
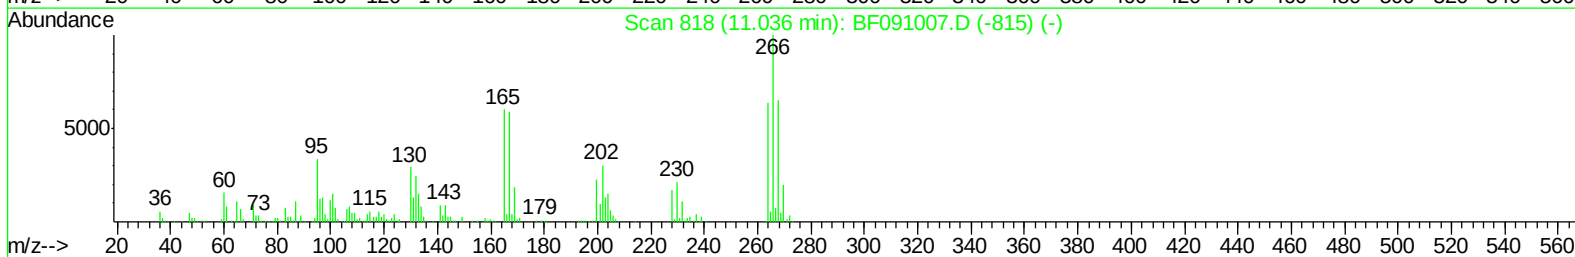
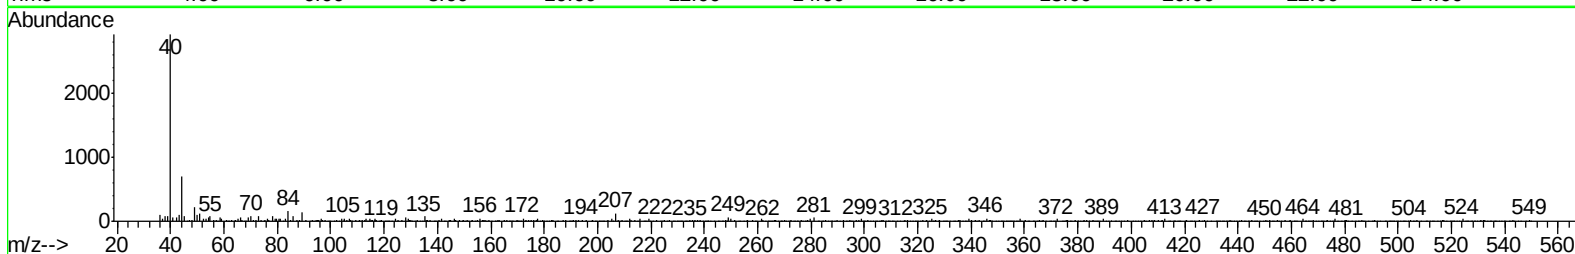


Data Path : Z:\HPCHEM1\BNA_E\Data\BE111716\
Data File : BE092556.D
Acq On : 17 Nov 2016 8:40
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 08:03:24 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

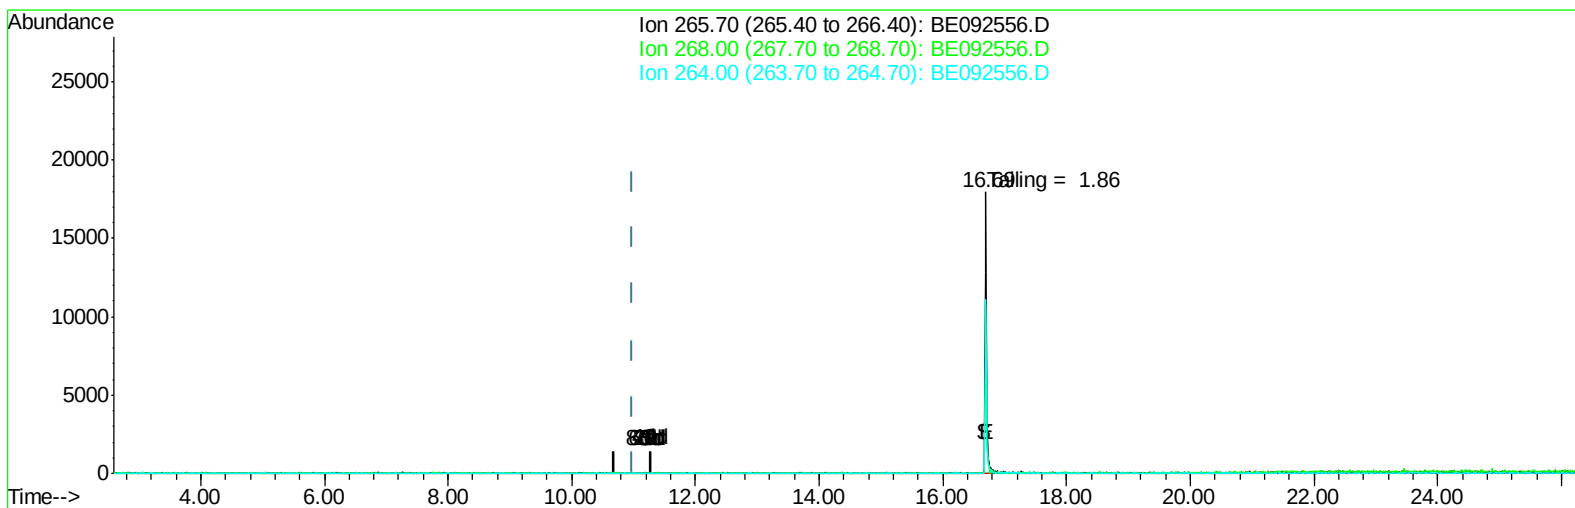

TIC: BE092556.D

(69) Pentachlorophenol (C)




11.233min (+0.242) 372.90ng

response 36

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	31.58#
264.00	63.90	52.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE111716\
Data File : BE092556.D
Acq On : 17 Nov 2016 8:40
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 08:03:24 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

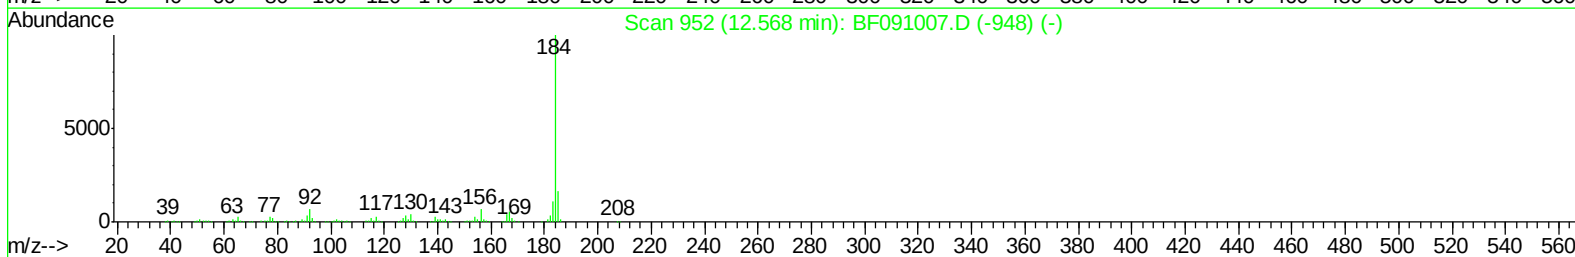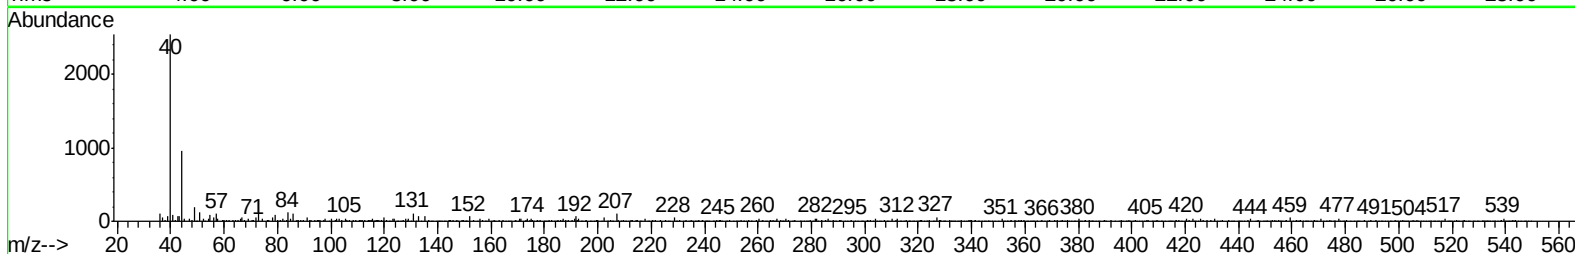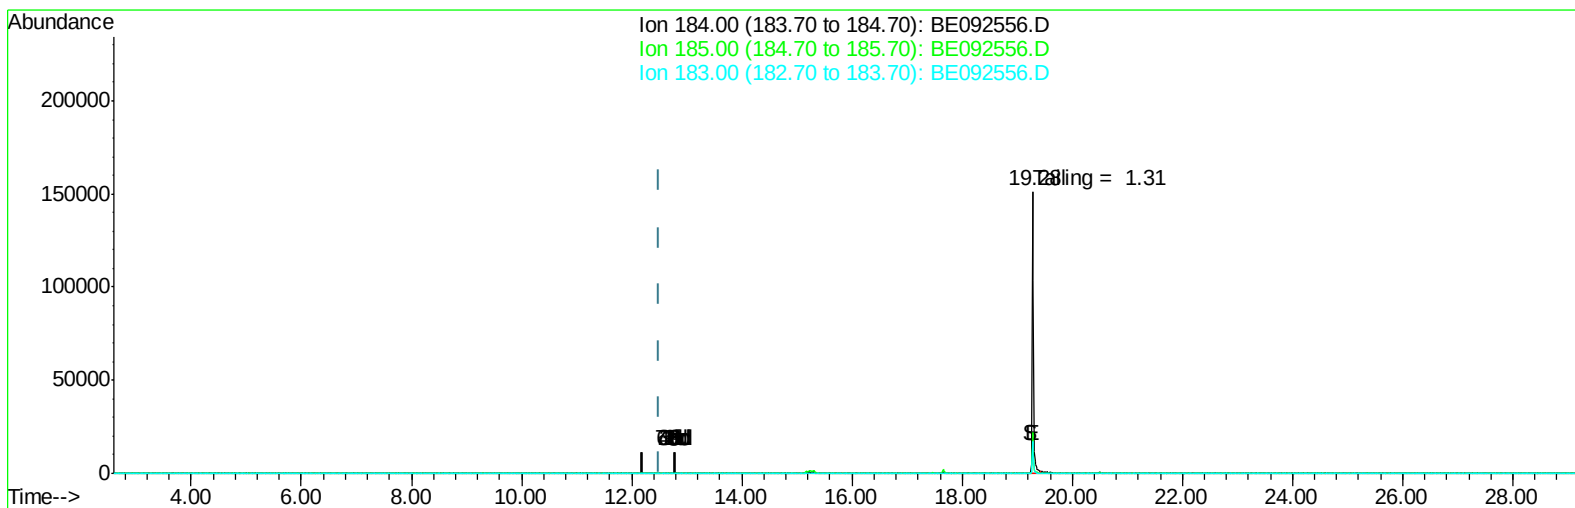

TIC: BE092556.D

(76) Benzidine

12.743min (+0.232) 73.25ng

response 18

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	66.67#
183.00	10.90	133.33#
0.00	0.00	0.00