

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111716\
 Data File : BE092559.D
 Acq On : 17 Nov 2016 11:18
 Operator : UM/SJ
 Sample : H5636-04RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 CPS043044RE

Quant Time: Nov 18 00:16:33 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE111616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 15:43:18 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	7451	5.00	ng	-0.02
7) Naphthalene-d8	10.93	136	33963	5.00	ng	0.00
12) Acenaphthene-d10	14.80	164	23155	5.00	ng	0.00
18) Phenanthrene-d10	17.56	188	49517	5.00	ng	0.00
24) Chrysene-d12	21.72	240	79032	5.00	ng	0.00
31) Perylene-d12	24.08	264	68644	5.00	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.65	112	7499	5.96	ng	-0.02
5) Phenol-d6	7.34	99	5426	2.66	ng	-0.02
8) Nitrobenzene-d5	9.32	82	12681	5.74	ng	-0.05
13) 2,4,6-Tribromophenol	16.30	330	7194	13.85	ng	-0.01
14) 2-Fluorobiphenyl	13.42	172	31197	5.53	ng	-0.01
26) Terphenyl-d14	20.16	244	53616	5.93	ng	-0.02
Target Compounds						
29) Bis(2-ethylhexyl)phthalate	21.61	149	2098	0.52	ng	Qvalue # 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111716\
Data File : BE092559.D
Acq On : 17 Nov 2016 11:18
Operator : UM/SJ
Sample : H5636-04RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
CPS043044RE

Quant Time: Nov 18 00:16:33 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE111616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 15:43:18 2016
Response via : Initial Calibration

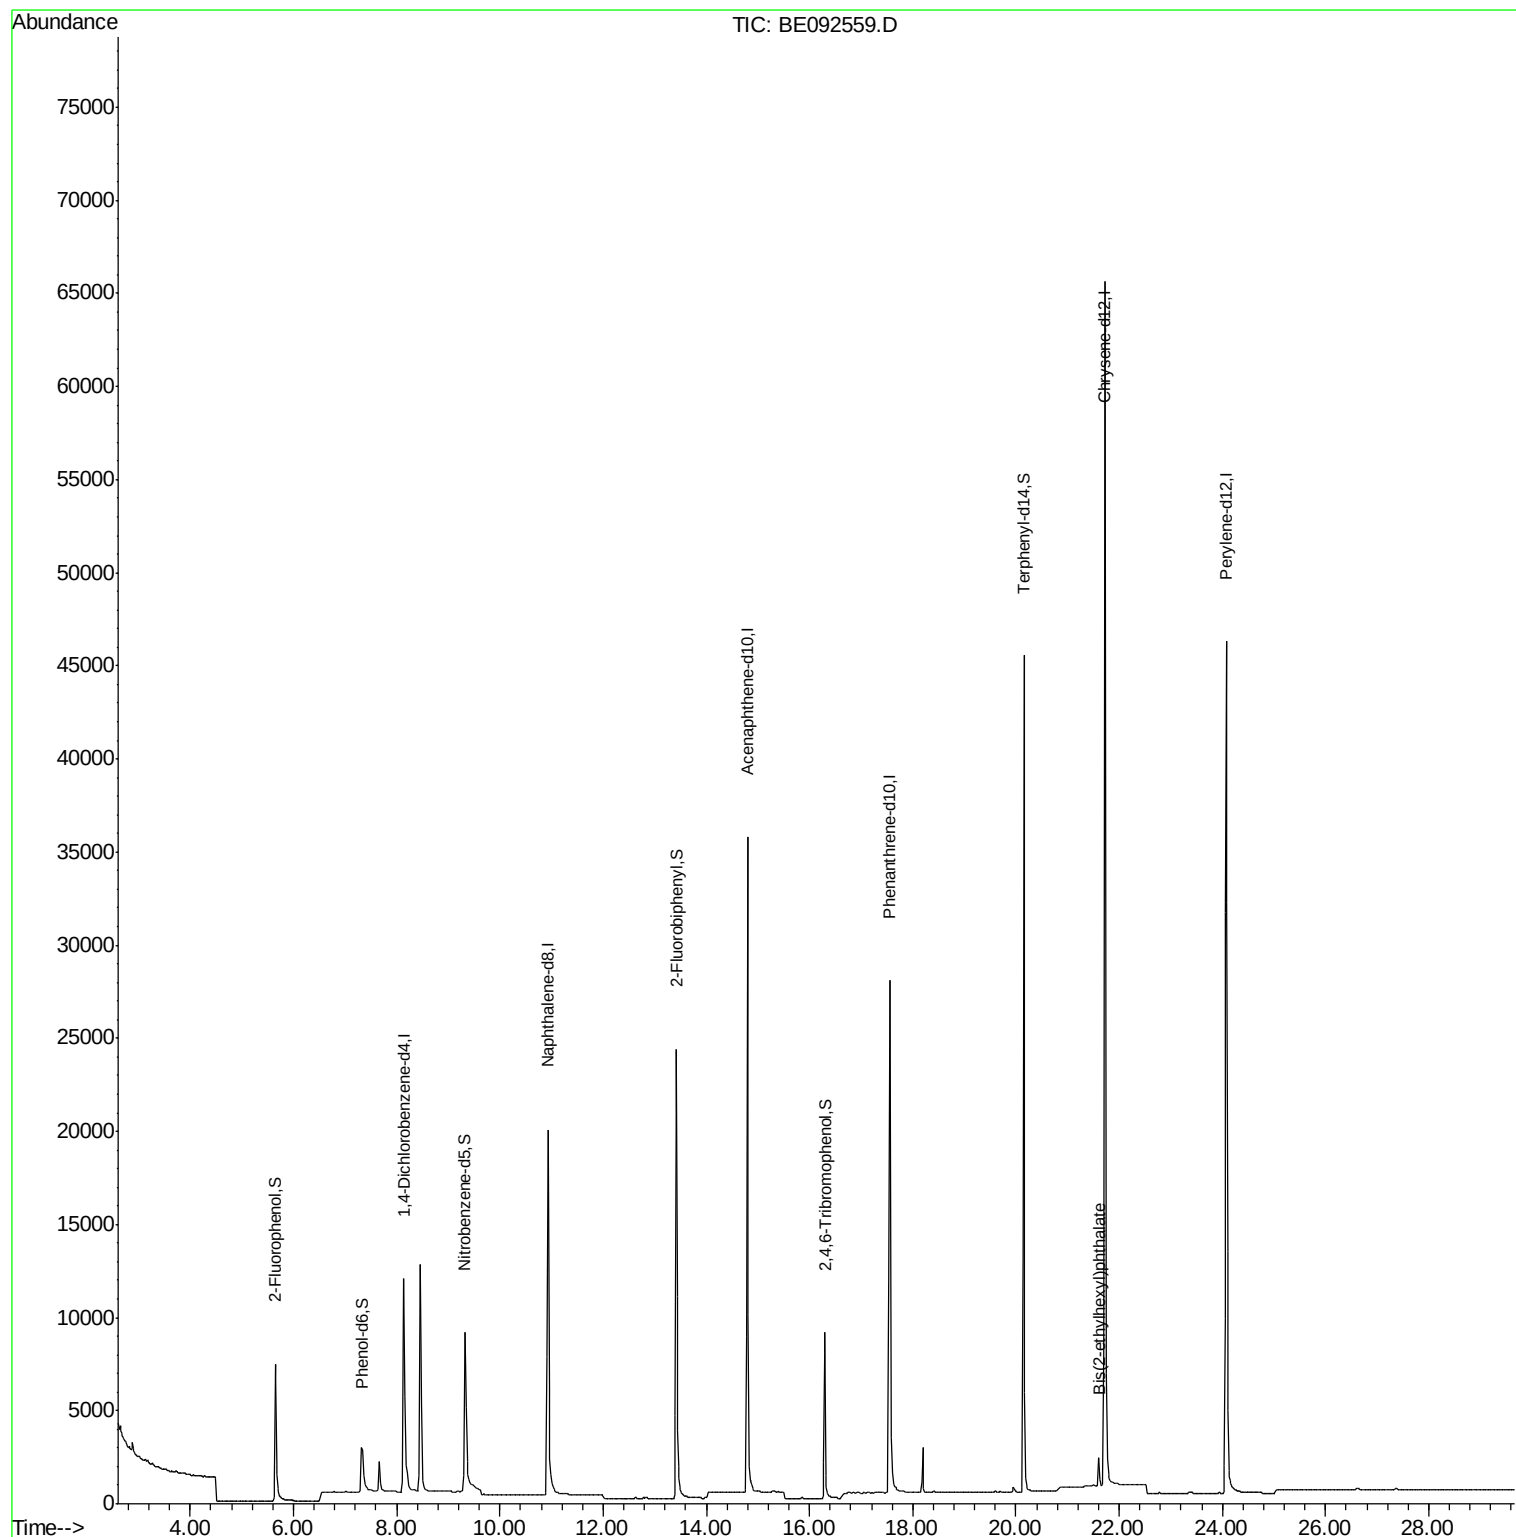



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.14 min Scan# 575

Delta R.T. -0.02 min

Lab File: BE092559.D

Acq: 17 Nov 2016 11:18

Instrument :

BNA_E

ClientSampleId :

CPS043044RE


Tot Ion:152 Resp: 7451

Ion Ratio Lower Upper

152 100

150 181.7 106.0 159.0#




115 85.5 31.2 46.8#

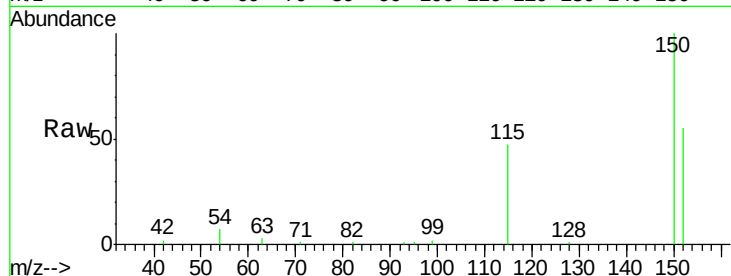

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

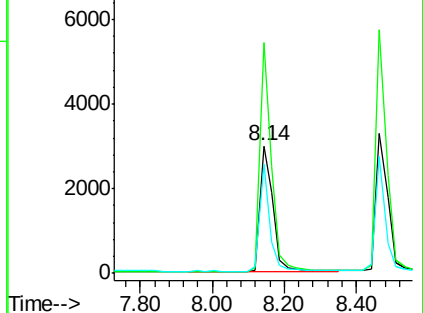

#4

2-Fluorophenol

Concen: 5.96 ng

RT: 5.65 min Scan# 360

Delta R.T. -0.02 min

Lab File: BE092559.D

Acq: 17 Nov 2016 11:18


Tgt Ion:112 Resp: 7499

Ion Ratio Lower Upper

112 100

64 67.6 53.5 80.3



63 35.8 27.9 41.9




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

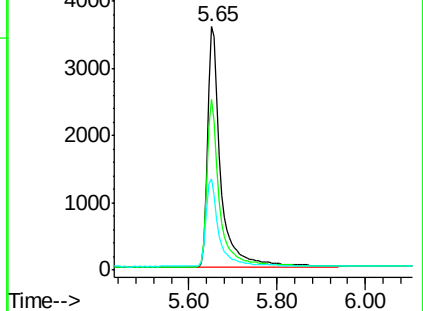



#5

Phenol-d6

Concen: 2.66 ng

RT: 7.34 min Scan# 540

Delta R.T. -0.02 min

Lab File: BE092559.D

Acq: 17 Nov 2016 11:18

Instrument :

BNA_E

ClientSampleId :

CPS043044RE


Tot Ion: 99 Resp: 5426

Ion Ratio Lower Upper

99 100

42 0.0 16.0 24.0#




71 0.0 30.6 45.8#

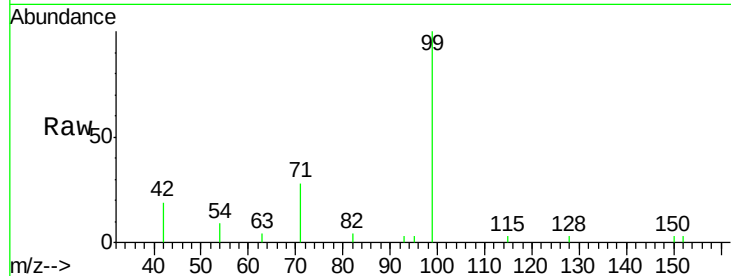

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

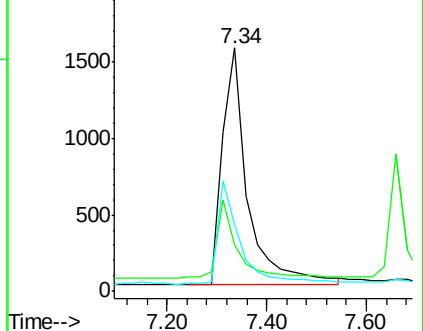

#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.93 min Scan# 707

Delta R.T. 0.00 min

Lab File: BE092559.D

Acq: 17 Nov 2016 11:18

Tgt Ion:136 Resp: 33963


Ion Ratio Lower Upper

136 100

137 11.3 8.2 12.4

54 7.2 9.6 14.4#

68 5.4 6.7 10.1#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

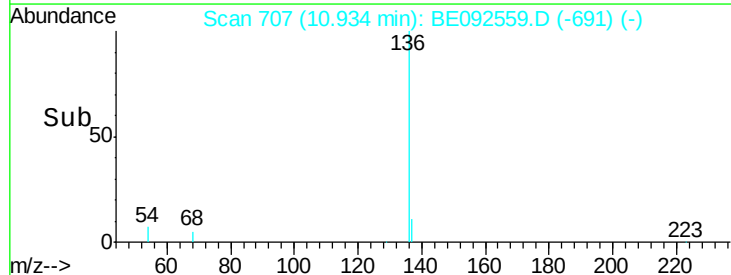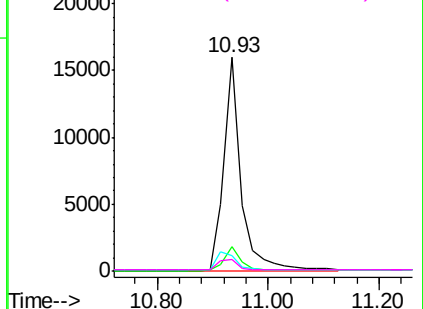

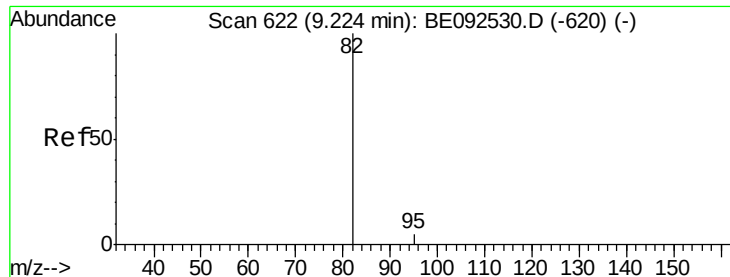

#8

Nitrobenzene-d5

Concen: 5.74 ng

RT: 9.32 min Scan# 626

Delta R.T. -0.05 min

Lab File: BE092559.D

Acq: 17 Nov 2016 11:18

Instrument :

BNA_E

ClientSampleId :

CPS043044RE


Tot Ion: 82 Resp: 12681

Ion Ratio Lower Upper

82 100

128 21.8 39.0 58.4#




54 62.1 44.8 67.2

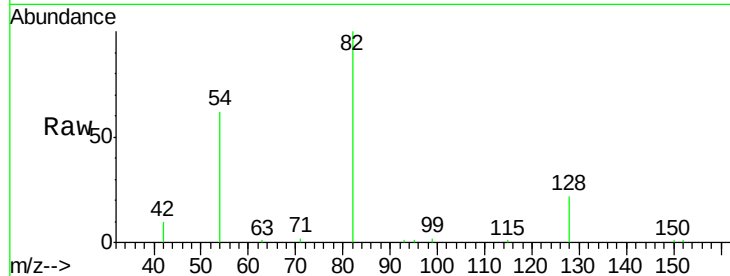

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

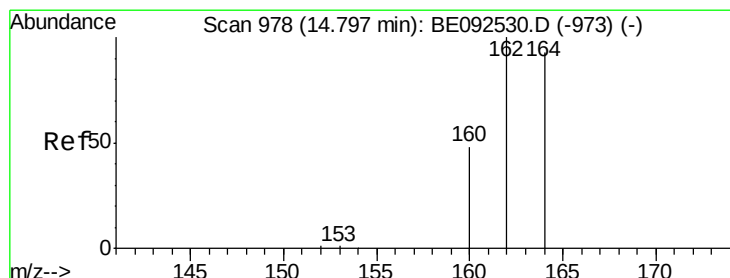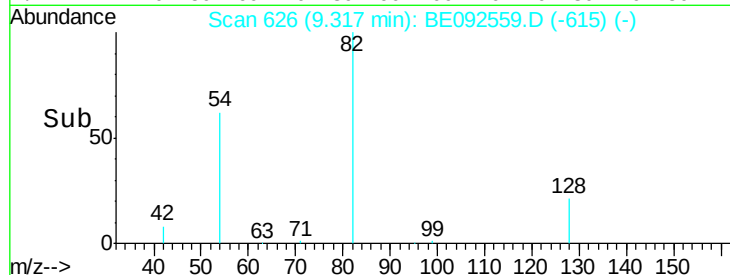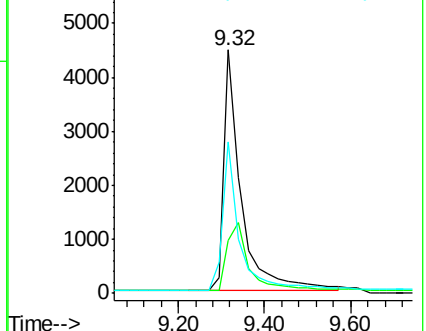

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.80 min Scan# 979

Delta R.T. 0.00 min

Lab File: BE092559.D

Acq: 17 Nov 2016 11:18


Tgt Ion: 164 Resp: 23155

Ion Ratio Lower Upper

164 100

162 99.5 71.4 107.0



160 43.6 27.4 41.2#

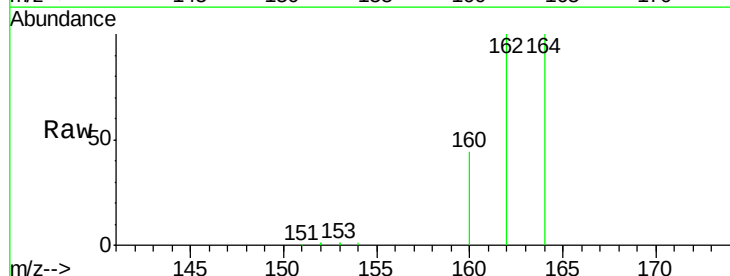


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

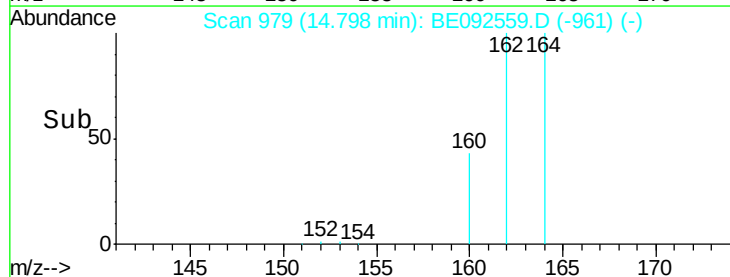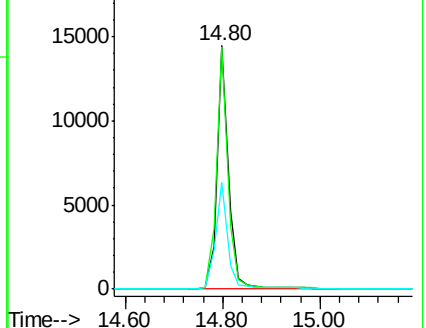


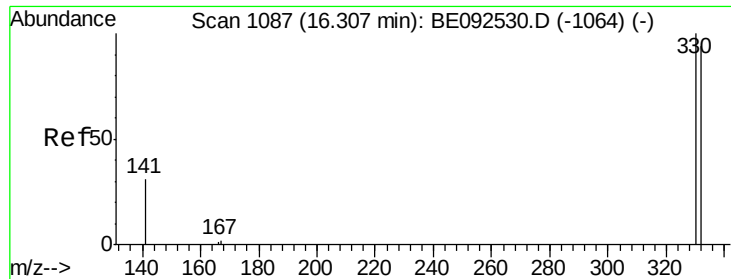




#13
 2,4,6-Tribromophenol
 Concen: 13.85 ng
 RT: 16.30 min Scan# 1087
 Delta R.T. -0.01 min
 Lab File: BE092559.D
 Acq: 17 Nov 2016 11:18

Instrument :
 BNA_E
 ClientSampleId :
 CPS043044RE

Tot Ion:330 Resp: 7194
 Ion Ratio Lower Upper
 330 100
 332 96.5 75.4 113.0
 141 43.5 31.0 46.6

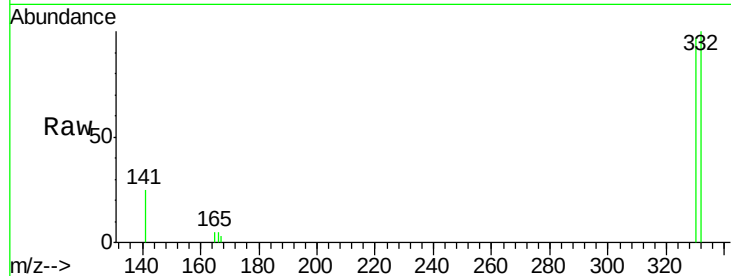


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

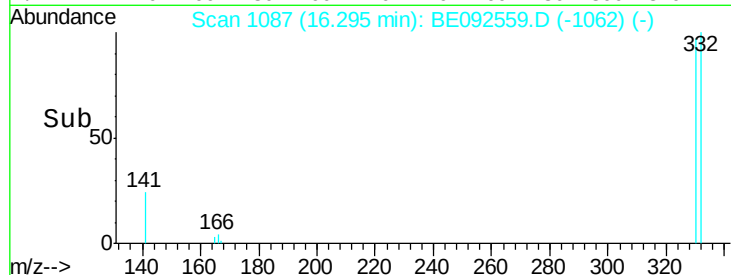
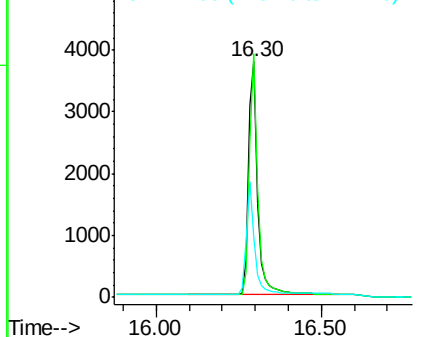



#14
 2-Fluorobiphenyl
 Concen: 5.53 ng
 RT: 13.42 min Scan# 883
 Delta R.T. -0.01 min
 Lab File: BE092559.D
 Acq: 17 Nov 2016 11:18

Tgt Ion:172 Resp: 31197
 Ion Ratio Lower Upper
 172 100
 171 31.7 30.1 45.1
 170 20.1 21.8 32.6#



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

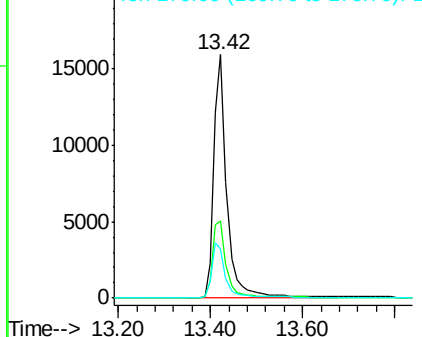

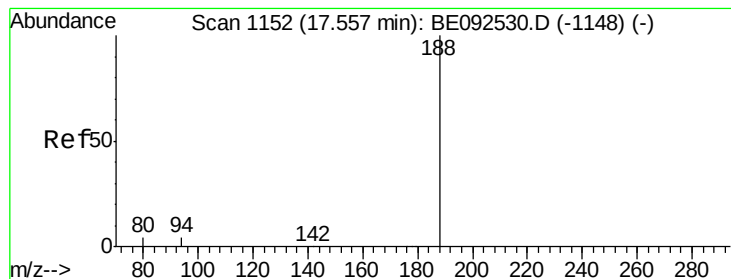

#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.56 min Scan# 1153

Delta R.T. -0.00 min

Lab File: BE092559.D

Acq: 17 Nov 2016 11:18

Instrument :

BNA_E

ClientSampleId :

CPS043044RE


Tot Ion:188 Resp: 49517

Ion Ratio Lower Upper

188 100

94 4.5 3.2 4.8




80 4.1 2.6 3.8#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

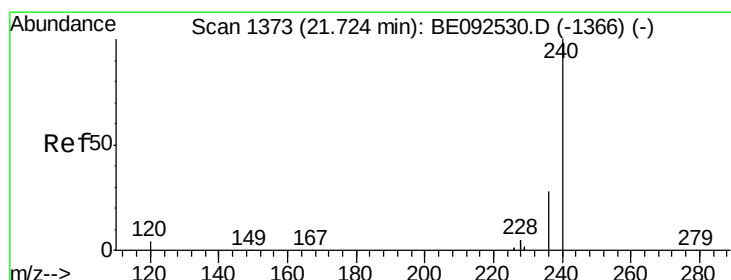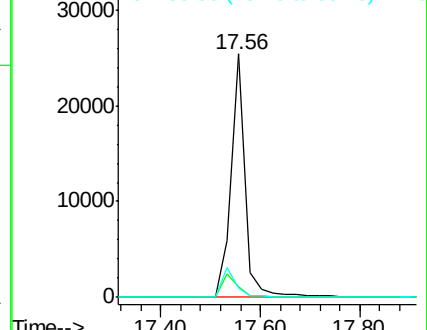

#24

Chrysene-d12

Concen: 5.00 ng

RT: 21.72 min Scan# 1374

Delta R.T. -0.00 min

Lab File: BE092559.D

Acq: 17 Nov 2016 11:18


Tgt Ion:240 Resp: 79032

Ion Ratio Lower Upper

240 100

120 2.2 2.6 4.0#



236 26.1 24.6 37.0




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

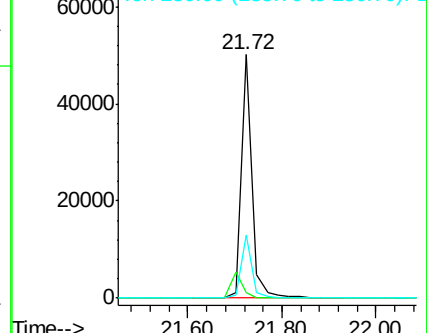



#26

Terphenyl-d14

Concen: 5.93 ng

RT: 20.16 min Scan# 1298

Delta R.T. -0.02 min

Lab File: BE092559.D

Acq: 17 Nov 2016 11:18

Instrument :

BNA_E

ClientSampleId :

CPS043044RE


Tot Ion:244 Resp: 53616

Ion Ratio Lower Upper

244 100

212 8.1 6.7 10.1




122 3.6 3.6 5.4

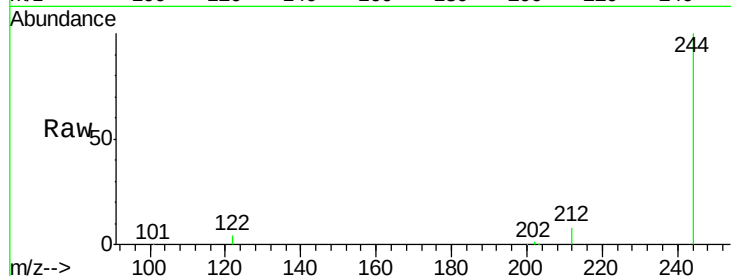

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

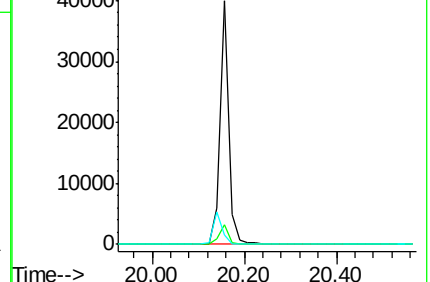

#29

Bis(2-ethylhexyl)phthalate

Concen: 0.52 ng

RT: 21.61 min Scan# 1369

Delta R.T. -0.02 min

Lab File: BE092559.D

Acq: 17 Nov 2016 11:18


Tgt Ion:149 Resp: 2098

Ion Ratio Lower Upper

149 100

167 22.4 16.0 24.0



279 0.0 16.0 24.0#






Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

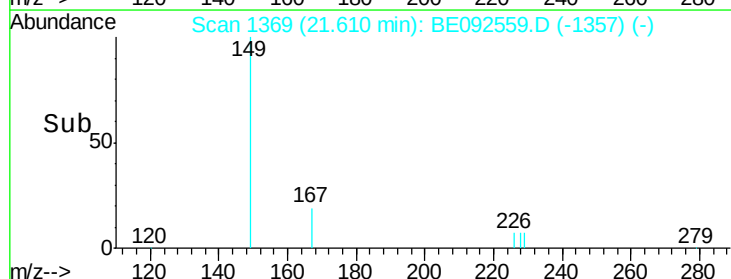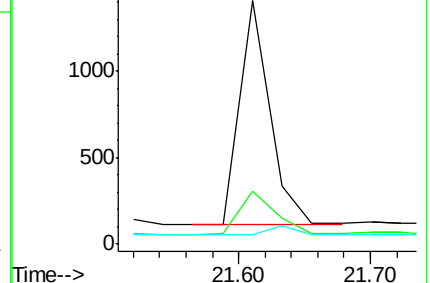

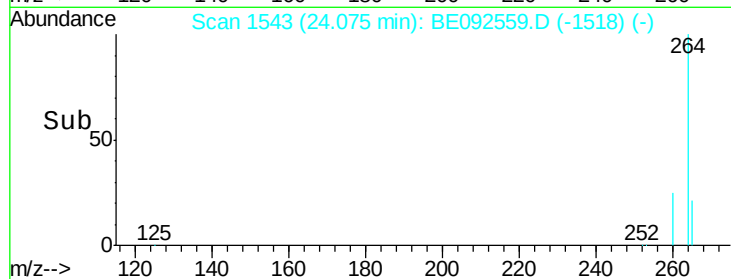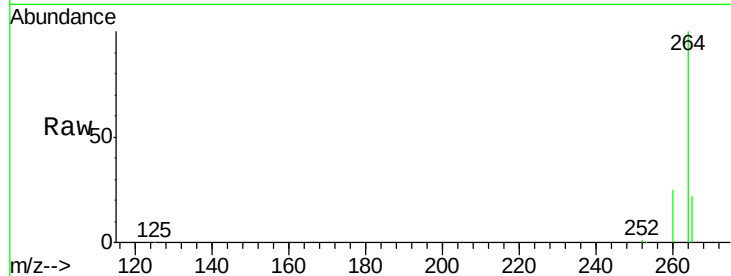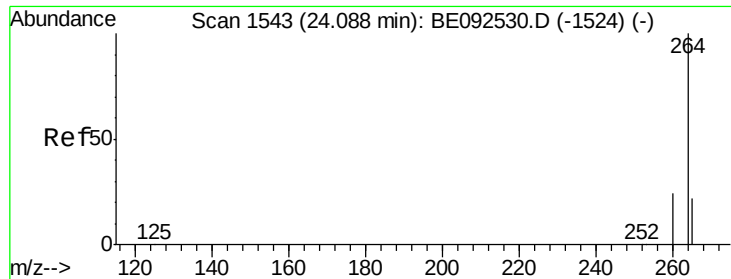

#31

Pervlene-d12

Concen: 5.00 ng

RT: 24.08 min Scan# 1543

Delta R.T. -0.01 min

Lab File: BE092559.D

Acq: 17 Nov 2016 11:18

Instrument :

BNA_E

ClientSampleId :

CPS043044RE

Tot Ion: 264 Resp: 68644

Ion Ratio Lower Upper

264 100

260 25.2 20.1 30.1

265 22.0 17.9 26.9

