


Data Path : Z:\HPCHEM1\BNA E\DATA\BE111716\
 Data File : BE092556.D
 Acq On : 17 Nov 2016 8:40
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 16 15:43:18 2016

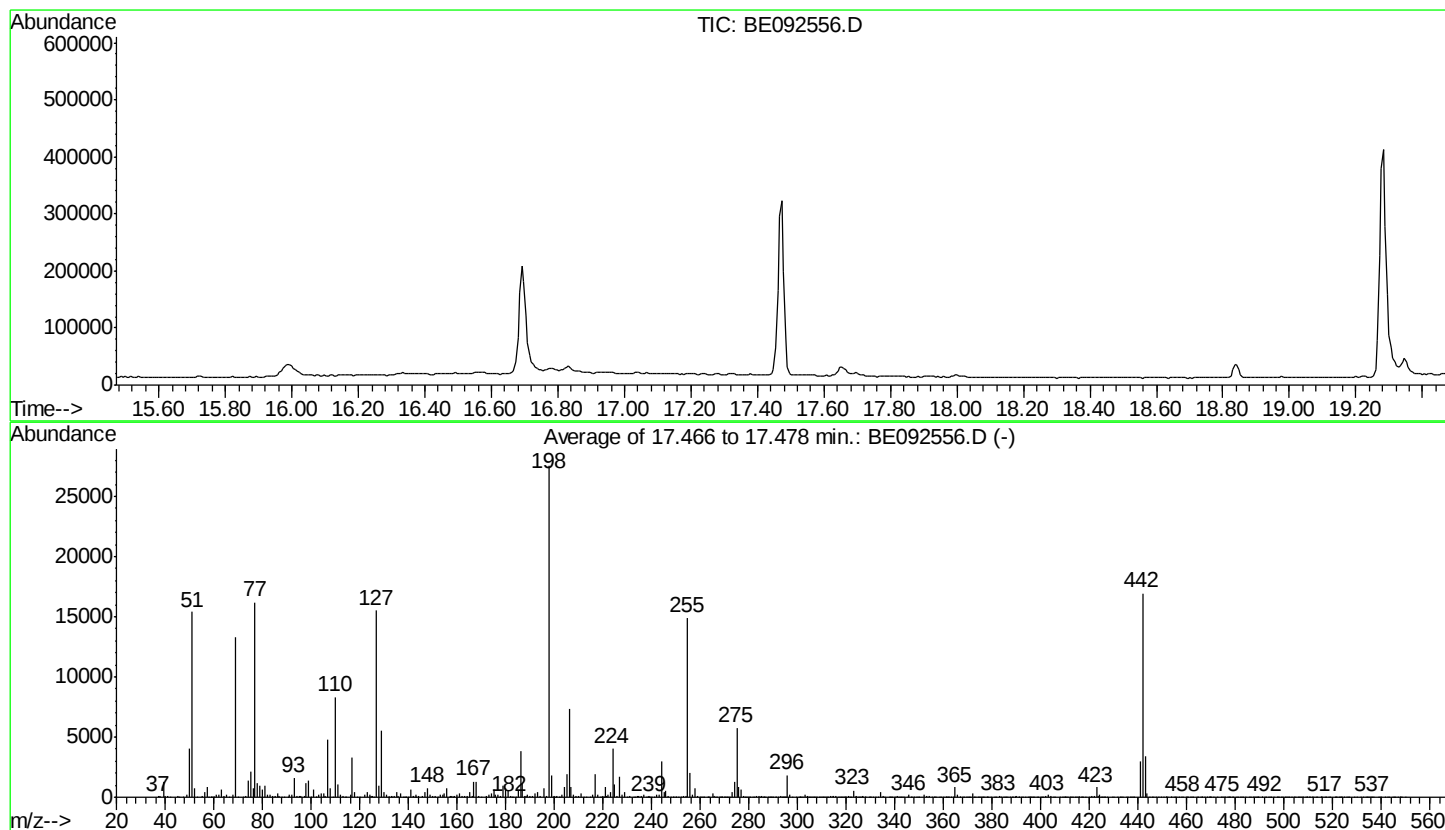

AutoFind: Scans 2532, 2533, 2534; Background Corrected with Scan 2524

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.8	15382	PASS
68	69	0.00	2	1.7	232	PASS
69	198	0.00	100	48.3	13308	PASS
70	69	0.00	2	0.3	44	PASS
127	198	10	80	56.3	15522	PASS
197	198	0.00	2	0.3	75	PASS
198	198	100	100	100.0	27550	PASS
199	198	5	9	6.4	1759	PASS
275	198	10	60	21.0	5794	PASS
365	198	1	100	2.9	807	PASS
441	442	0.01	24	17.8	3009	PASS
442	198	50	100	61.5	16938	PASS
443	442	15	24	20.3	3438	PASS