

Data Path : Z:\HPCHEM1\BNA E\Data\BE111815\
 Data File : BE091228.D
 Acq On : 18 Nov 2015 15:17
 Operator : UM/NP
 Sample : G4342-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 D9KP0

Manual Integrations
 APPROVED

Mmdadoda
 11/19/2015 6:46:36 PM

Quant Time: Nov 19 17:48:02 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 19 04:25:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	3974	0.40	ng/ul	-0.02
4) Naphthalene-d8	9.56	136	20192	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.36	164	11914	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.09	188	35083m	0.40	ng/ul	0.00
18) Chrysene-d12	20.23	240	63216	0.40	ng/ul	0.00
22) Perylene-d12	22.11	264	52753m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.97	96	17186	6.01	ng/uL	-0.02
6) 2-Methylnaphthalene-d10	11.07	152	4626	0.17	ng/ul	0.00
16) Fluoranthene-d10	18.07	212	15610	0.16	ng/ul	0.00
Target Compounds						
17) Fluoranthene	18.09	202	24697	0.05	ng/ul	Ovalue 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\Data\BE111815\
Data File : BE091228.D
Acq On : 18 Nov 2015 15:17
Operator : UM/NP
Sample : G4342-03
Misc :
ALS Vial : 35 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
D9KP0

Manual Integrations
APPROVED

Mmdadoda
11/19/2015 6:46:36 PM

Quant Time: Nov 19 17:48:02 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 19 04:25:56 2015
Response via : Initial Calibration

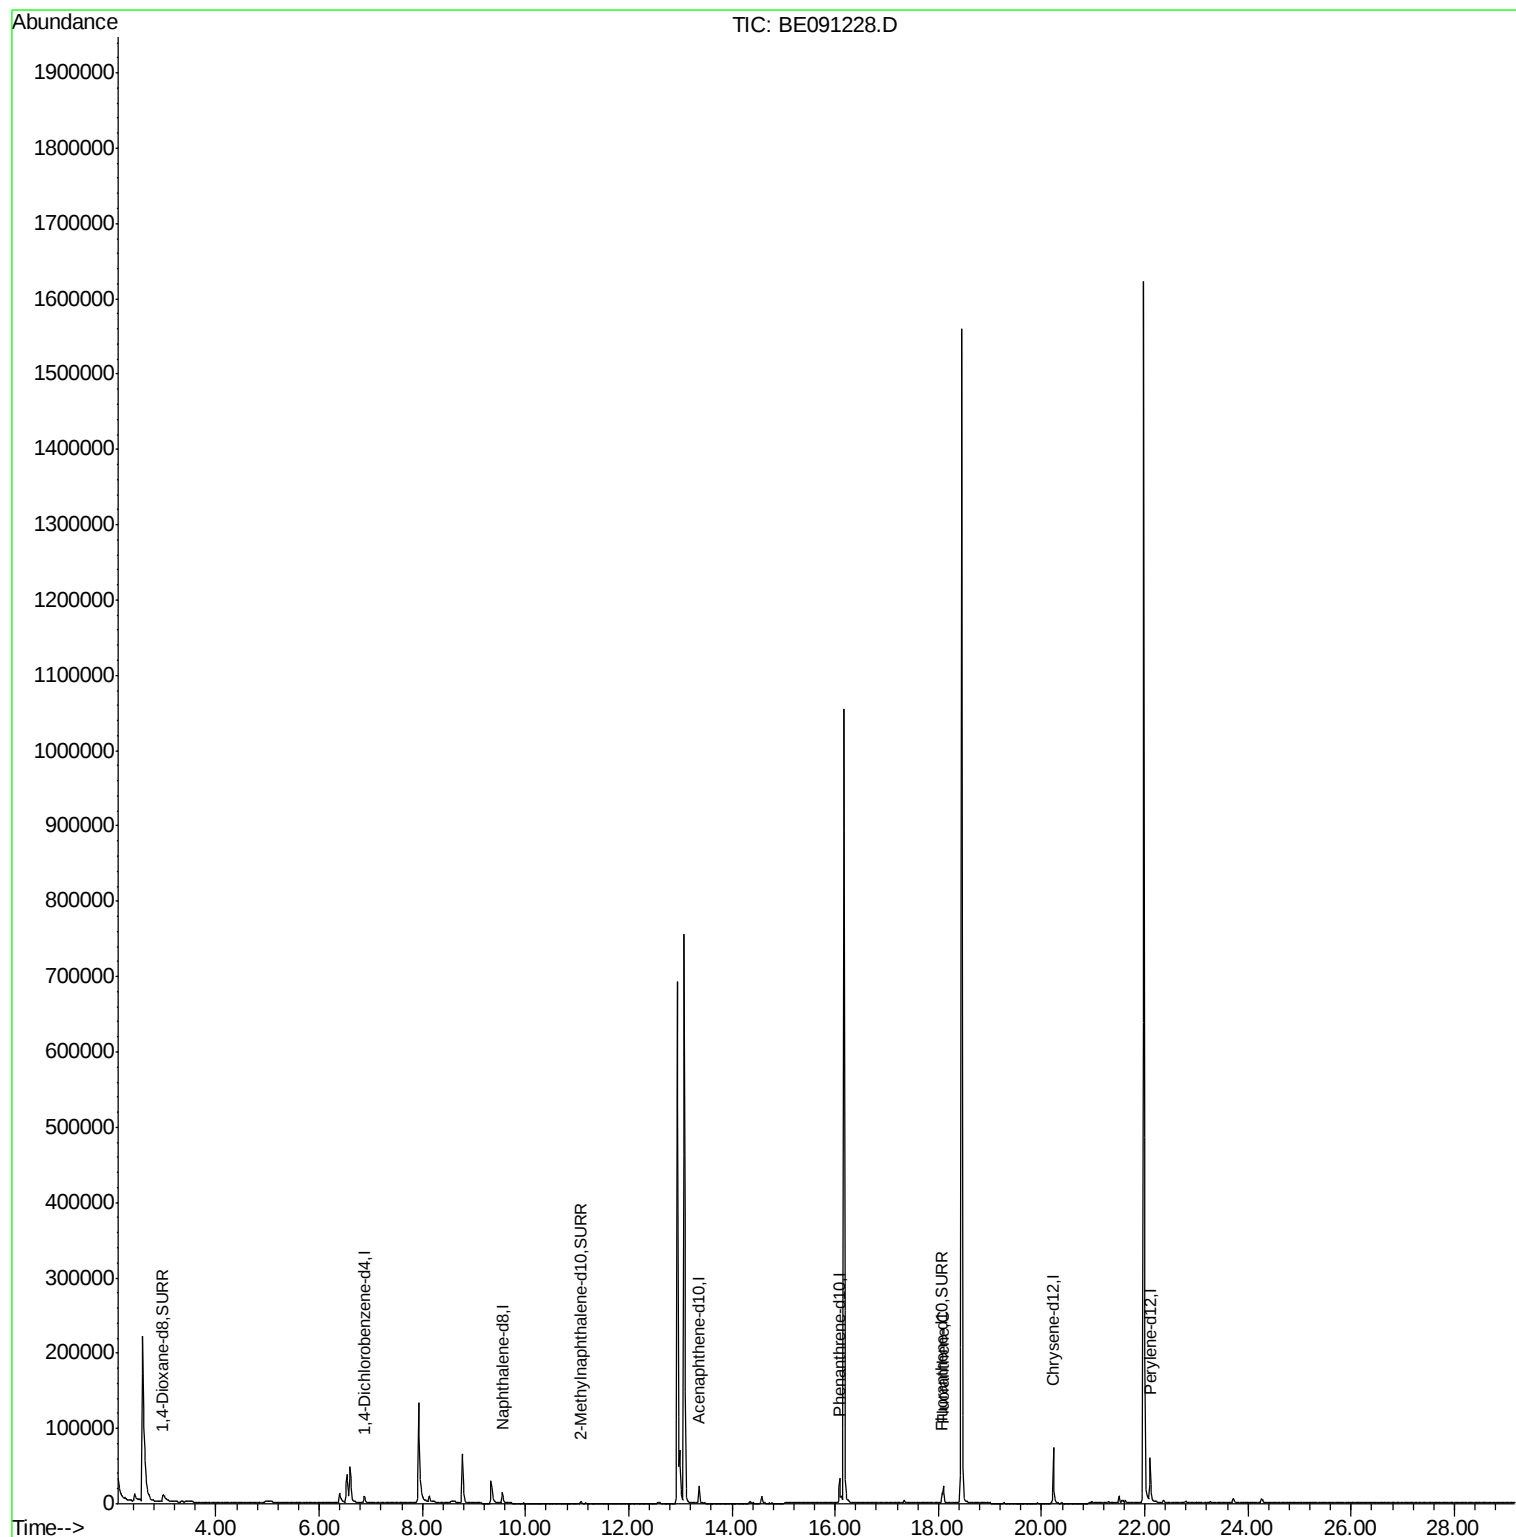

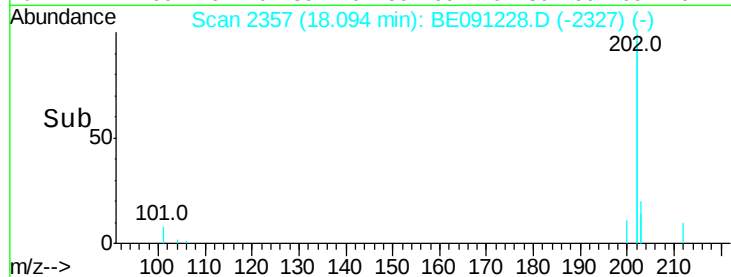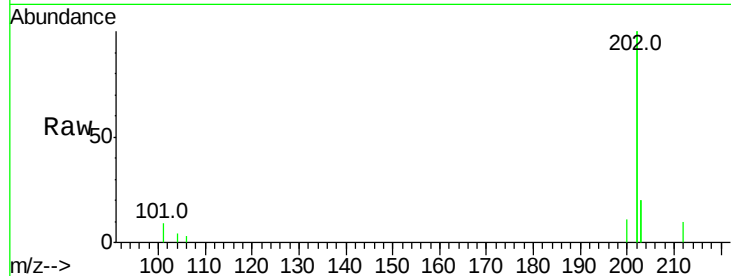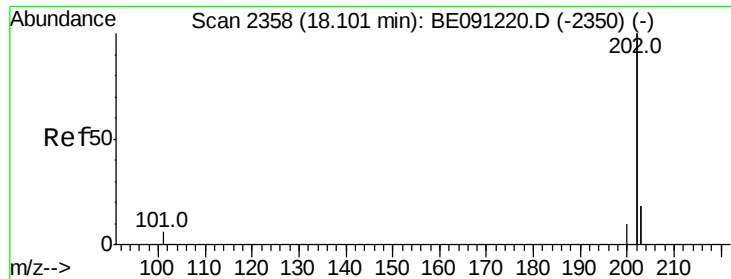

#17

Fluoranthene

Concen: 0.05 ng/ul

RT: 18.09 min Scan# 2357

Delta R.T. -0.01 min

Lab File: BE091228.D

Acq: 18 Nov 2015 15:17

Tot Ion:	202	Resp:	24697
Ion Ratio	Lower	Upper	
202	100		
101	4.5	0.0	33.1
203	19.6	0.0	37.2

Instrument :

BNA_E

ClientSampleId :

D9KP0

Manual Integrations
APPROVED

Mmdadoda
11/19/2015 6:46:36 PM

