

Data Path : Z:\HPCHEM1\BNA E\DATA\BE111815\
 Data File : BE091237.D
 Acq On : 18 Nov 2015 20:48
 Operator : UM/NP
 Sample : G4310-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 D9KL6

Manual Integrations
 APPROVED

Mmdadoda
 11/19/2015 7:01:03 PM

Quant Time: Nov 19 18:33:34 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 19 06:02:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	3793	0.40	ng/ul	-0.03
4) Naphthalene-d8	9.55	136	19782	0.40	ng/ul	-0.02
8) Acenaphthene-d10	13.36	164	13181	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.09	188	37205m	0.40	ng/ul	0.00
18) Chrysene-d12	20.23	240	63289	0.40	ng/ul	0.00
22) Perylene-d12	22.11	264	55765m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.96	96	24459	8.96	ng/uL	-0.03
6) 2-Methylnaphthalene-d10	11.06	152	7319	0.27	ng/ul	0.00
16) Fluoranthene-d10	18.07	212	24368	0.23	ng/ul	0.00
Target Compounds						
14) Phenanthrene	16.11	178	13293	0.03	ng/ul	Ovalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE111815\
Data File : BE091237.D
Acq On : 18 Nov 2015 20:48
Operator : UM/NP
Sample : G4310-01
Misc :
ALS Vial : 43 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
D9KL6

Manual Integrations
APPROVED

Mmdadoda
11/19/2015 7:01:03 PM

Quant Time: Nov 19 18:33:34 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 19 06:02:12 2015
Response via : Initial Calibration

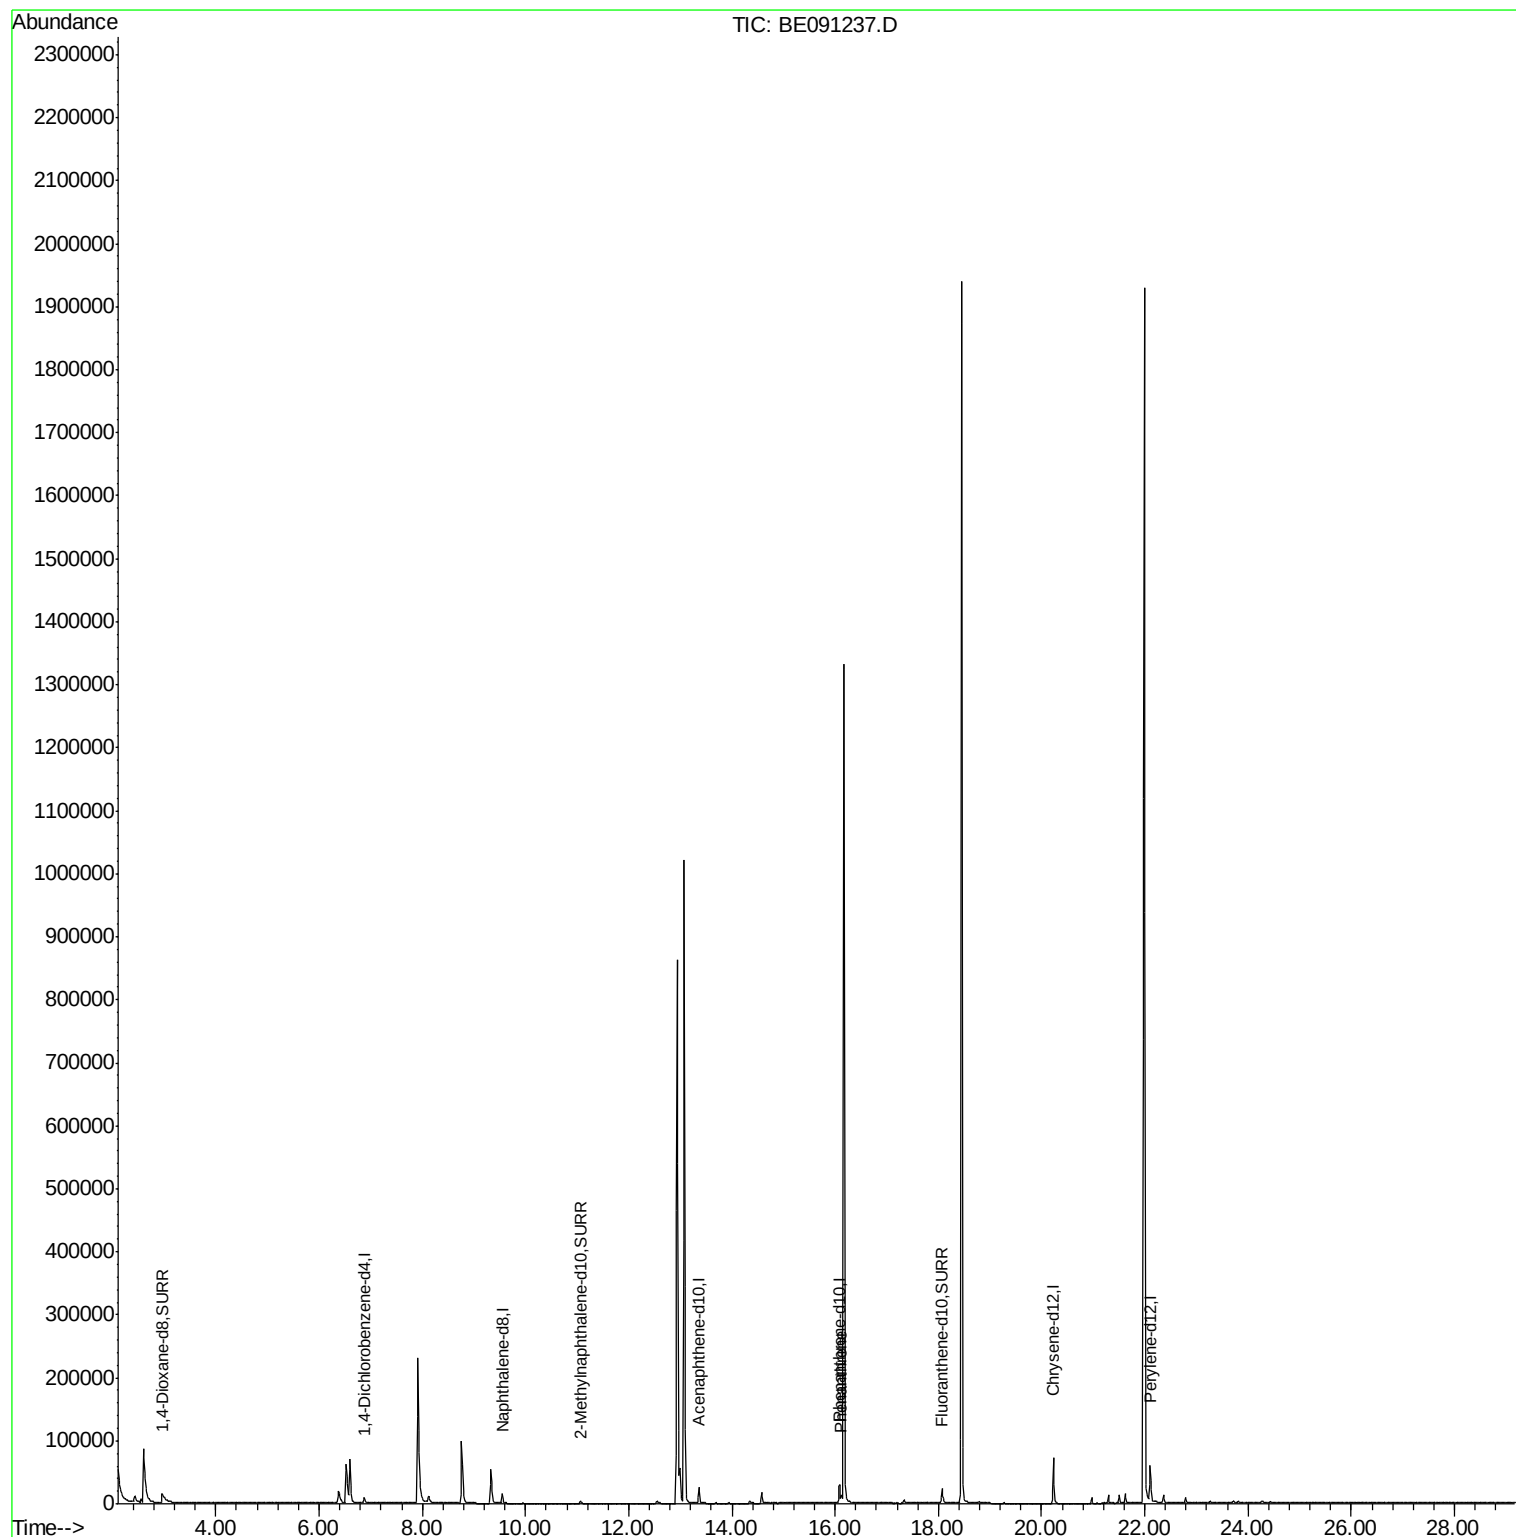

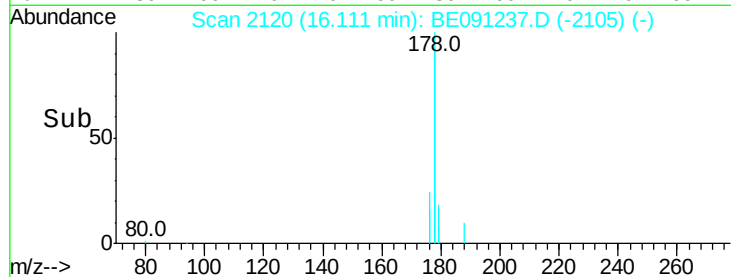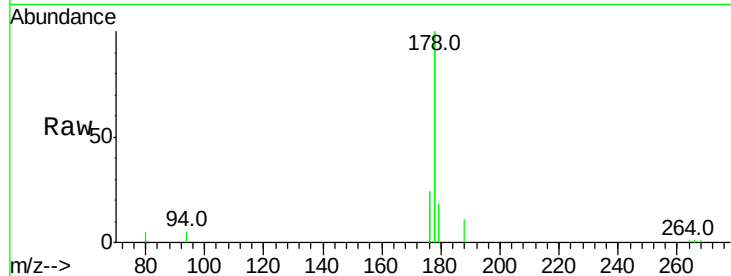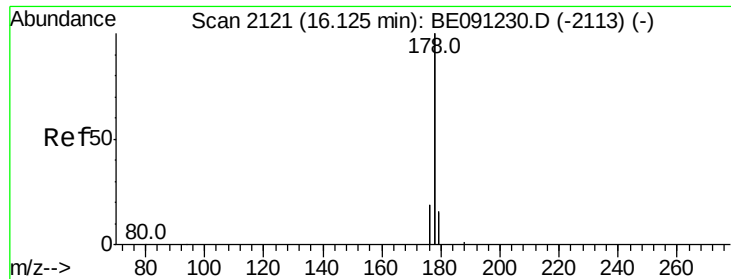

#14

Phenanthrene

Concen: 0.03 ng/ul

RT: 16.11 min Scan# 2120

Delta R.T. -0.01 min

Lab File: BE091237.D

Acq: 18 Nov 2015 20:48

Instrument :

BNA_E

ClientSampleId :

D9KL6

Tot Ion:178 Resp: 13293

Ion Ratio Lower Upper

178 100

176 24.0 16.2 24.4

179 18.2 12.8 19.2

Manual Integrations
APPROVED

Mmdadoda
11/19/2015 7:01:03 PM

