


Data Path : Z:\HPCHEM1\BNA_E\Data\BE111816\
 Data File : BE092562.D
 Acq On : 18 Nov 2016 11:31
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 16 15:43:18 2016

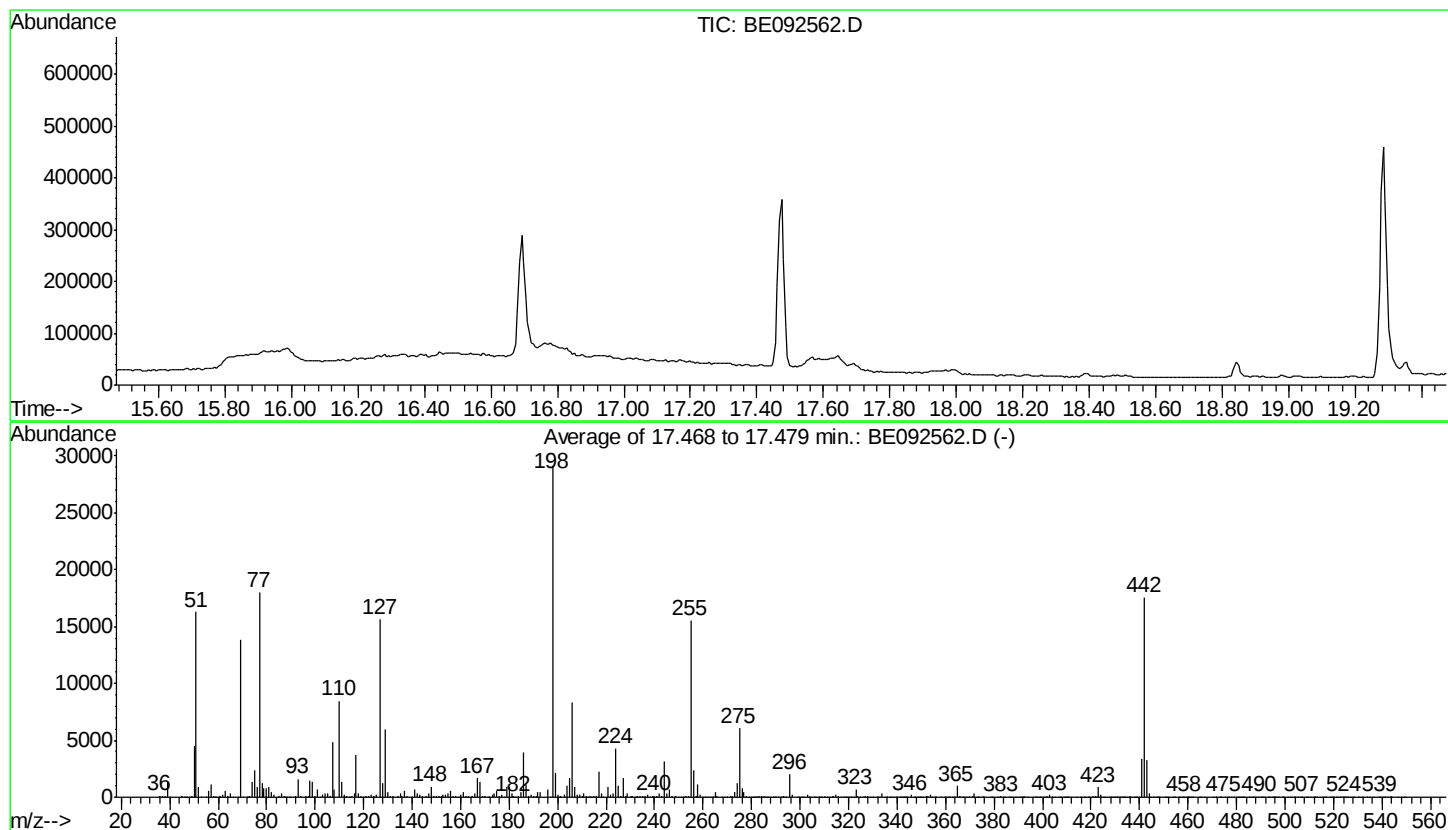

AutoFind: Scans 2532, 2533, 2534; Background Corrected with Scan 2522

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.9	16273	PASS
68	69	0.00	2	0.3	41	PASS
69	198	0.00	100	47.7	13889	PASS
70	69	0.00	2	0.2	30	PASS
127	198	10	80	53.6	15615	PASS
197	198	0.00	2	0.1	35	PASS
198	198	100	100	100.0	29135	PASS
199	198	5	9	7.2	2085	PASS
275	198	10	60	20.8	6052	PASS
365	198	1	100	3.4	981	PASS
441	442	0.01	24	19.5	3415	PASS
442	198	50	100	60.1	17522	PASS
443	442	15	24	18.3	3211	PASS