


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE111918\
 Data File : BE098243.D
 Acq On : 19 Nov 2018 8:34
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 16 19:05:33 2018

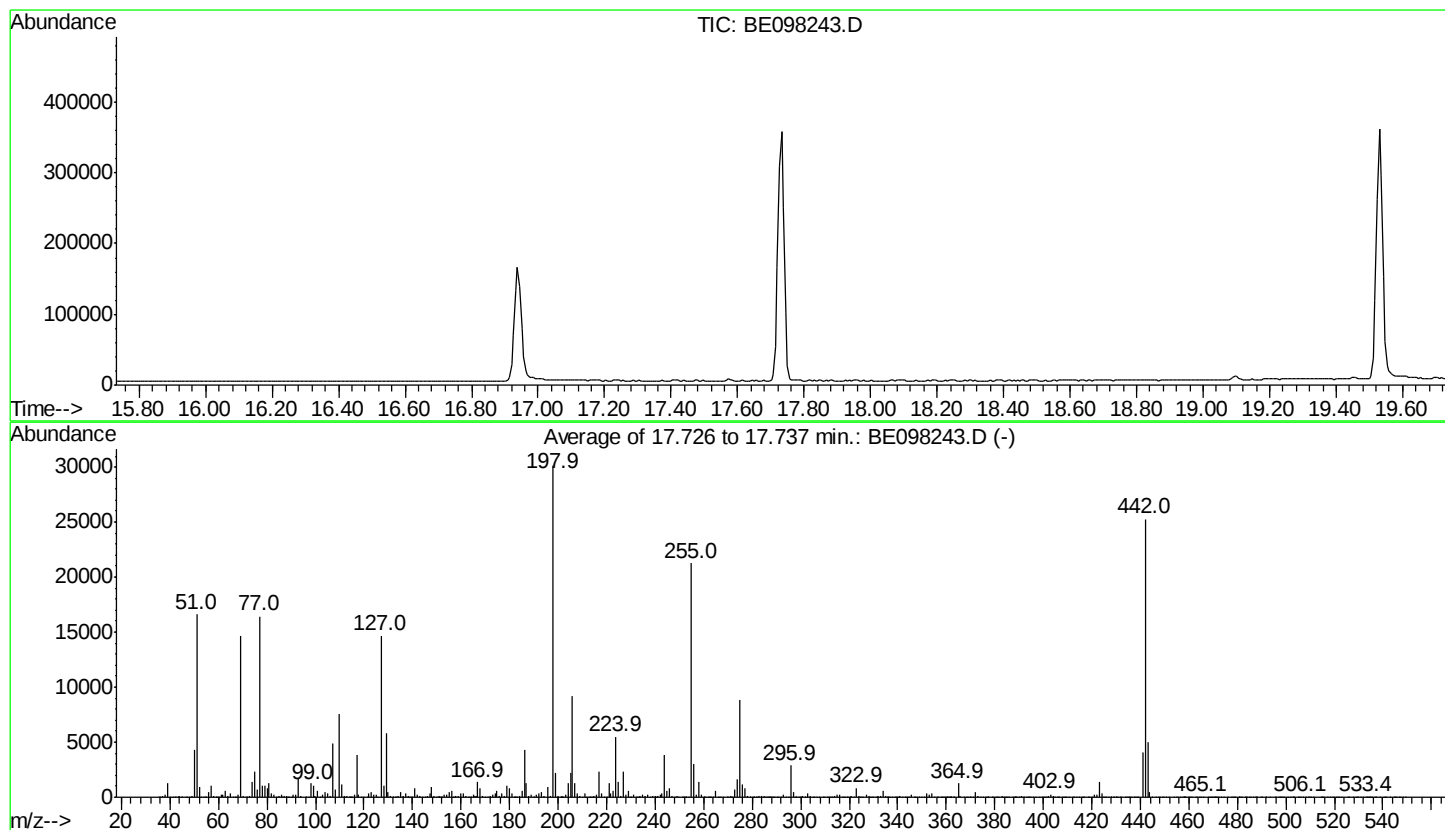

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.1	16594	PASS
68	69	0.00	2	1.6	237	PASS
69	198	0.00	100	48.5	14615	PASS
70	69	0.00	2	0.6	88	PASS
127	198	10	80	48.7	14664	PASS
197	198	0.00	2	0.5	154	PASS
198	198	100	100	100.0	30130	PASS
199	198	5	9	7.4	2229	PASS
275	198	10	60	29.3	8834	PASS
365	198	1	100	4.2	1261	PASS
441	198	0.01	100	13.7	4118	PASS
442	198	50	100	83.9	25288	PASS
443	442	15	24	19.9	5025	PASS