

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112015\
 Data File : BE091256.D
 Acq On : 20 Nov 2015 22:33
 Operator : UM/NP
 Sample : SSTDC00.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTD0.478

Quant Time: Nov 21 02:54:49 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 21 02:52:22 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	2748	0.40	ng/ul	0.00
4) Naphthalene-d8	9.57	136	11839	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.37	164	4907	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.09	188	14343	0.40	ng/ul	0.00
18) Chrysene-d12	20.23	240	18592	0.40	ng/ul	0.00
22) Perylene-d12	22.11	264	14202	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.96	96	4322	2.19	ng/uL	0.00
6) 2-Methylnaphthalene-d10	11.07	152	5841	0.36	ng/ul	0.00
16) Fluoranthene-d10	18.07	212	14814	0.37	ng/ul	0.00
Target Compounds				Ovalue		
3) 1,4-Dioxane	2.97	88	4732	2.12	ng/ul#	65
5) Naphthalene	9.61	128	12030	0.41	ng/ul	99
7) 2-Methylnaphthalene	11.14	142	6646	0.35	ng/ul	87
9) Acenaphthylene	13.12	152	10323	0.42	ng/ul	98
10) Acenaphthene	13.43	153	7164	0.43	ng/ul#	84
11) Fluorene	14.42	166	9483	0.44	ng/ul	95
13) Pentachlorophenol	15.86	266	943	0.69	ng/ul	97
14) Phenanthrene	16.12	178	66548	0.40	ng/ul	99
15) Anthracene	16.21	178	62839	0.42	ng/ul	98
17) Fluoranthene	18.10	202	82523	0.43	ng/ul	88
19) Pyrene	18.49	202	76050	0.36	ng/ul#	79
20) Benzo(a)anthracene	20.20	228	17382	0.36	ng/ul	98
21) Chrysene	20.26	228	21941	0.40	ng/ul	98
23) Benzo(b)fluoranthene	21.56	252	18542	0.42	ng/ul	94
24) Benzo(k)fluoranthene	21.58	252	20068	0.44	ng/ul	94
25) Benzo(a)pyrene	22.02	252	17272	0.42	ng/ul	93
26) Indeno(1,2,3-cd)pyrene	23.71	276	72007	0.42	ng/ul#	91
27) Dibenzo(a,h)anthracene	23.66	278	16831	0.41	ng/ul#	71
28) Benzo(g,h,i)perylene	24.26	276	74878	0.41	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112015\
Data File : BE091256.D
Acq On : 20 Nov 2015 22:33
Operator : UM/NP
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTD0.478

Quant Time: Nov 21 02:54:49 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 21 02:52:22 2015
Response via : Initial Calibration

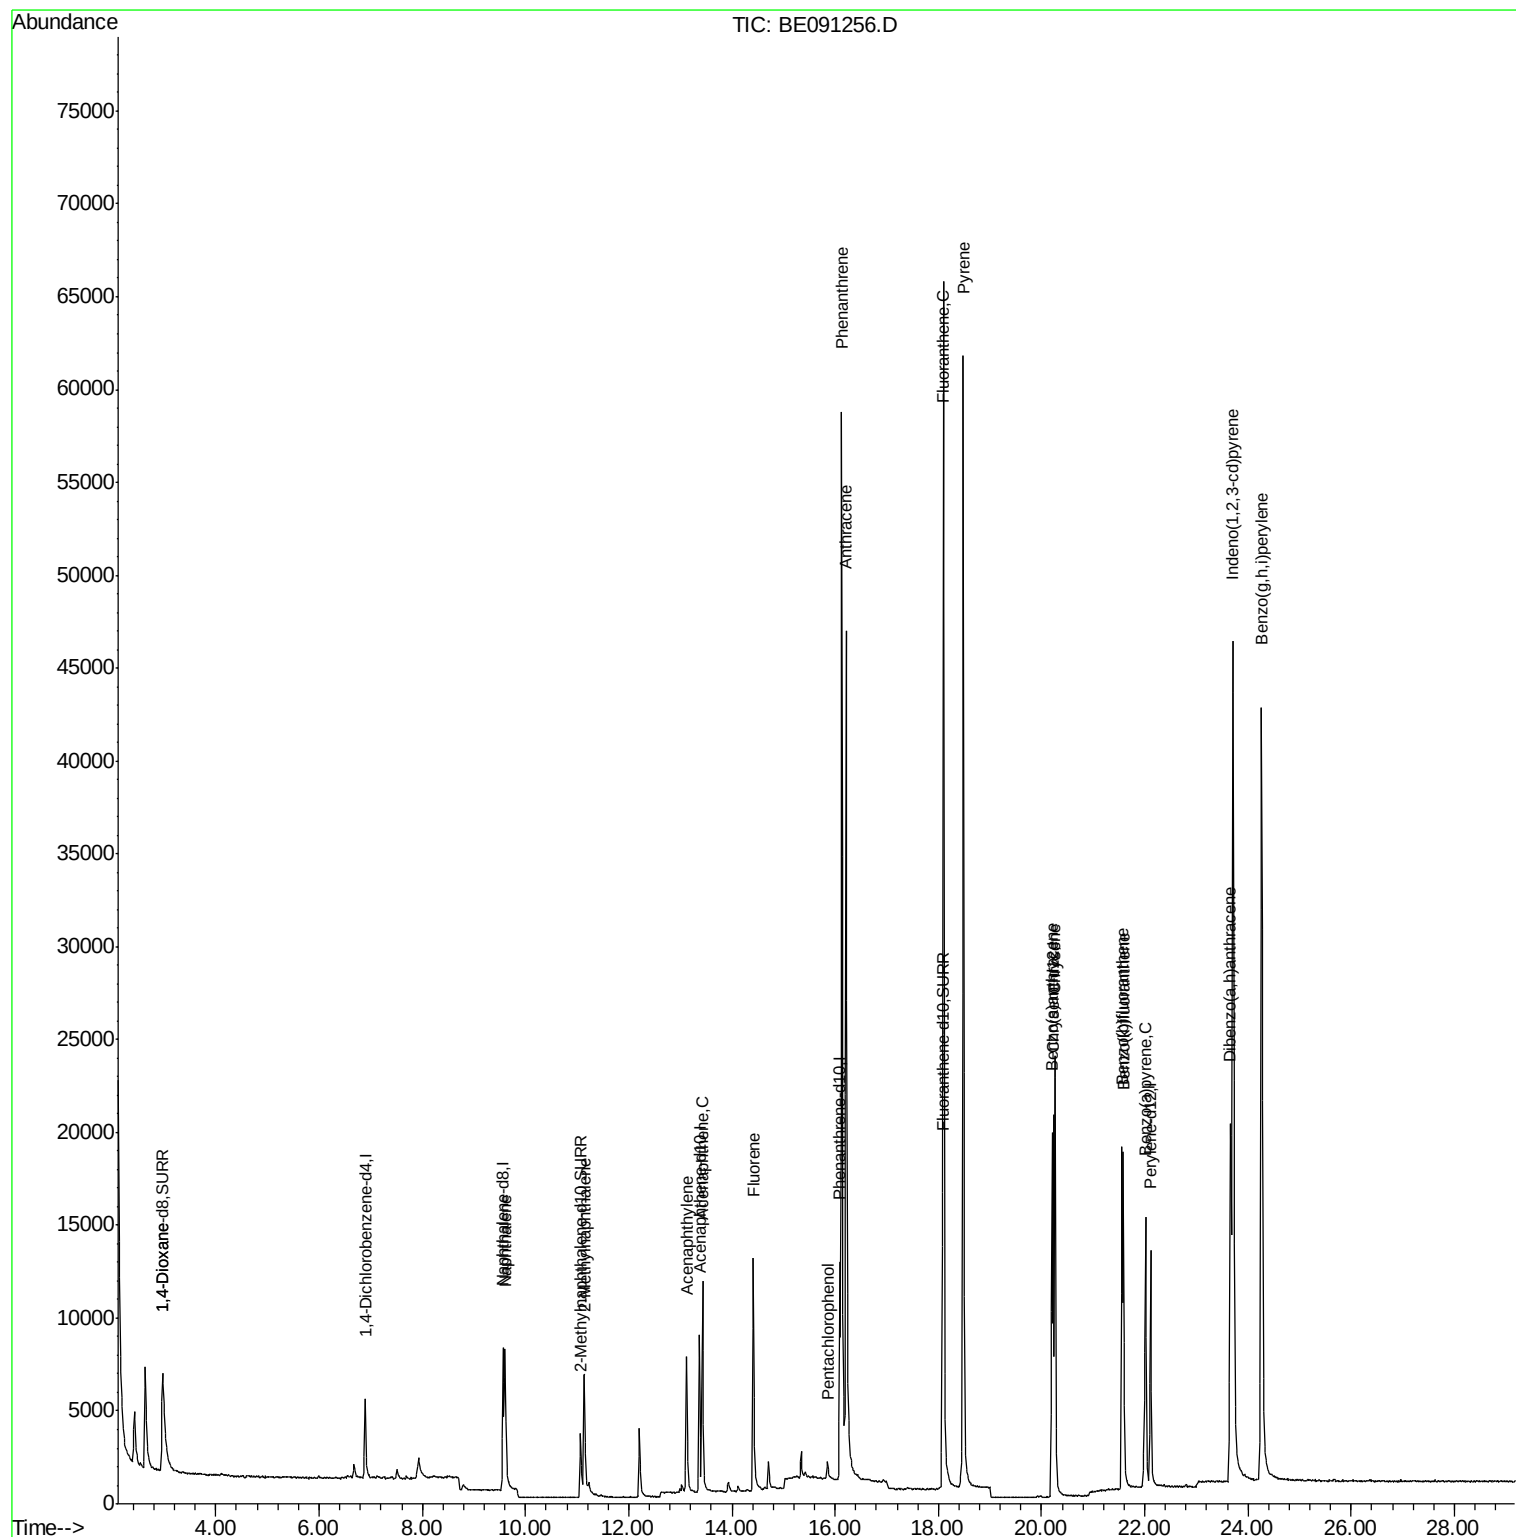

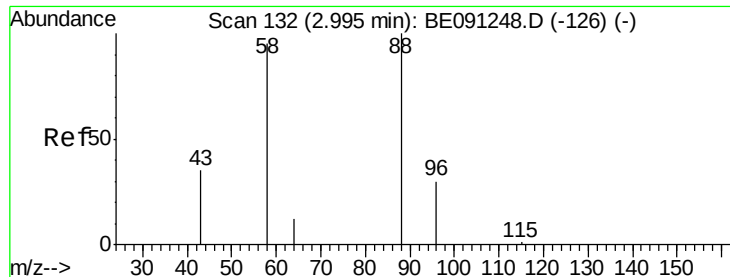

#3

1,4-Dioxane

Concen: 2.12 ng/ul

RT: 2.97 min Scan# 129

Delta R.T. -0.02 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33

Instrument :

BNA_E

ClientSampleId :

SSTD0.478


Tot Ion: 88 Resp: 4732

Ion Ratio Lower Upper

88 100

58 104.4 55.4 83.2#




43 39.8 24.2 36.2#

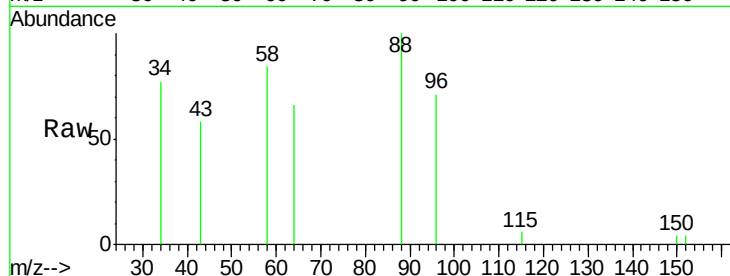

Abundance Ion 88.00 (87.70 to 88.70): BE091248.D (-126) (-)

Ion 58.00 (57.70 to 58.70): BE091248.D (-126) (-)

Ion 43.00 (42.70 to 43.70): BE091248.D (-126) (-)

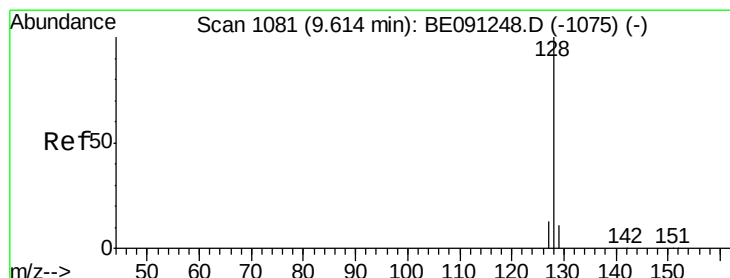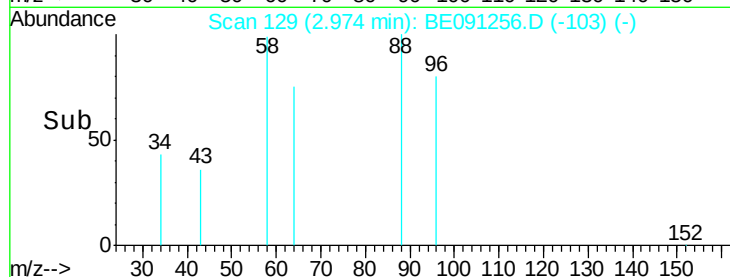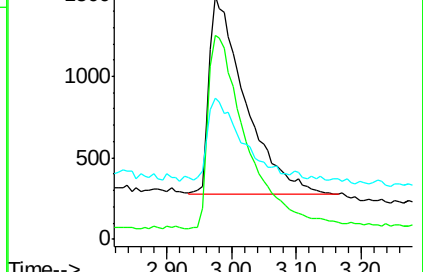

#5

Naphthalene

Concen: 0.41 ng/ul

RT: 9.61 min Scan# 1080

Delta R.T. -0.01 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33


Tgt Ion: 128 Resp: 12030

Ion Ratio Lower Upper

128 100

129 12.1 9.8 14.8



127 14.4 10.7 16.1

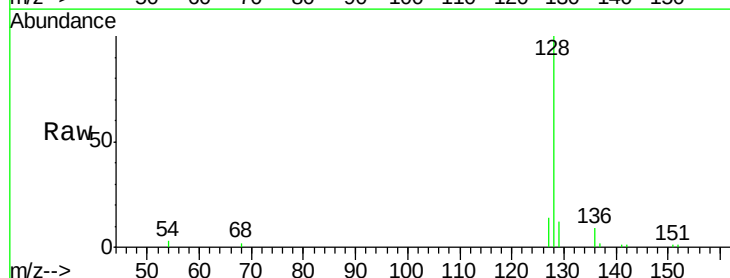


Abundance Ion 128.00 (127.70 to 128.70): BE091248.D (-1075) (-)

Ion 129.00 (128.70 to 129.70): BE091248.D (-1075) (-)

Ion 127.00 (126.70 to 127.70): BE091248.D (-1075) (-)

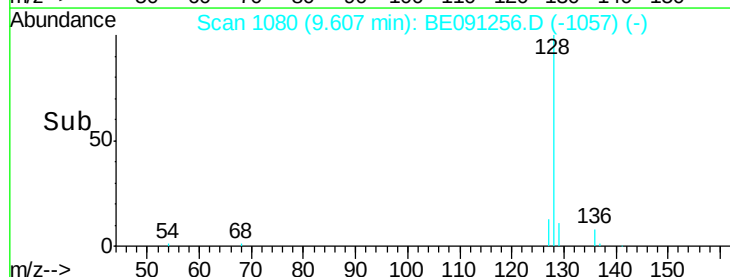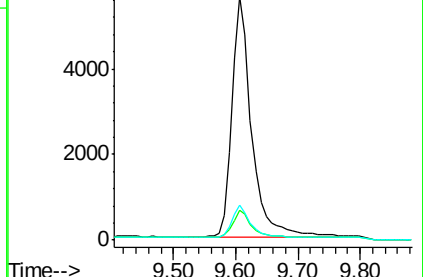

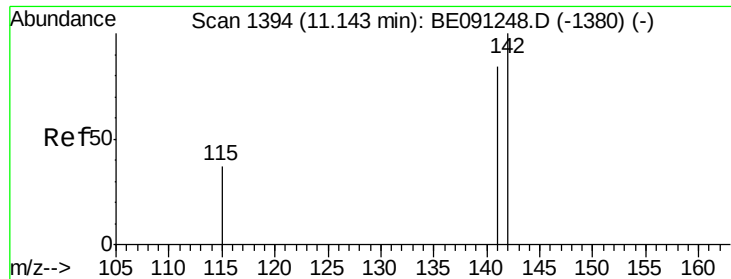

#7

2-Methylnaphthalene

Concen: 0.35 ng/ul

RT: 11.14 min Scan# 1393

Delta R.T. -0.00 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33

Instrument :

BNA_E

ClientSampleId :


SSTD0.478

Tot Ion:142 Resp: 6646

Ion Ratio Lower Upper

142 100

141 99.7 70.3 105.5

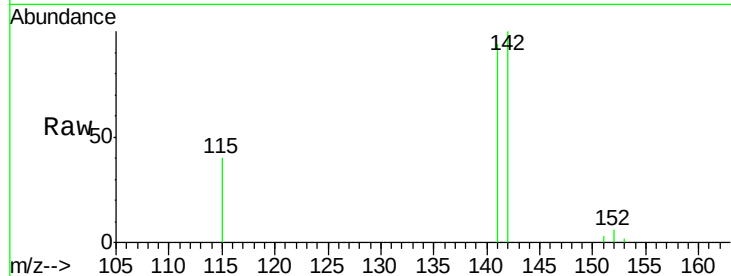

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

11.14



3000

2000

1000

0

Time--> 11.05 11.10 11.15 11.20

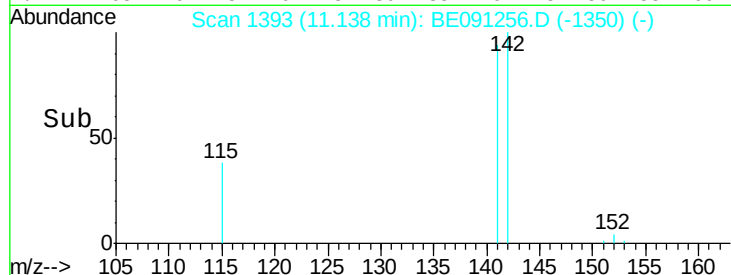

#9

Acenaphthylene

Concen: 0.42 ng/ul

RT: 13.12 min Scan# 1781

Delta R.T. -0.00 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33


Tgt Ion:152 Resp: 10323

Ion Ratio Lower Upper

152 100

151 20.1 16.8 25.2

153 14.6 11.3 16.9



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

13.12


6000


4000

2000

0

Time--> 13.00 13.10 13.20 13.30





#10

Acenaphthene

Concen: 0.43 ng/ul

RT: 13.43 min Scan# 1822

Delta R.T. -0.00 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33

Instrument :

BNA_E

ClientSampleId :

SSTD0.478





Tot Ion:153 Resp: 7164

Ion Ratio Lower Upper

153 100

152 67.5 42.3 63.5#

154 93.1 64.7 97.1

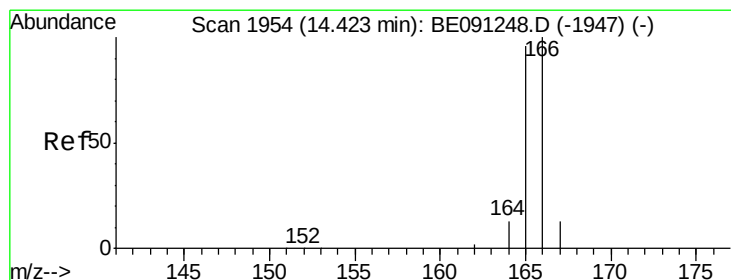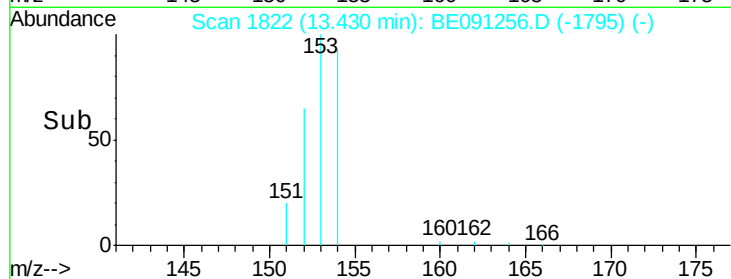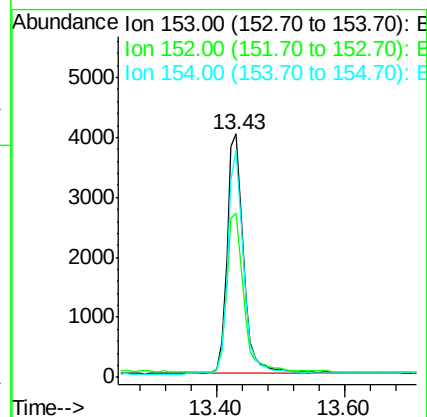

#11

Fluorene

Concen: 0.44 ng/ul

RT: 14.42 min Scan# 1953

Delta R.T. -0.01 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33




Tgt Ion:166 Resp: 9483


Ion Ratio Lower Upper

166 100

165 104.2 87.6 131.4

167 14.7 11.1 16.7



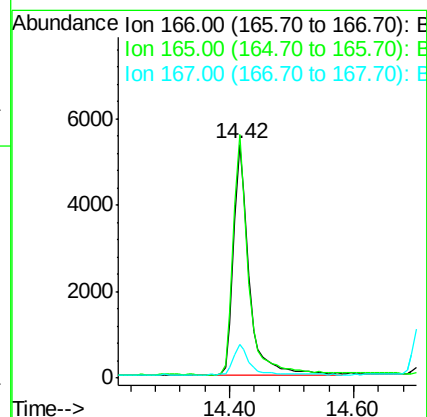



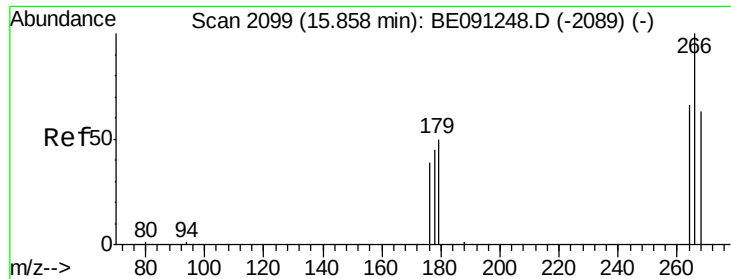

#13
 Pentachlorophenol
 Concen: 0.69 ng/ul
 RT: 15.86 min Scan# 2099
 Delta R.T. -0.00 min
 Lab File: BE091256.D
 Acq: 20 Nov 2015 22:33




Instrument :
 BNA_E
 ClientSampleId :
 SST0.478


Tot Ion:266 Resp: 943
 Ion Ratio Lower Upper
 266 100
 264 64.9 53.5 80.3
 268 64.7 54.2 81.2

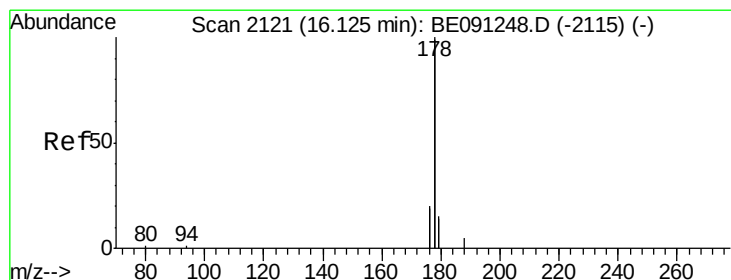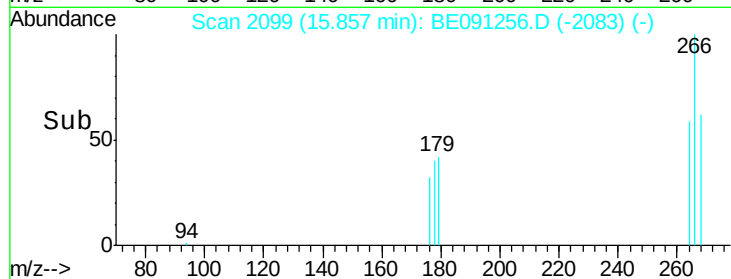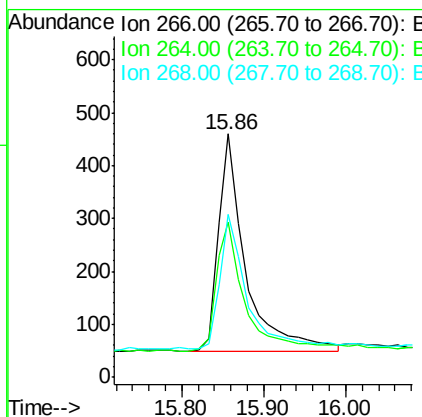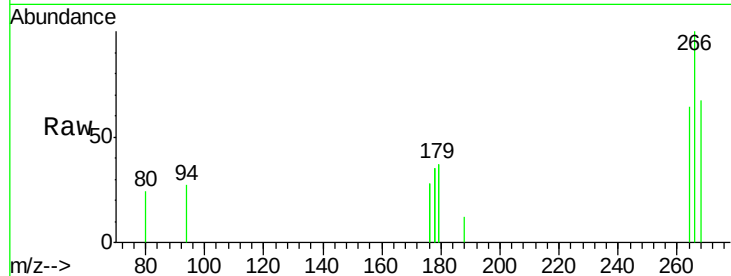

#14
 Phenanthrene
 Concen: 0.40 ng/ul
 RT: 16.12 min Scan# 2121
 Delta R.T. -0.00 min
 Lab File: BE091256.D
 Acq: 20 Nov 2015 22:33

Tgt Ion:178 Resp: 66548
 Ion Ratio Lower Upper
 178 100
 176 20.2 16.2 24.4
 179 15.6 12.8 19.2

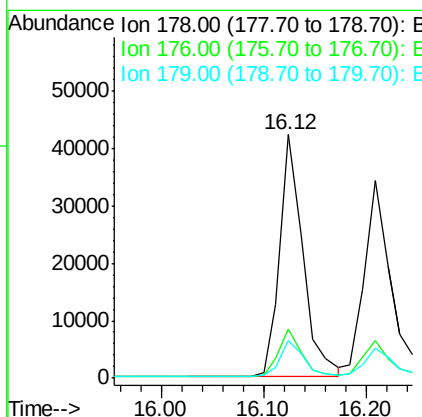

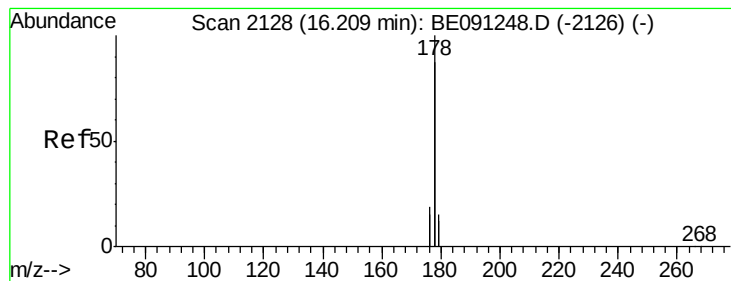

#15

Anthracene

Concen: 0.42 ng/ul

RT: 16.21 min Scan# 2128

Delta R.T. -0.00 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33

Instrument :

BNA_E

ClientSampleId :

SSTD0.478


Tot Ion:178 Resp: 62839

Ion Ratio Lower Upper

178 100

176 19.3 15.8 23.8




179 15.2 13.3 19.9



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

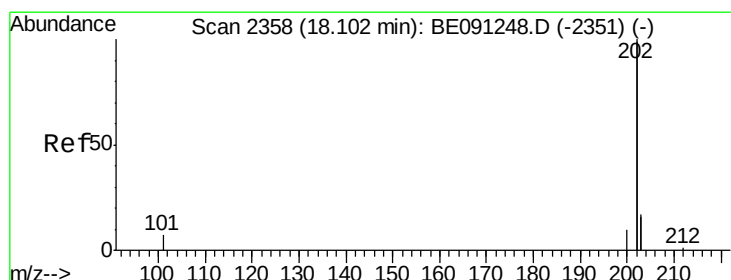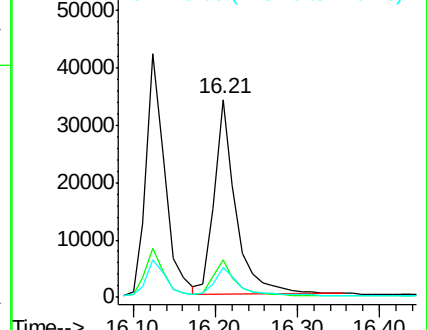

#17

Fluoranthene

Concen: 0.43 ng/ul

RT: 18.10 min Scan# 2358

Delta R.T. -0.00 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33


Tgt Ion:202 Resp: 82523

Ion Ratio Lower Upper

202 100

101 3.6 0.0 33.1



203 18.2 0.0 37.2




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

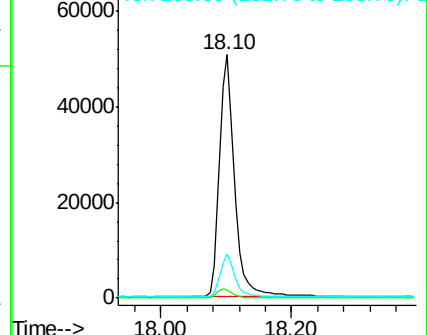



#19

Pvrene

Concen: 0.36 ng/ul

RT: 18.49 min Scan# 2417

Delta R.T. -0.00 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33

Instrument :

BNA_E

ClientSampleId :

SSTD0.478





Tot Ion:202 Resp: 76050

Ion Ratio Lower Upper

202 100

200 5.5 18.0 27.0#

203 17.9 13.8 20.6

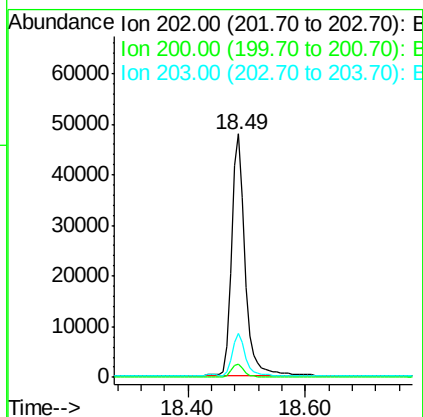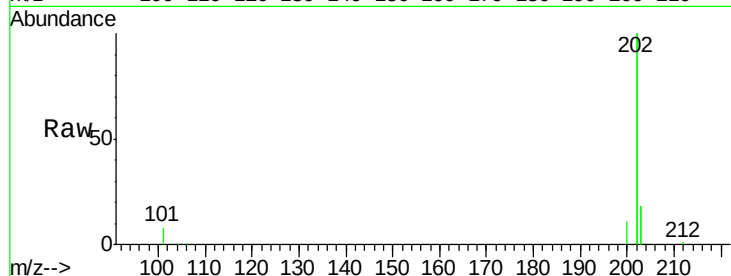

#20

Benzo(a)anthracene

Concen: 0.36 ng/ul

RT: 20.20 min Scan# 2756

Delta R.T. -0.00 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33




Tgt Ion:228 Resp: 17382


Ion Ratio Lower Upper

228 100

226 28.0 23.0 34.4

229 20.0 15.2 22.8

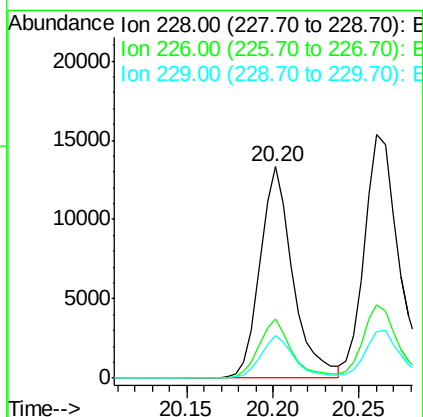

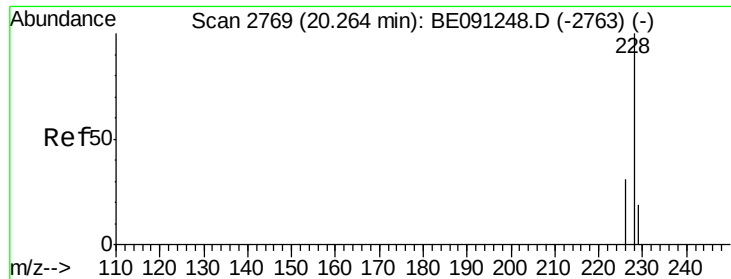

#21

Chrysene

Concen: 0.40 ng/ul

RT: 20.26 min Scan# 2769

Delta R.T. -0.00 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33

Instrument :

BNA_E

ClientSampleId :

SSTD0.478


Tot Ion:228 Resp: 21941

Ion Ratio Lower Upper

228 100

226 30.3 25.7 38.5




229 19.3 15.2 22.8



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

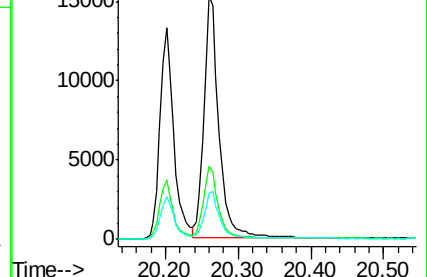

#23

Benzo(b)fluoranthene

Concen: 0.42 ng/ul

RT: 21.56 min Scan# 3050

Delta R.T. 0.00 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33


Tgt Ion:252 Resp: 18542

Ion Ratio Lower Upper

252 100

253 22.7 0.0 48.0



125 13.4 0.0 36.6




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

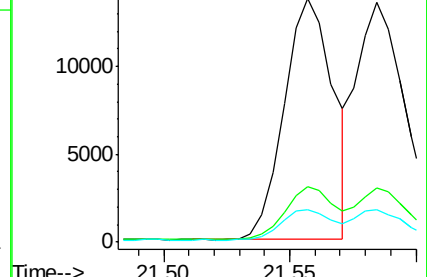

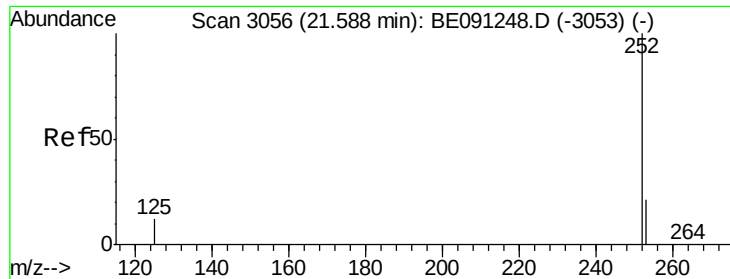

#24

Benzo(k)fluoranthene

Concen: 0.44 ng/ul

RT: 21.58 min Scan# 3056

Delta R.T. -0.00 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33

Instrument :

BNA_E

ClientSampleId :

SSTD0.478


Tot Ion:252 Resp: 20068

Ion Ratio Lower Upper

252 100

253 22.7 20.8 31.2




125 13.5 12.2 18.4

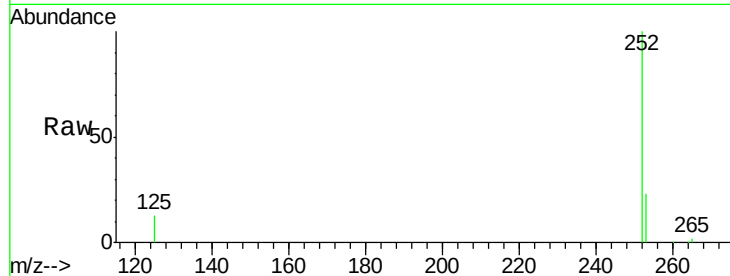

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

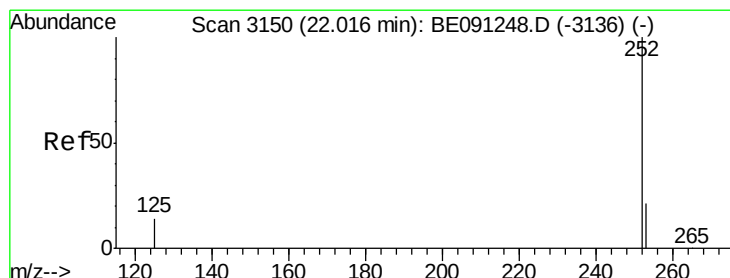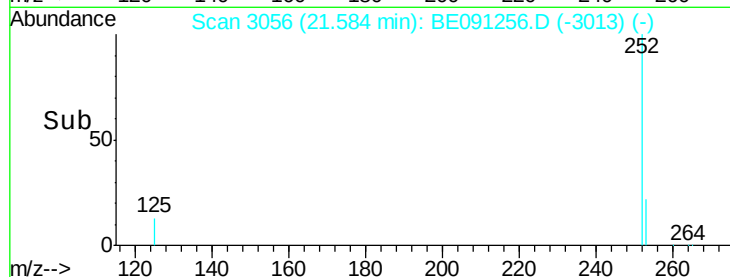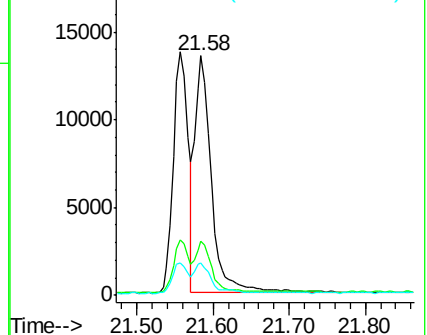

#25

Benzo(a)pyrene

Concen: 0.42 ng/ul

RT: 22.02 min Scan# 3151

Delta R.T. 0.00 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33


Tgt Ion:252 Resp: 17272

Ion Ratio Lower Upper

252 100

253 23.7 21.8 32.8



125 14.9 14.5 21.7

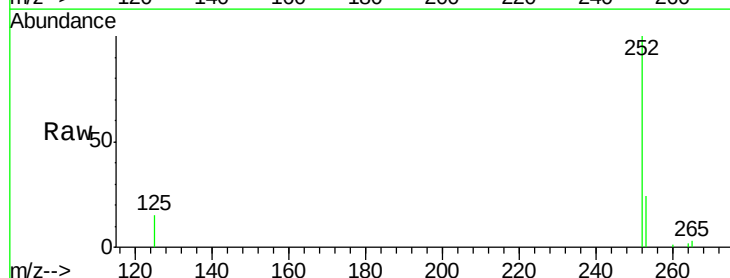


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

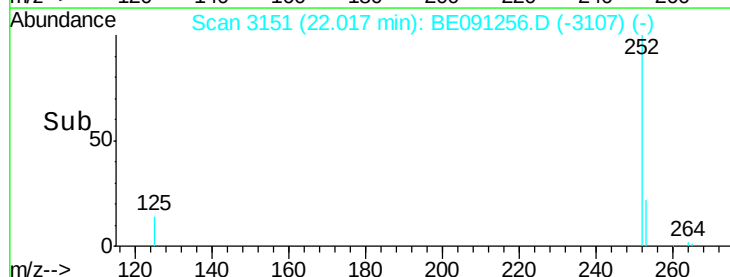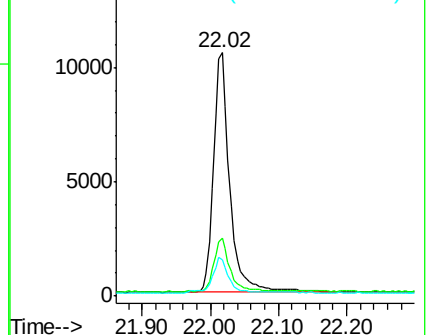

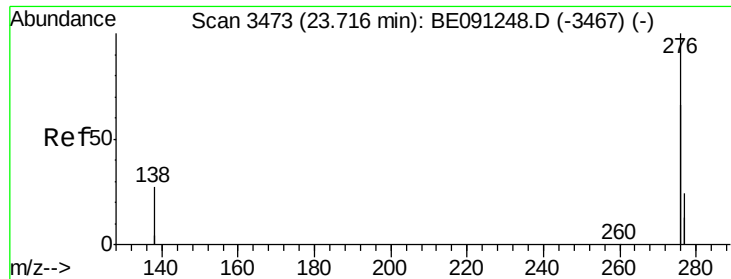

#26

Indeno(1,2,3-cd)pyrene

Concen: 0.42 ng/ul

RT: 23.71 min Scan# 3473

Delta R.T. -0.01 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33

Instrument :

BNA_E

ClientSampleId :

SSTD0.478





Tot Ion:276 Resp: 72007

Ion Ratio Lower Upper

276 100

138 26.0 27.5 41.3#

277 24.0 19.3 28.9

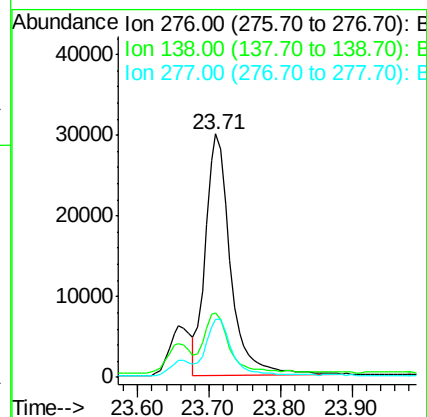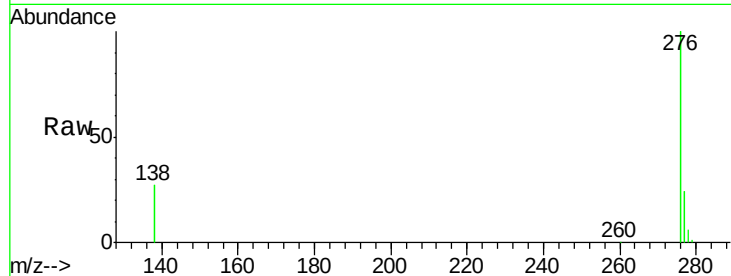

#27

Dibenzo(a,h)anthracene

Concen: 0.41 ng/ul

RT: 23.66 min Scan# 3466

Delta R.T. -0.01 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33




Tgt Ion:278 Resp: 16831


Ion Ratio Lower Upper

278 100

139 0.0 21.7 32.5#

279 24.4 21.9 32.9

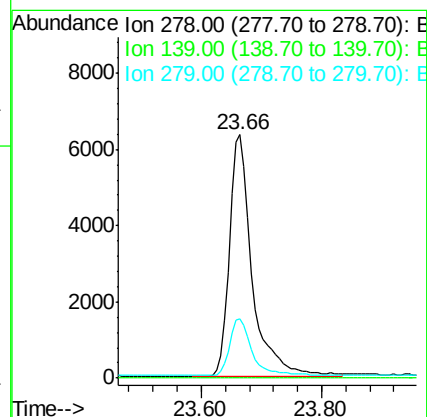



#28

Benzo(a,h,i)perylene

Concen: 0.41 ng/ul

RT: 24.26 min Scan# 3558

Delta R.T. 0.00 min

Lab File: BE091256.D

Acq: 20 Nov 2015 22:33

Instrument :

BNA_E

ClientSampleId :

SSTD0.478


Tot Ion: 276 Resp: 74878

Ion Ratio Lower Upper

276 100

277 23.8 21.3 31.9

138 28.0 25.5 38.3



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

