


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE112118\
 Data File : BE098253.D
 Acq On : 21 Nov 2018 9:00
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE111618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 16 19:05:33 2018

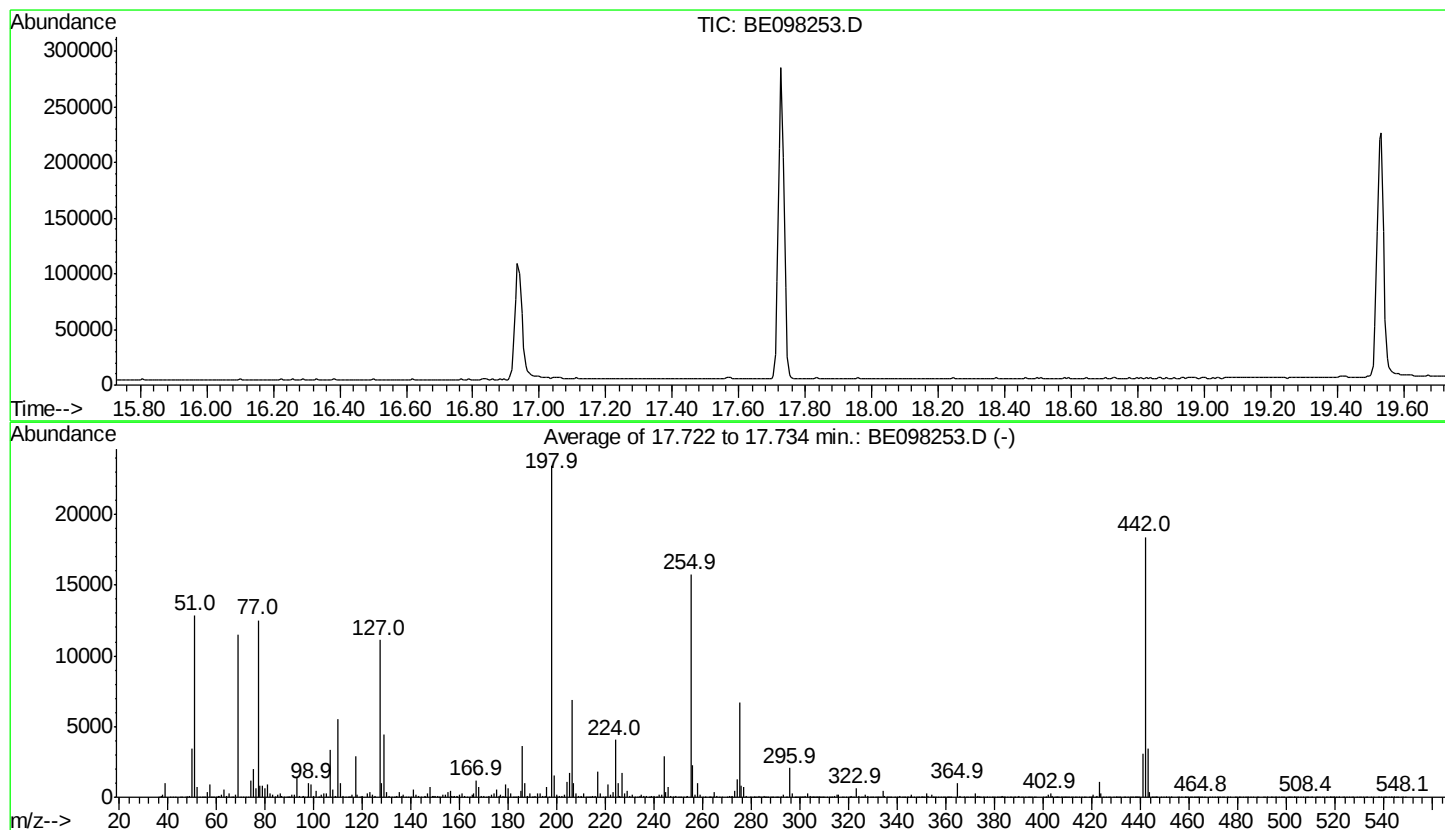

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.6	12817	PASS
68	69	0.00	2	1.8	205	PASS
69	198	0.00	100	49.1	11514	PASS
70	69	0.00	2	0.4	43	PASS
127	198	10	80	47.3	11097	PASS
197	198	0.00	2	0.1	35	PASS
198	198	100	100	100.0	23453	PASS
199	198	5	9	6.7	1562	PASS
275	198	10	60	28.7	6741	PASS
365	198	1	100	4.2	975	PASS
441	198	0.01	100	13.0	3052	PASS
442	198	50	100	78.4	18398	PASS
443	442	15	24	18.7	3435	PASS