


Instrument :
BNA_E
ClientSampleId :

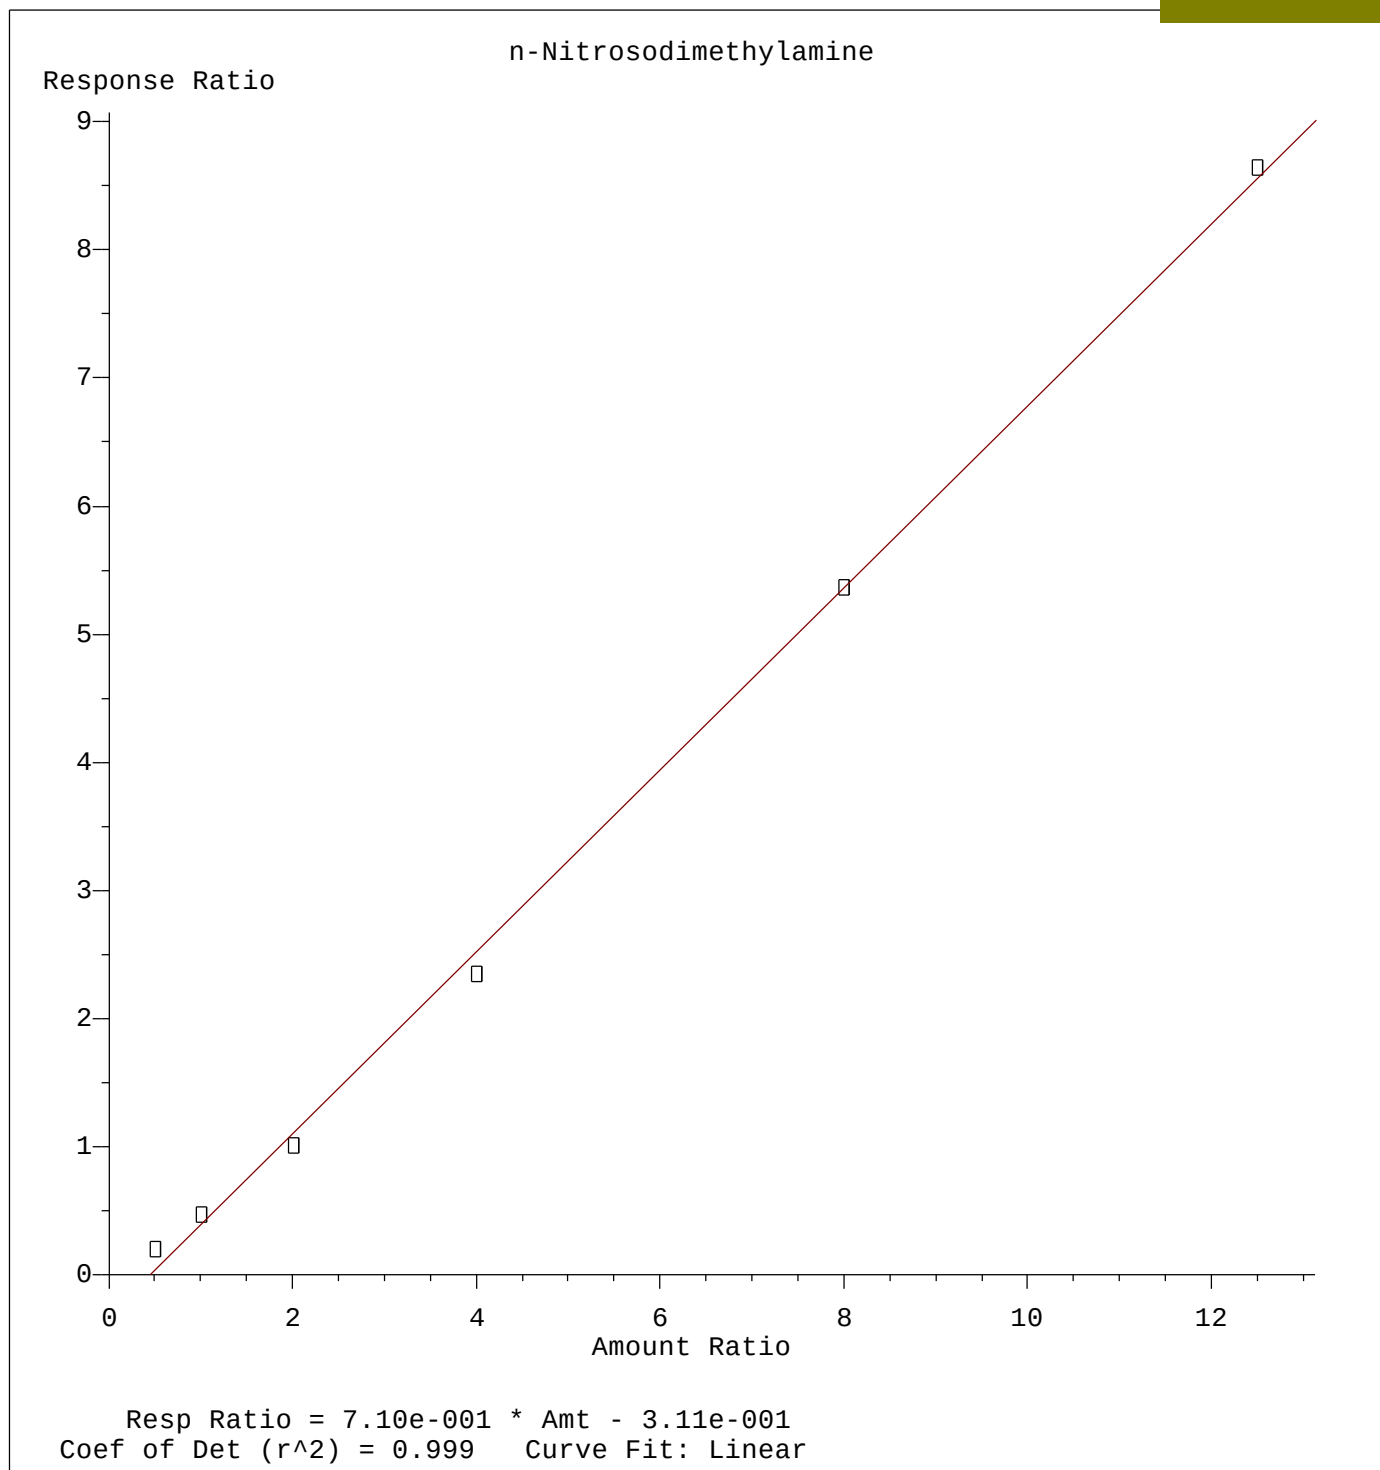


Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE112119.M
Calibration Table Last Updated: Fri Nov 22 06:40:44 2019

Instrument :
BNA_E
ClientSampleId :

Pentachlorophenol

Response Ratio

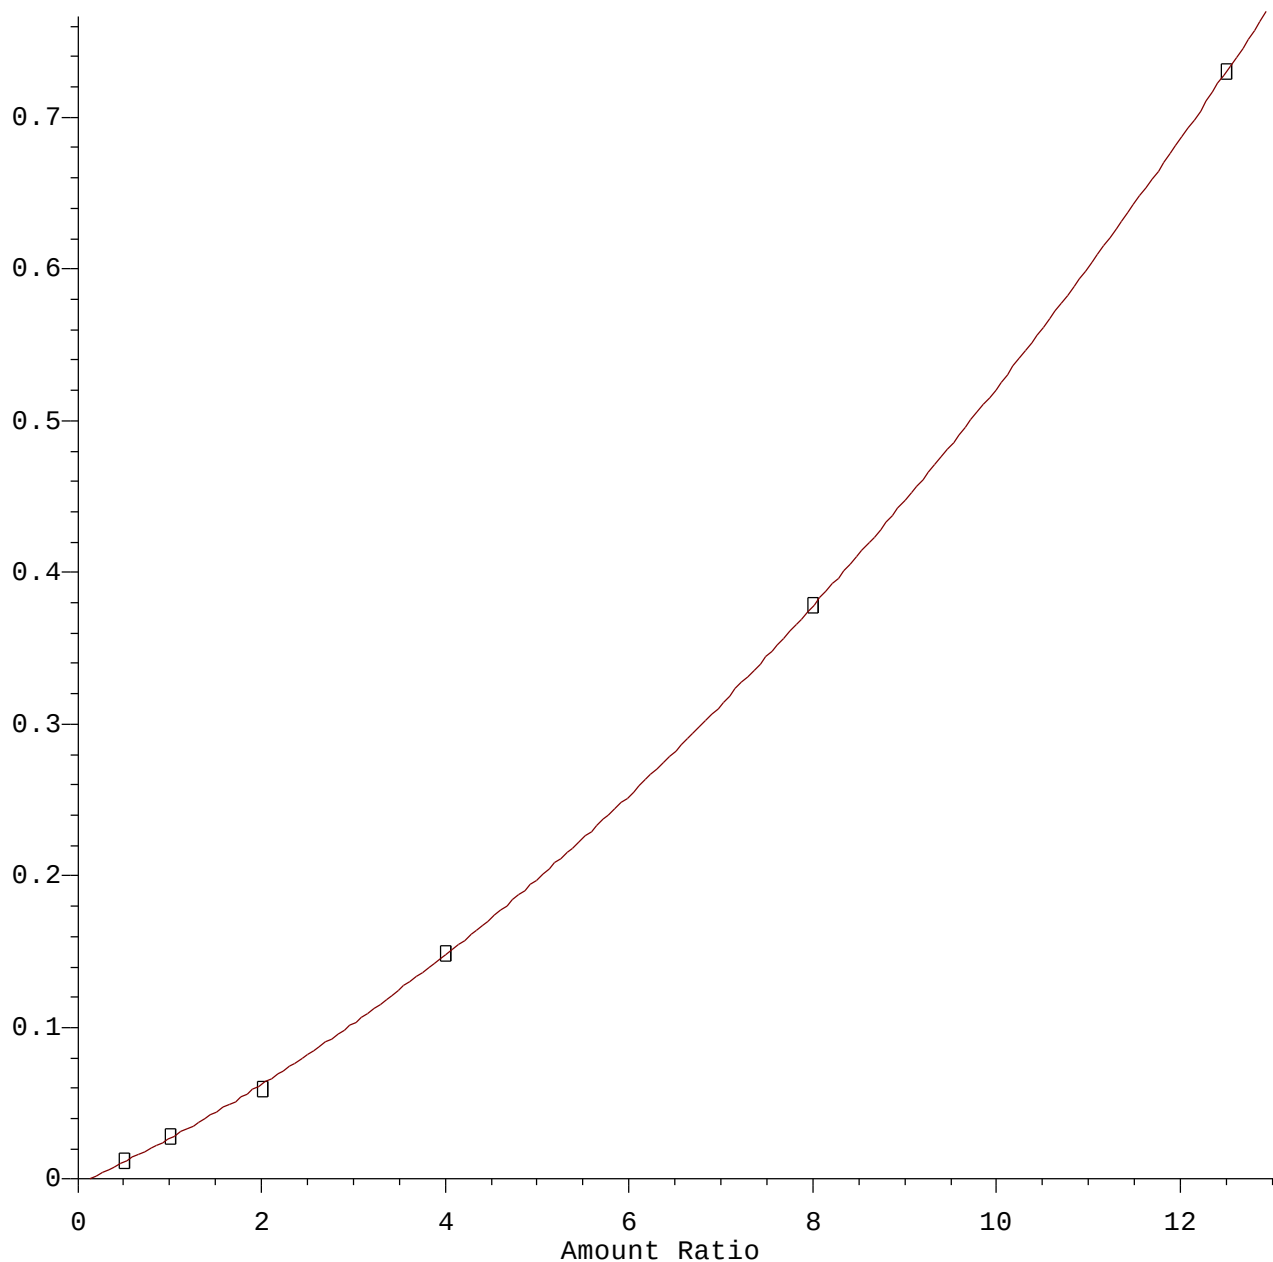


$R = 2.45e-003 A^2 + 2.81e-002 A - 3.73e-003$
Coef of Det (r^2) = 1.000 Curve Fit: Quadratic

Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE112119.M
Calibration Table Last Updated: Fri Nov 22 06:40:44 2019

Instrument :
BNA_E
ClientSampleId :

Bis(2-ethylhexyl)phthalate

Response Ratio

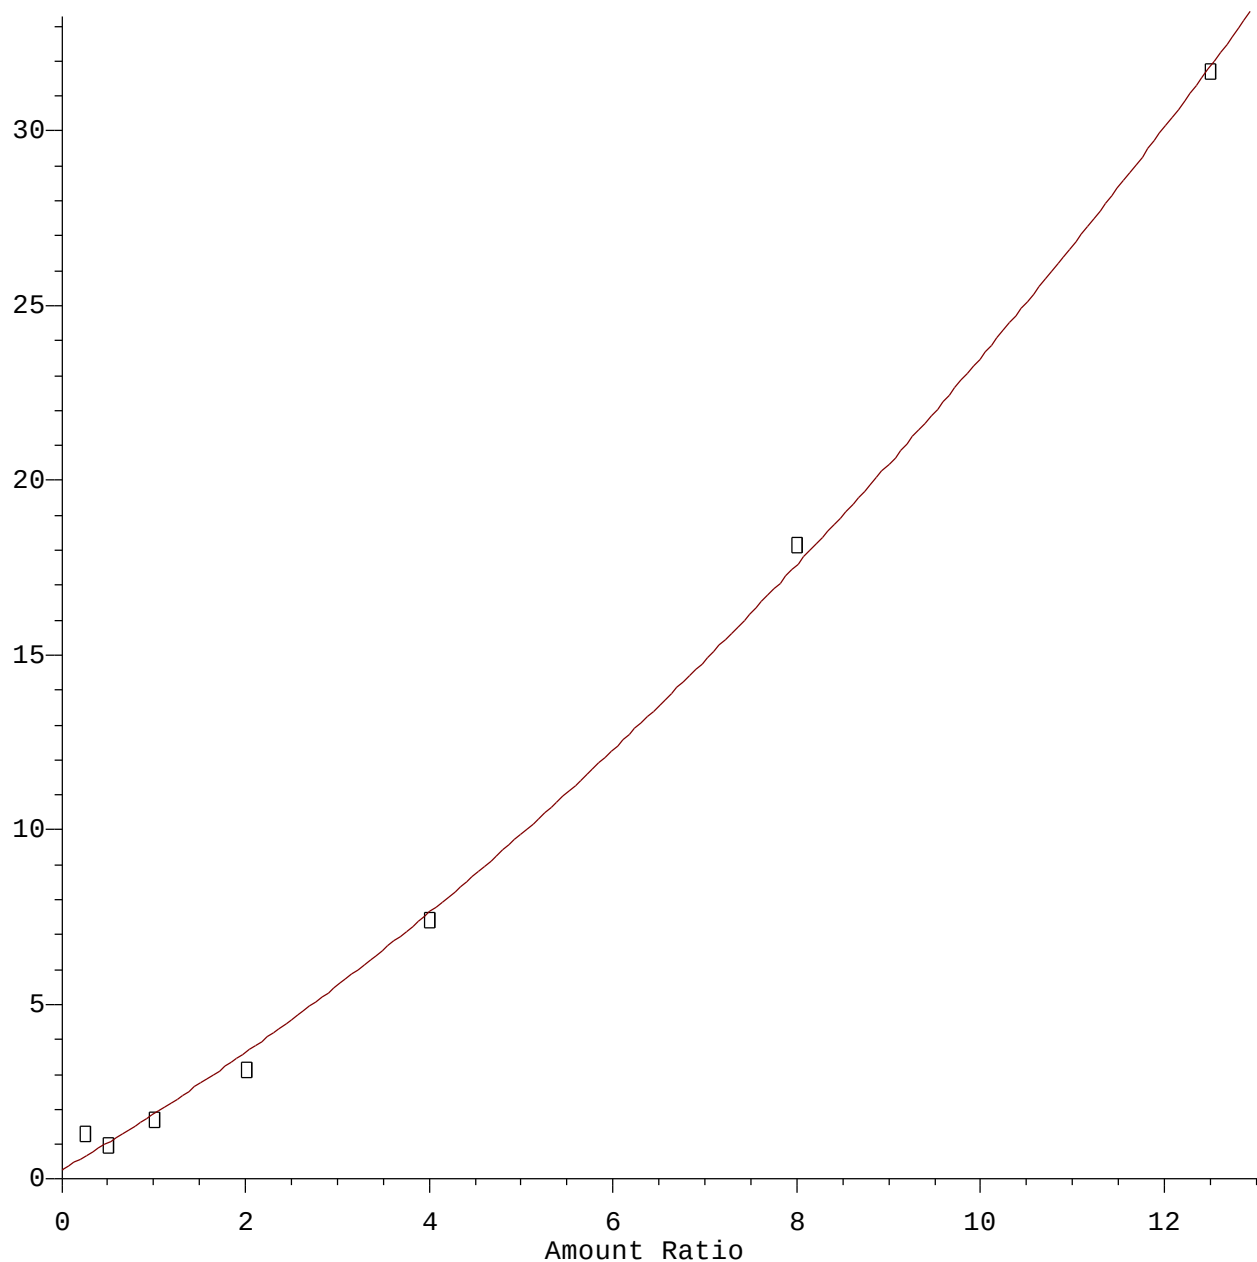


$R = 8.06e-002 A^2 + 1.52e+000 A + 2.62e-001$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic

Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE112119.M
Calibration Table Last Updated: Fri Nov 22 06:40:44 2019

Instrument :
BNA_E
ClientSampleId :

Indeno(1,2,3-cd)pyrene

Response Ratio

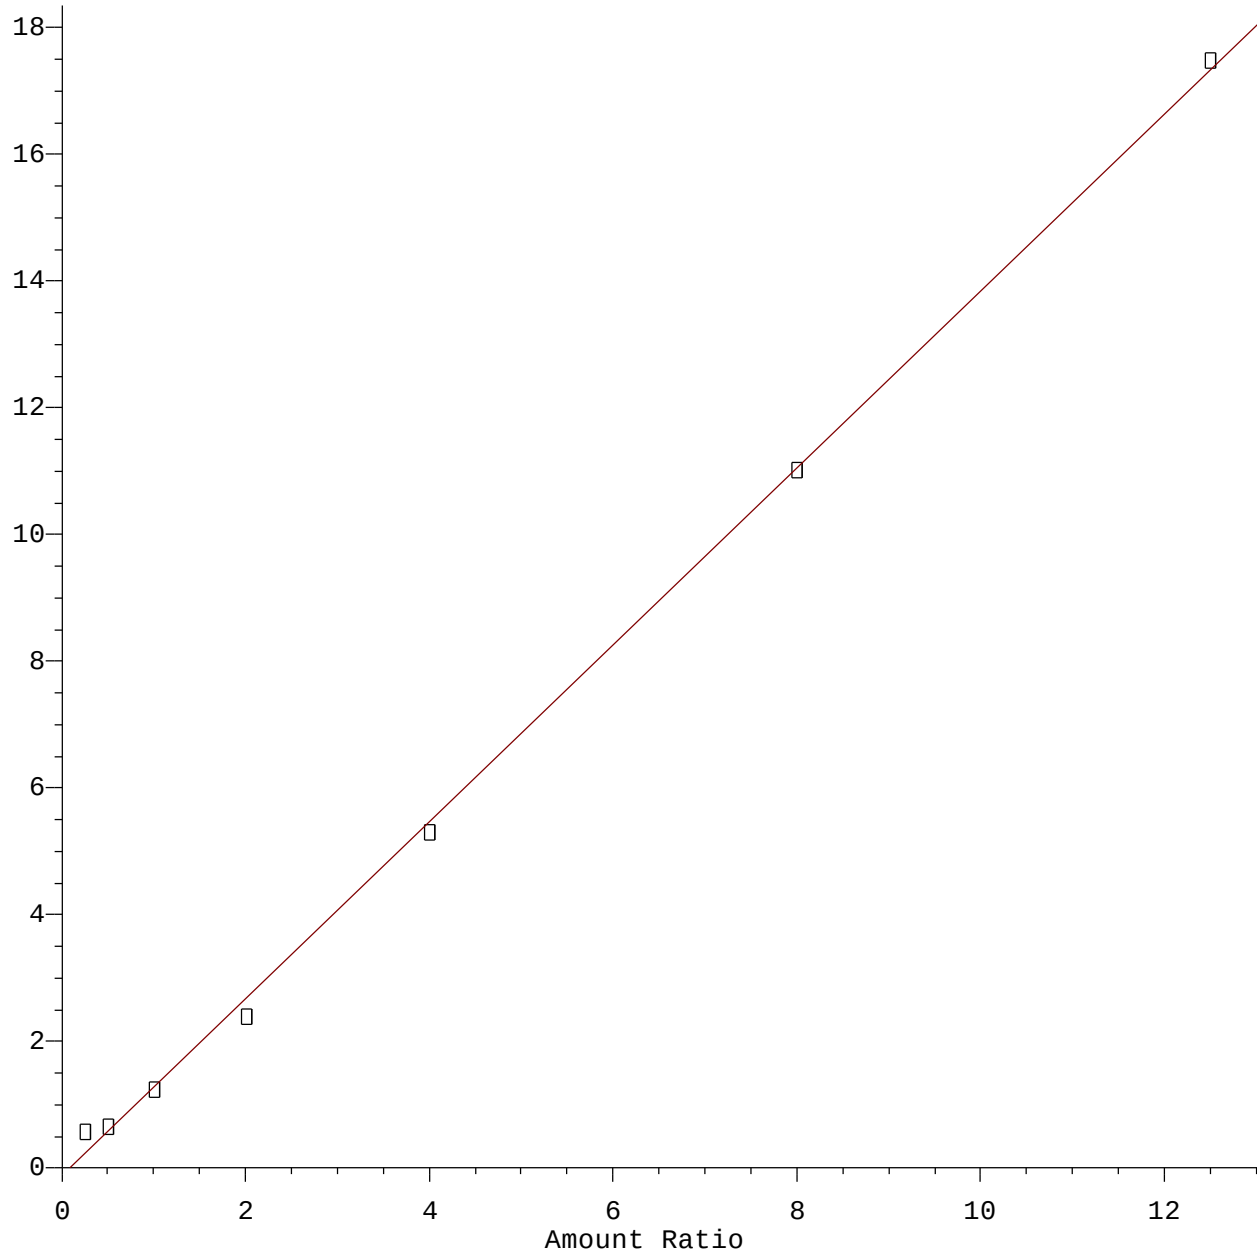


Resp Ratio = 1.40e+000 * Amt - 1.28e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE112119.M
Calibration Table Last Updated: Fri Nov 22 06:40:44 2019

Instrument :
BNA_E
ClientSampleId :

Benzo(g,h,i)perylene

Response Ratio

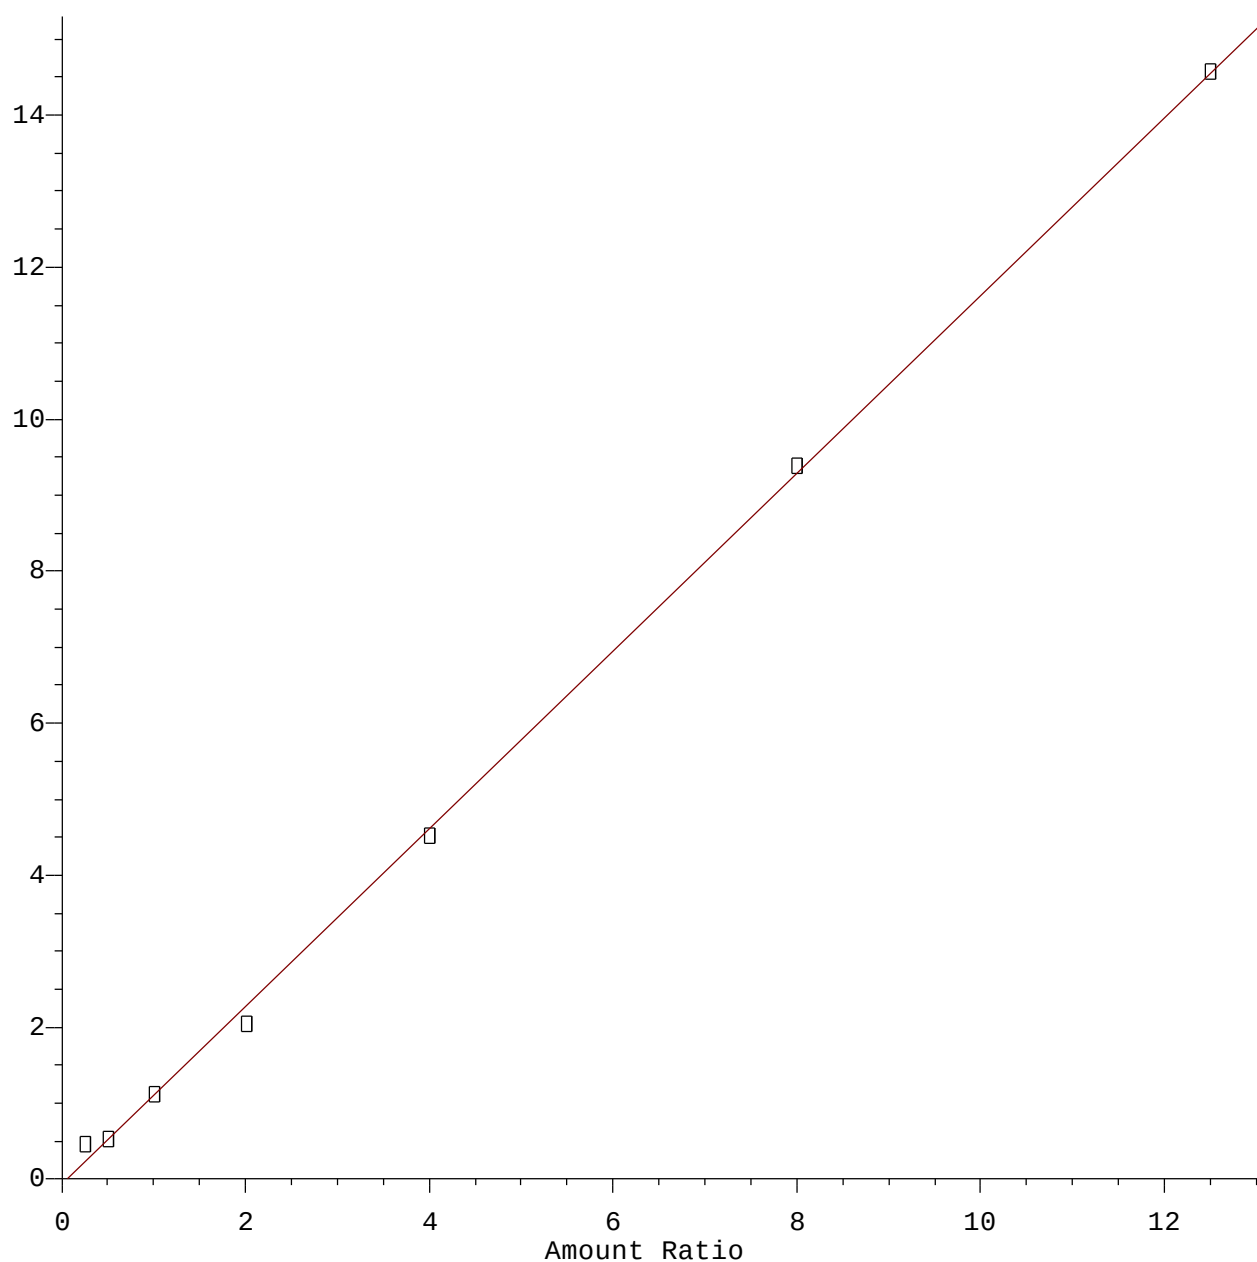

Resp Ratio = 1.17e+000 * Amt - 6.33e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE112119.M
Calibration Table Last Updated: Fri Nov 22 06:40:44 2019