


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE112119\
Data File : BE100746.D
Acq On : 21 Nov 2019 15:04
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE112119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 22 06:40:44 2019

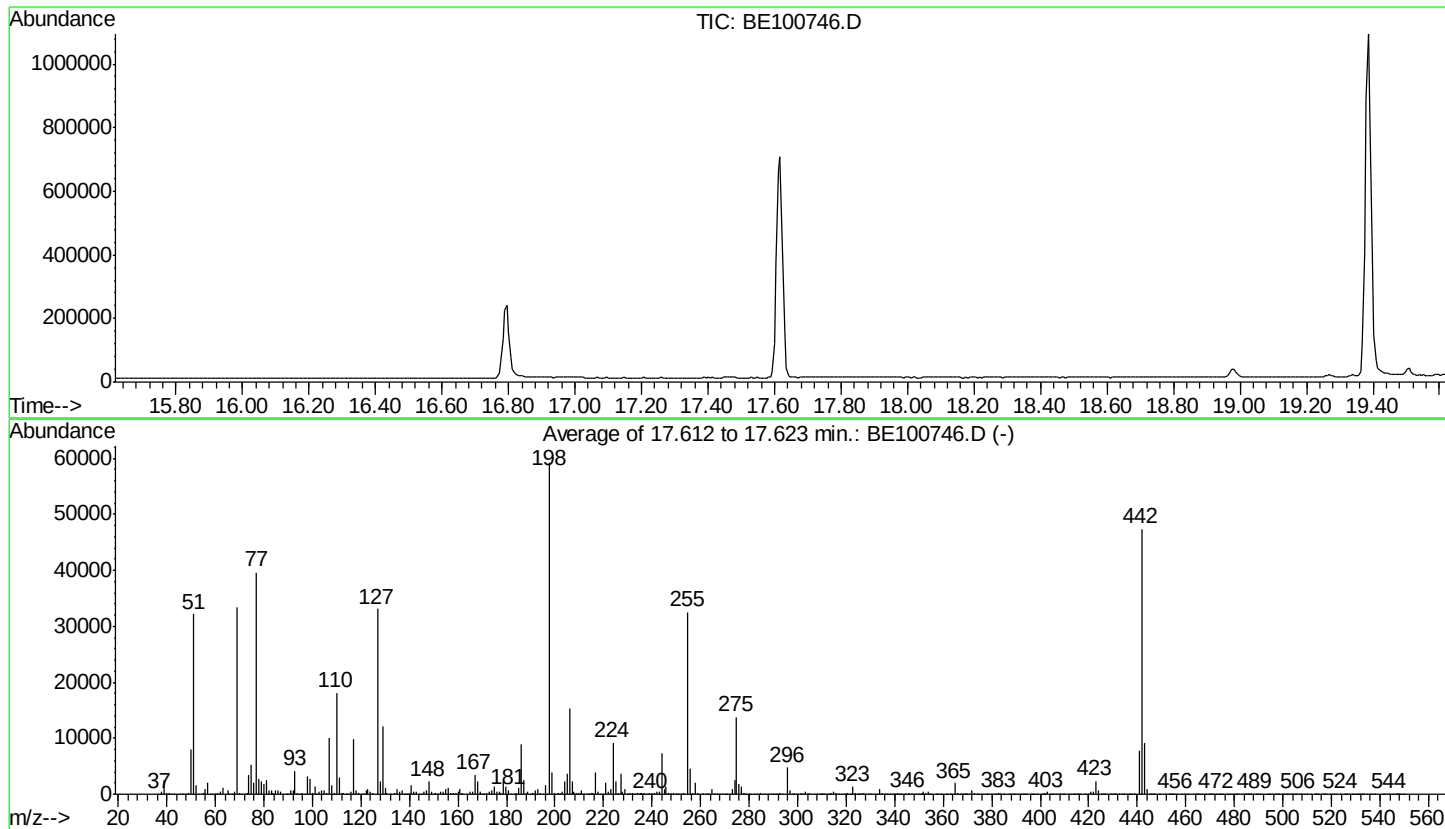

AutoFind: Scans 2557, 2558, 2559; Background Corrected with Scan 2547

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.3	32143	PASS
68	69	0.00	2	1.6	546	PASS
69	198	0.00	100	56.5	33442	PASS
70	69	0.00	2	0.7	250	PASS
127	198	10	80	55.9	33127	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59219	PASS
199	198	5	9	6.6	3927	PASS
275	198	10	60	23.2	13753	PASS
365	198	1	100	3.3	1963	PASS
441	198	0.01	100	13.2	7810	PASS
442	198	50	100	80.1	47413	PASS
443	442	15	24	19.4	9178	PASS