


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112215\
Data File : BE091293.D
Acq On : 22 Nov 2015 10:48
Operator : UM/NP
Sample : PB86663BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Nov 23 00:52:07 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 00:41:30 2015
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
SBLK63

Manual Integrations
APPROVED

Mmdadoda
11/23/2015 2:14:42 PM

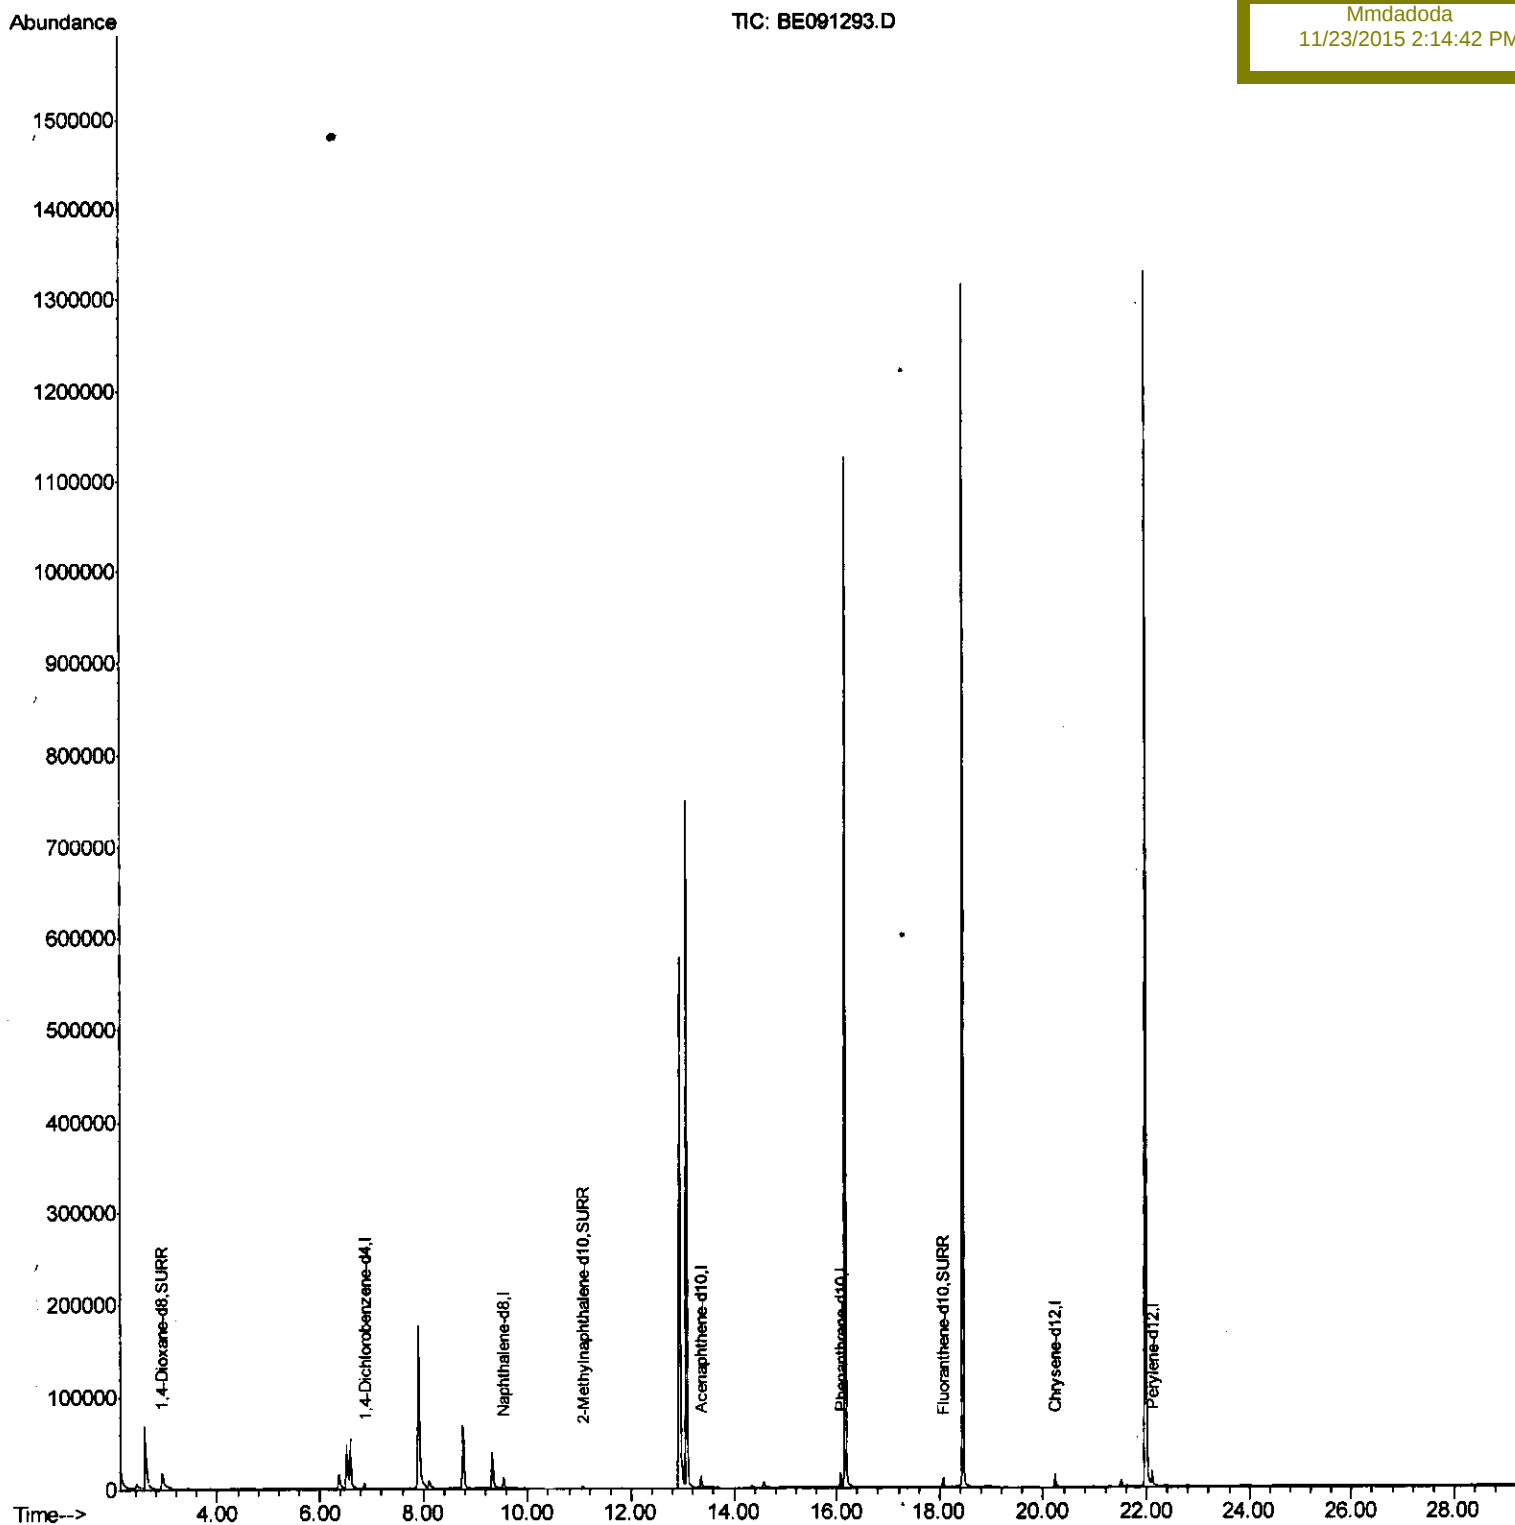


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112215\
 Data File : BE091293.D
 Acq On : 22 Nov 2015 10:48
 Operator : UM/NP
 Sample : PB86663BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Quant Time: Nov 23 00:52:07 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 00:41:30 2015
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 SBLK63

Manual Integrations
 APPROVED

Mmdadoda
 11/23/2015 2:14:42 PM

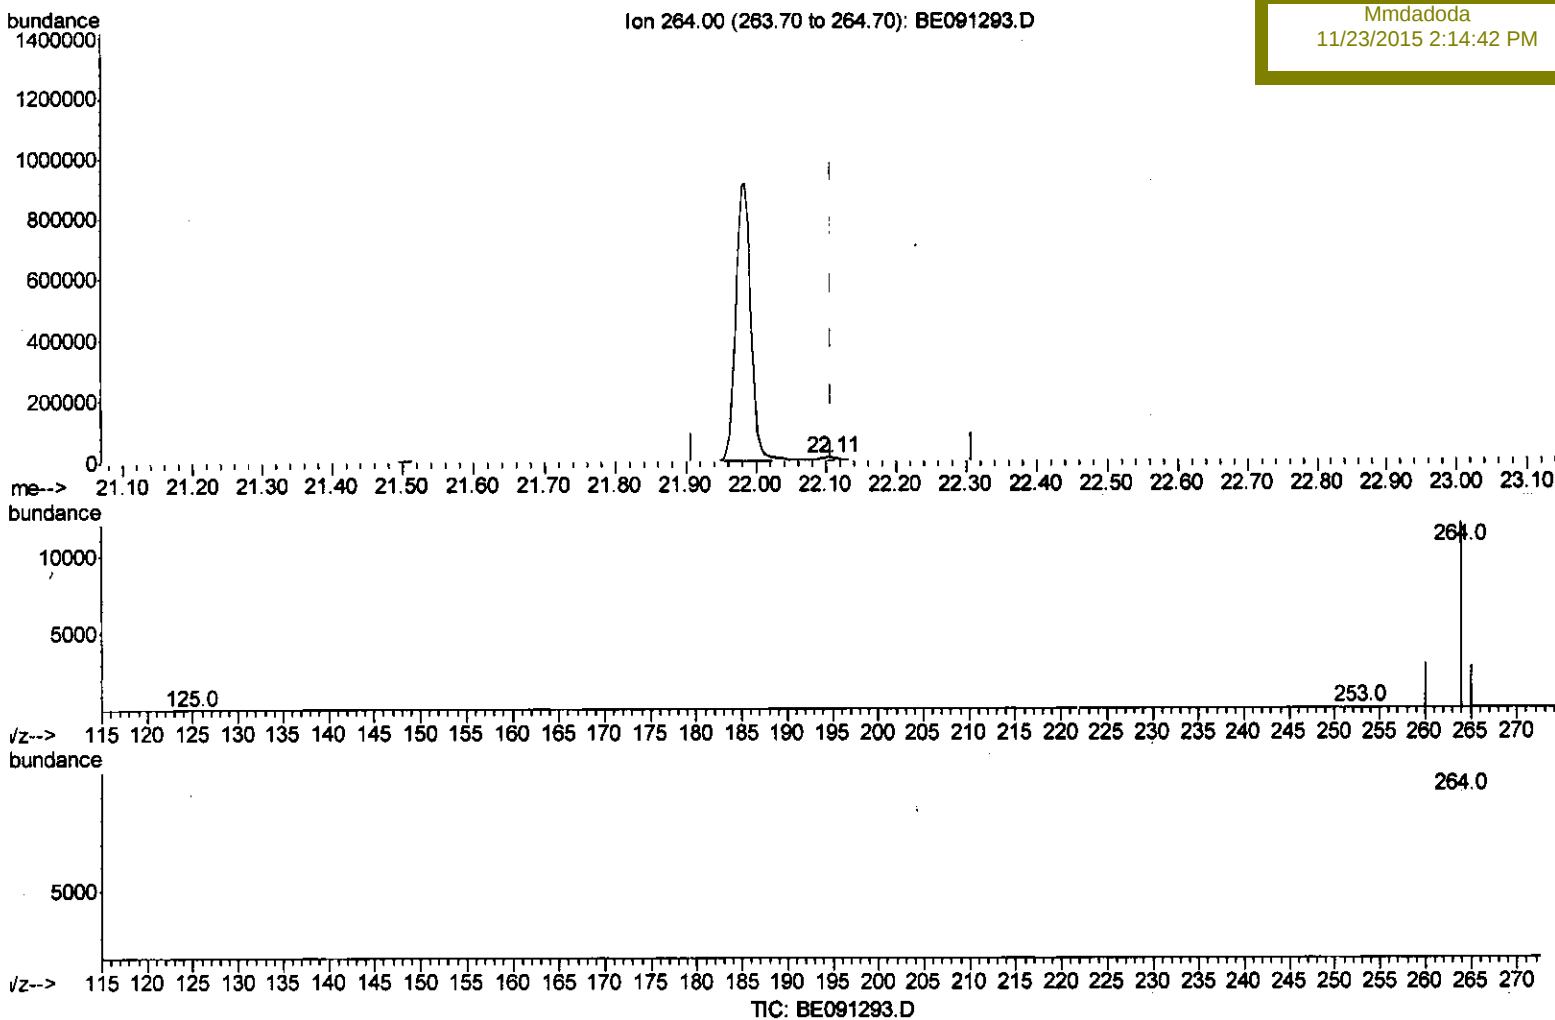

(22) Perylene-d12 (I)

22.107min (-0.001) 0.40ng/ul m

response 25208

Ion	Exp%	Act%
264.00	100	100
260.00	28.90	25.26
265.00	34.70	23.93#
0.00	0.00	0.00

U.M
 11/25/15


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112215\
 Data File : BE091293.D
 Acq On : 22 Nov 2015 10:48
 Operator : UM/NP
 Sample : PB86663BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Quant Time: Nov 23 00:45:04 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 00:41:30 2015
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 SBLK63

Manual Integrations
 APPROVED

Mmdadoda
 11/23/2015 2:14:42 PM

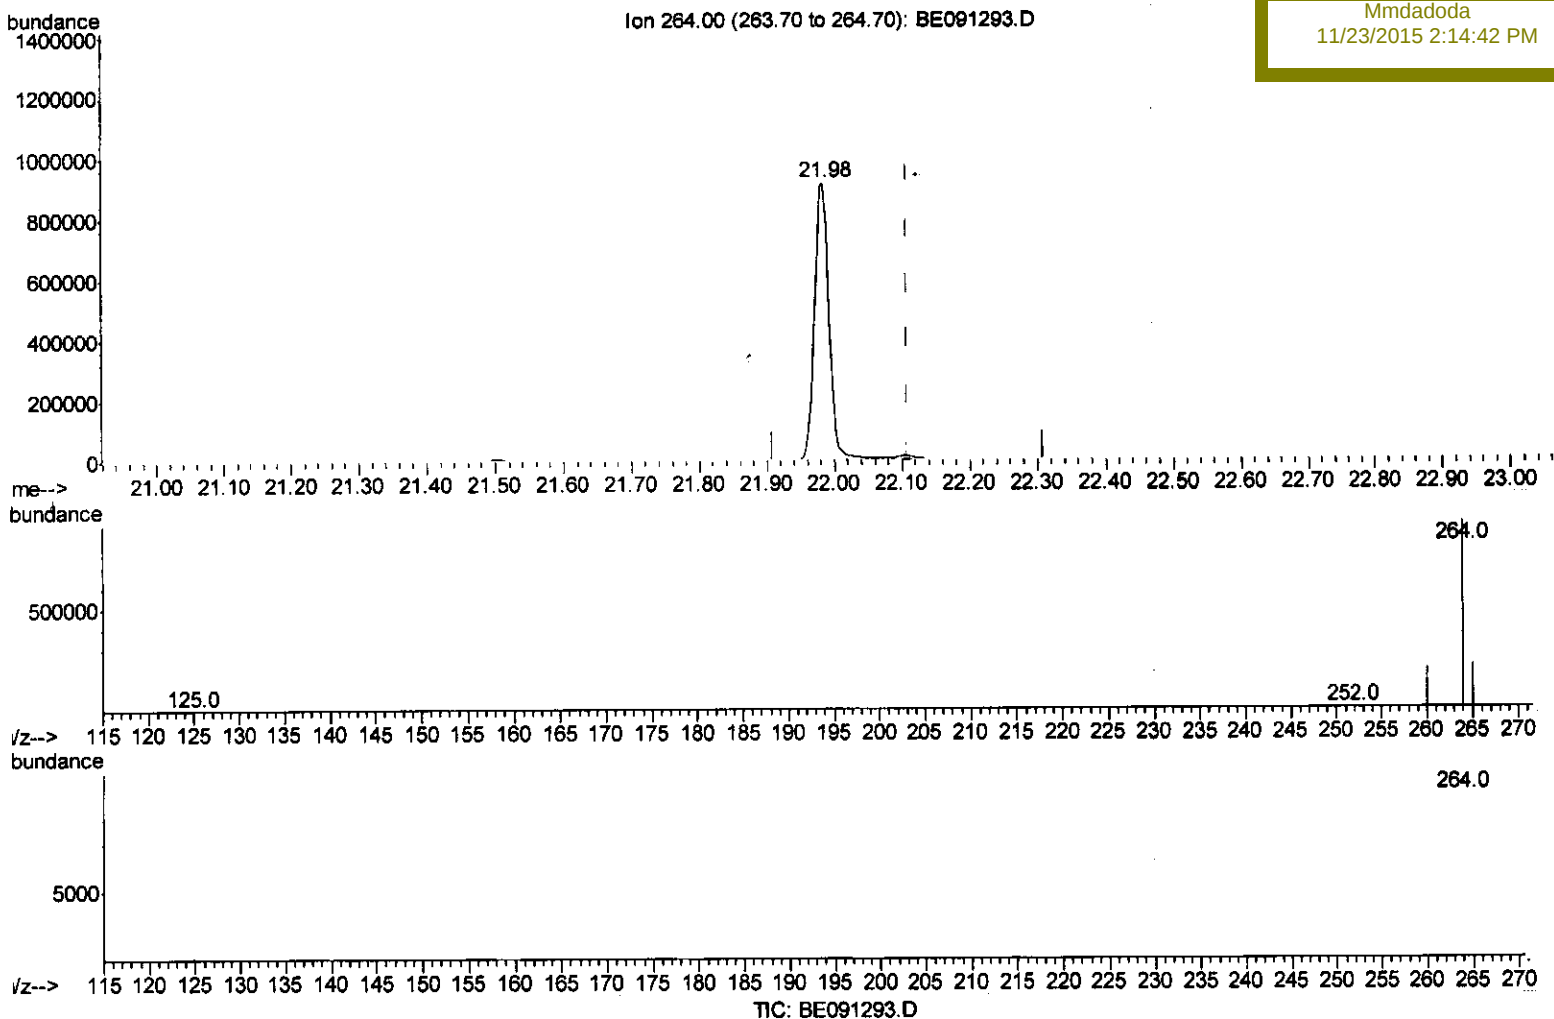

(22) Perylene-d12 (I)

21.984min (-0.124) 0.40ng/ul

response 1361638

Ion	Exp%	Act%
264.00	100	100
260.00	28.90	21.25#
265.00	34.70	23.26#
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112215\
 Data File : BE091293.D
 Acq On : 22 Nov 2015 10:48
 Operator : UM/NP
 Sample : PB86663BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK63

Manual Integrations
 APPROVED

Mmdadoda
 11/23/2015 2:14:42 PM

Quant Time: Nov 23 00:45:04 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 00:41:30 2015
 Response via : Initial Calibration

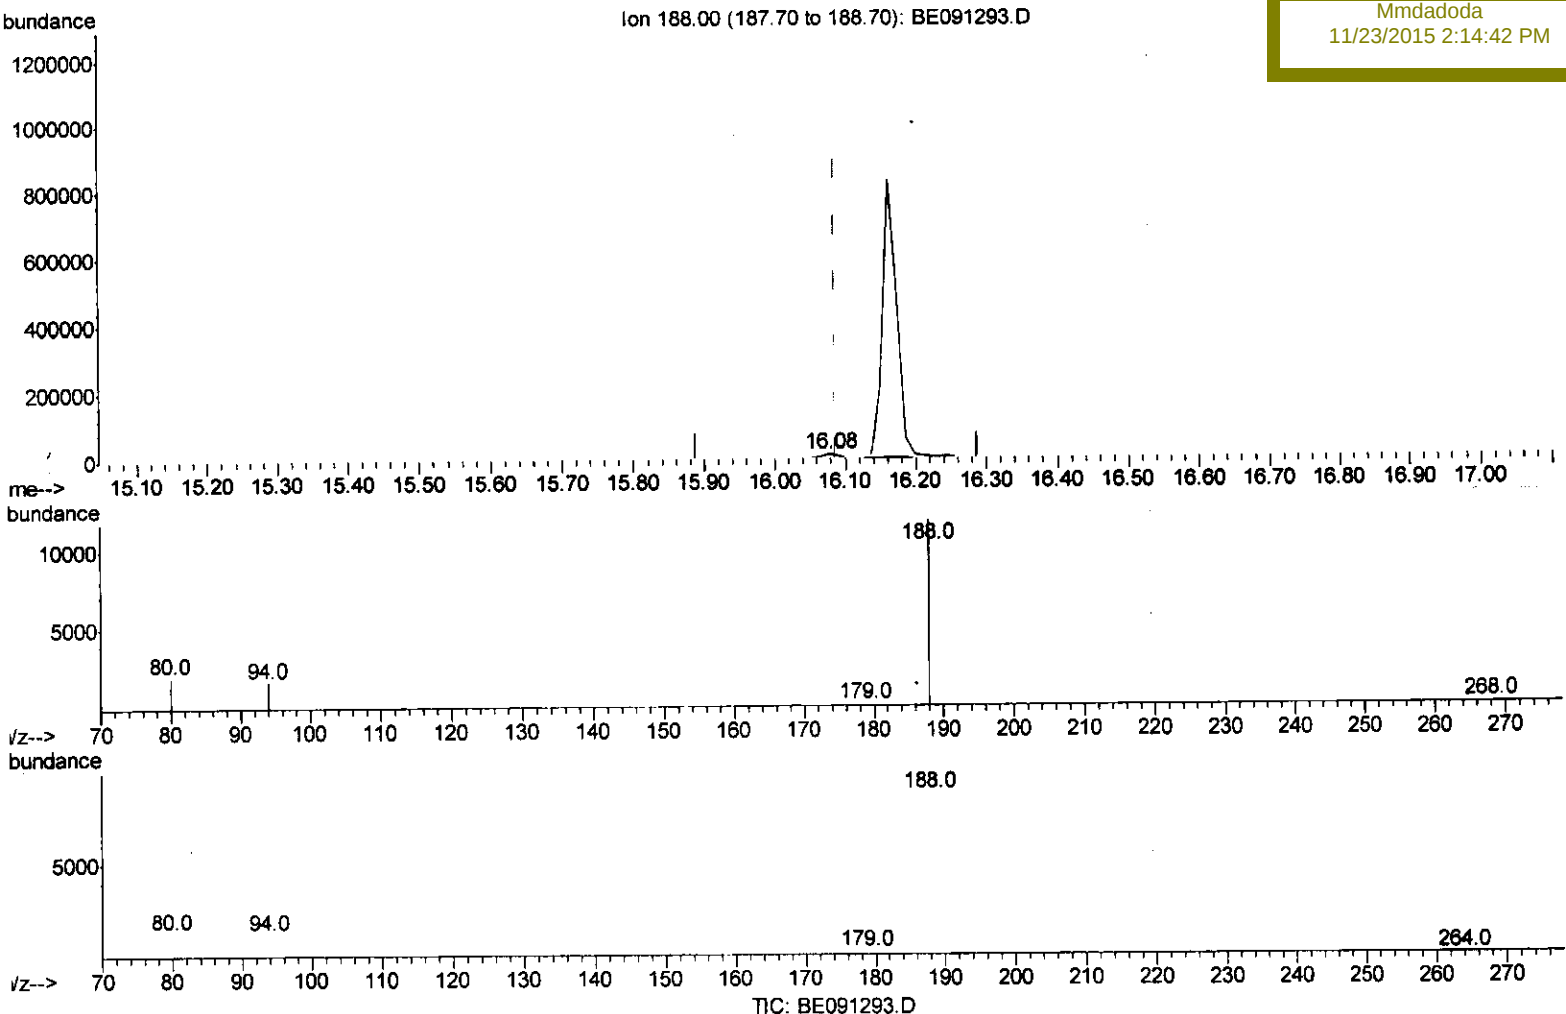

(12) Phenanthrene-d10 (l)

16.077min (-0.012) 0.40ng/ul m

response 16466

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	14.73#
80.00	8.90	17.08#
0.00	0.00	0.00

U.M
 11/25/15


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112215\
 Data File : BE091293.D
 Acq On : 22 Nov 2015 10:48
 Operator : UM/NP
 Sample : PB86663BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Quant Time: Nov 23 00:45:04 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 00:41:30 2015
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 SBLK63

Manual Integrations
 APPROVED

Mmdadoda
 11/23/2015 2:14:42 PM

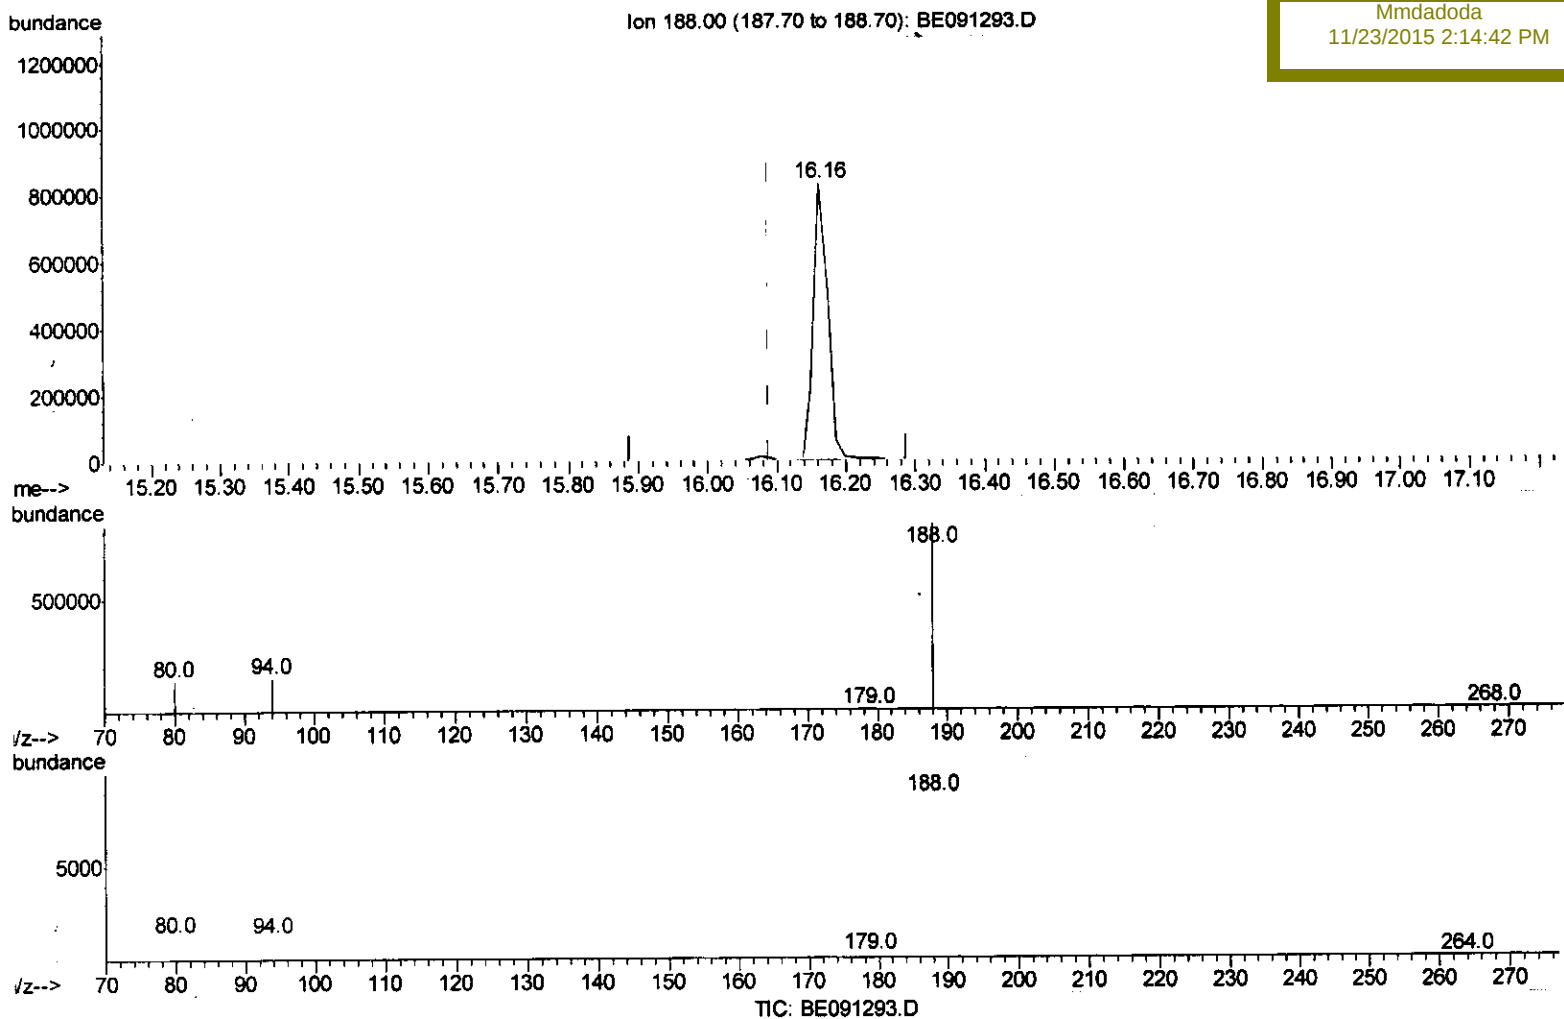

(12) Phenanthrene-d10 (I)

16.162min (+0.073) 0.40ng/ul

response 1195531

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	17.98#
80.00	8.90	16.72#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112215\
 Data File : BE091293.D
 Acc On : 22 Nov 2015 10:48
 Operator : UM/NP
 Sample : PB86663BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Quant Time: Nov 23 00:52:07 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 OLast Update : Mon Nov 23 00:41:30 2015
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 SBLK63

Manual Integrations
 APPROVED

Mmdadoda
 11/23/2015 2:14:42 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	2937	0.40	ng/ul	-0.02
4) Naphthalene-d8	9.54	136	14509	0.40	ng/ul	-0.02
8) Acenaphthene-d10	13.36	164	7491	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.08	188	16466m	0.40	ng/ul	-0.01
18) Chrysene-d12	20.23	240	15577	0.40	ng/ul	0.00
22) Perylene-d12	22.11	264	25208m	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.92	96	23947	11.33	ng/uL	-0.03
6) 2-Methylnaphthalene-d10	11.07	152	5234	0.26	ng/ul	0.00
16) Fluoranthene-d10	18.07	212	12232	0.26	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U.M
 11/25/15