
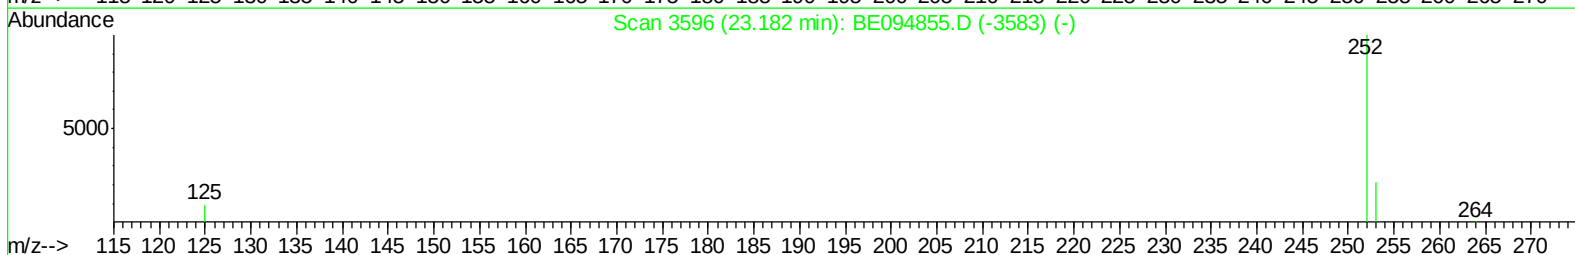
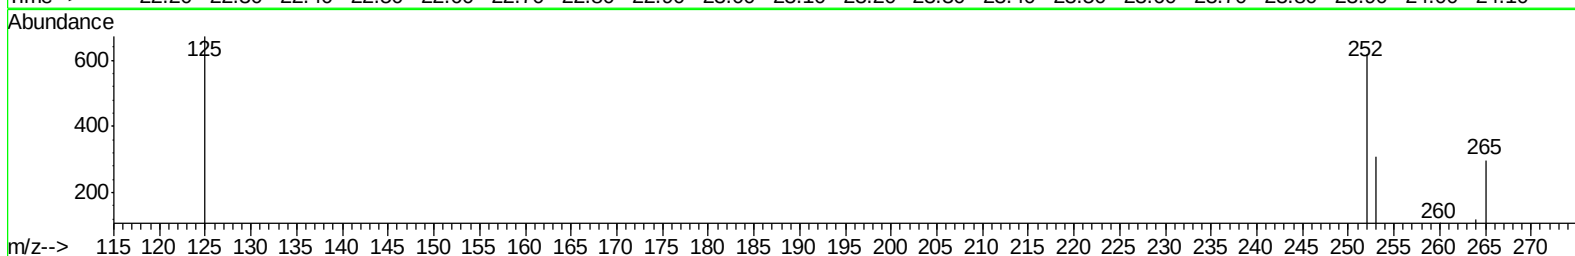


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
Data File : BE094857.D
Acq On : 23 Nov 2017 6:06
Operator : SJ/JU
Sample : I6496-17
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Nov 23 23:22:18 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 23 23:11:00 2017
Response via : Initial Calibration

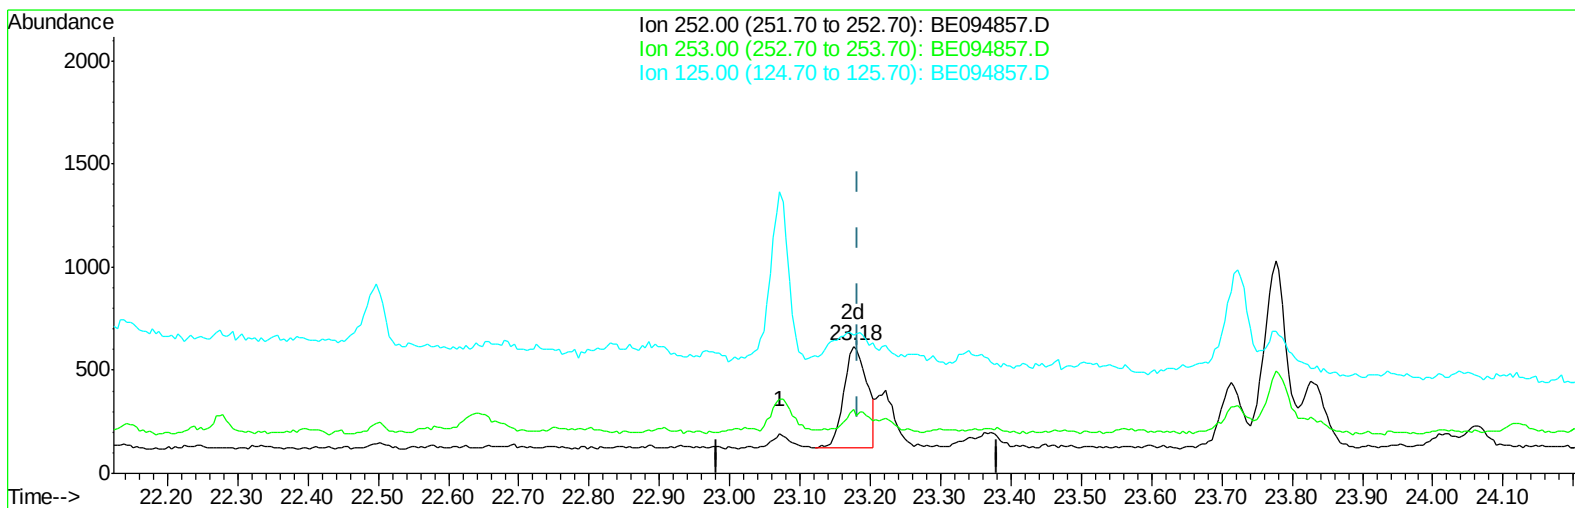

TIC: BE094857.D

(21) Benzo(b)fluoranthene

23.176min (-0.006) 0.04ng/ul m

response 1122

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	49.92
125.00	17.50	108.91#
0.00	0.00	0.00