
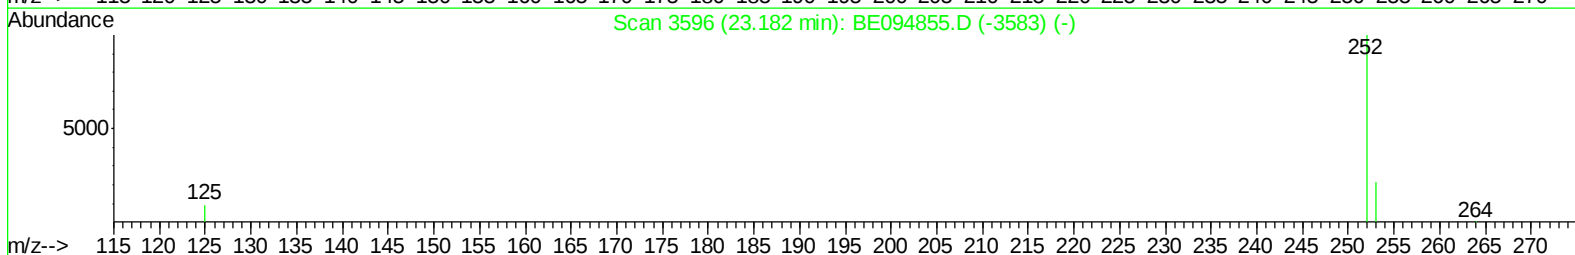
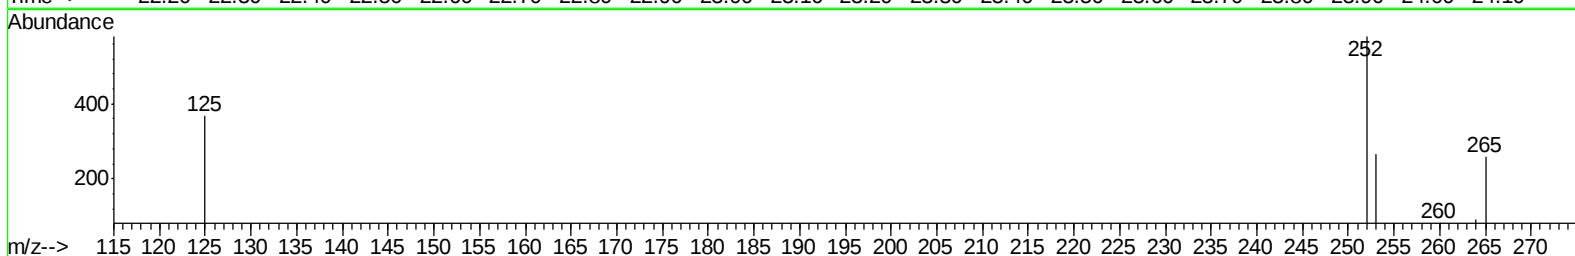


Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
Data File : BE094858.D
Acq On : 23 Nov 2017 6:42
Operator : SJ/JU
Sample : I6496-18
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Nov 23 23:15:57 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 23 23:11:00 2017
Response via : Initial Calibration

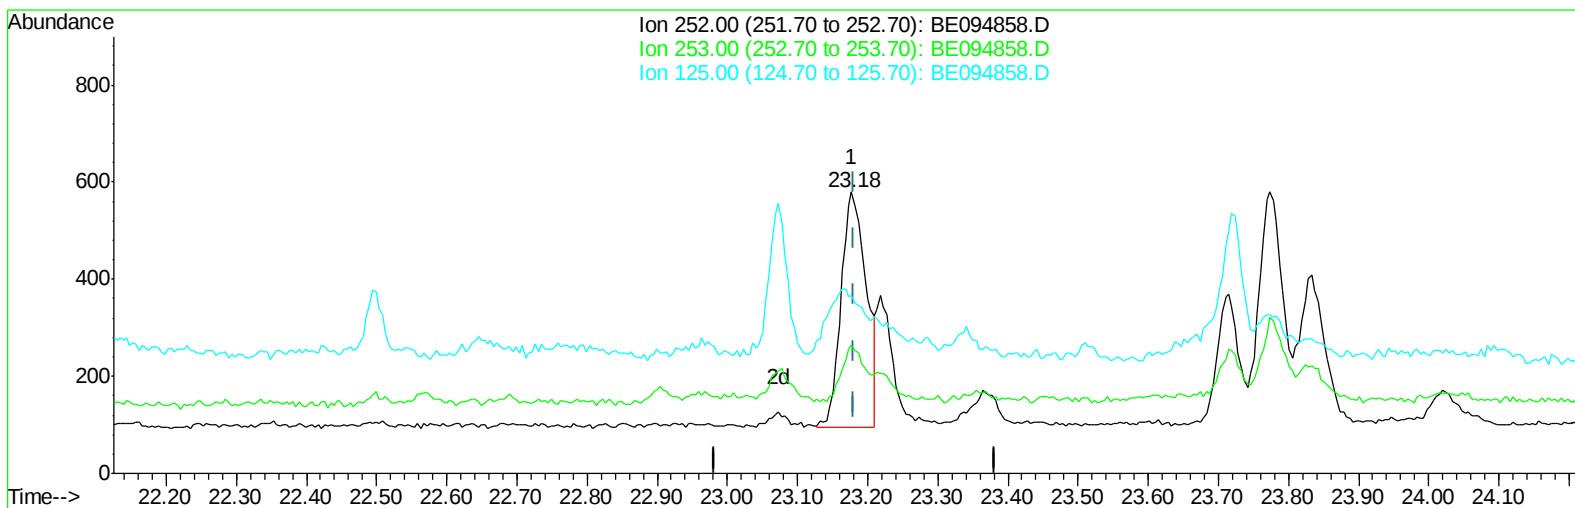

TIC: BE094858.D

(21) Benzo(b)fluoranthene

23.177min (-0.004) 0.05ng/ul m

response 1214

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	45.69
125.00	17.50	63.28#
0.00	0.00	0.00