

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094831.D
 Acq On : 22 Nov 2017 14:46
 Operator : SJ/JU
 Sample : I6514-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 23 00:57:57 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	679	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.67	136	4543	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.50	164	3346	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.43	240	7936	0.40	ng/ul	0.00
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.96
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	2981	0.41	ng/ul	0.01
14) Fluoranthene-d10	19.27	212	9403	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.65	202	898	0.04	ng/ul#	68
18) Benzo(a)anthracene	21.41	228	687	0.03	ng/ul#	69
19) Chrysene	21.47	228	840	0.03	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
Data File : BE094831.D
Acq On : 22 Nov 2017 14:46
Operator : SJ/JU
Sample : I6514-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 23 00:57:57 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 23 00:56:52 2017
Response via : Initial Calibration




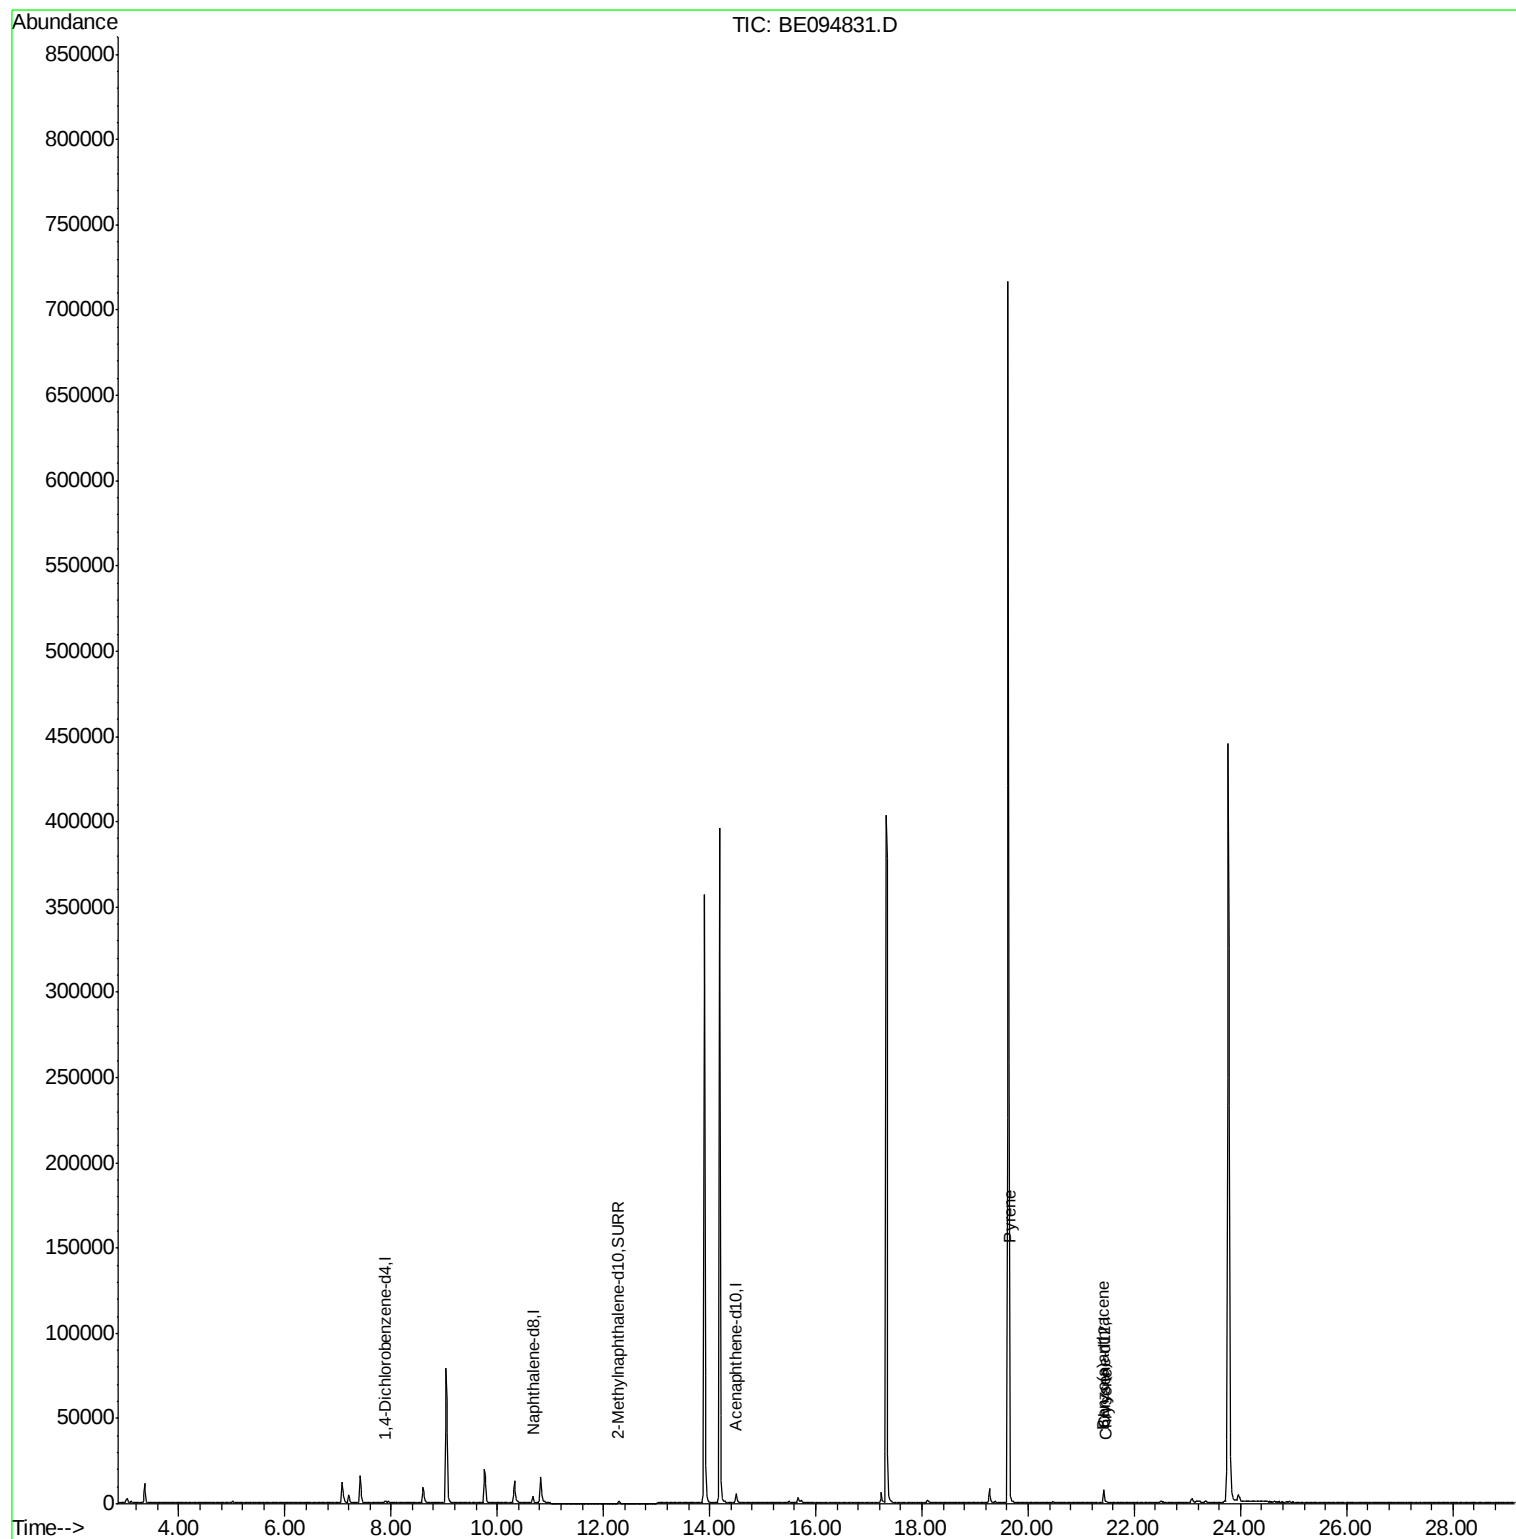


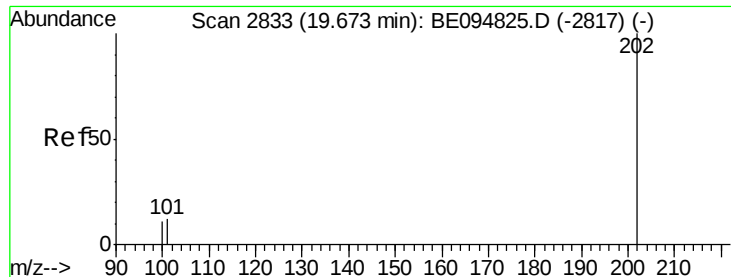

#17
 Pvrene
 Concen: 0.04 ng/ul
 RT: 19.65 min Scan# 2828
 Delta R.T. -0.02 min
 Lab File: BE094831.D
 Acq: 22 Nov 2017 14:46




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:202 Resp: 898
 Ion Ratio Lower Upper
 202 100
 101 34.5 18.2 27.4#
 100 38.3 15.6 23.4#

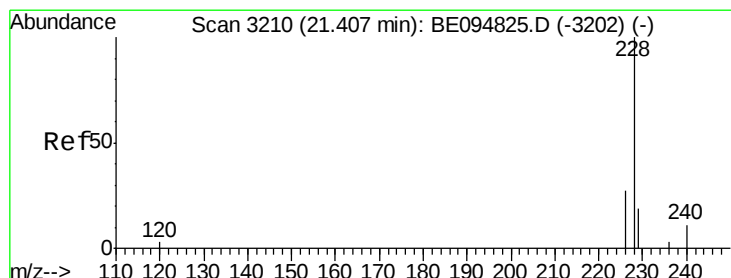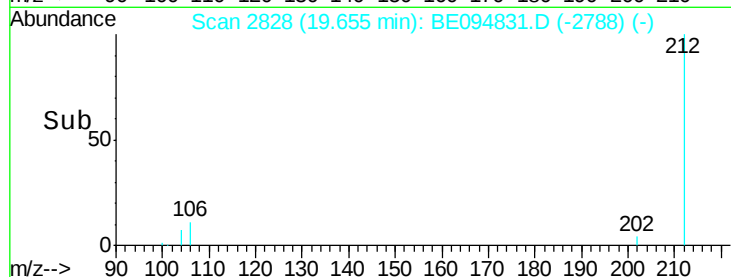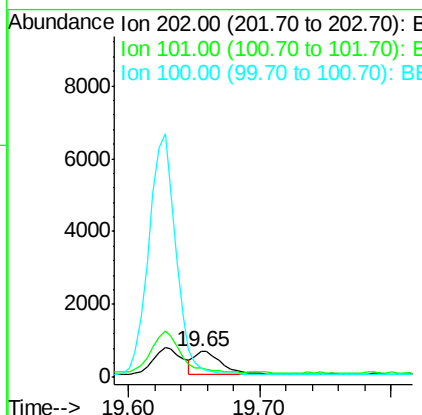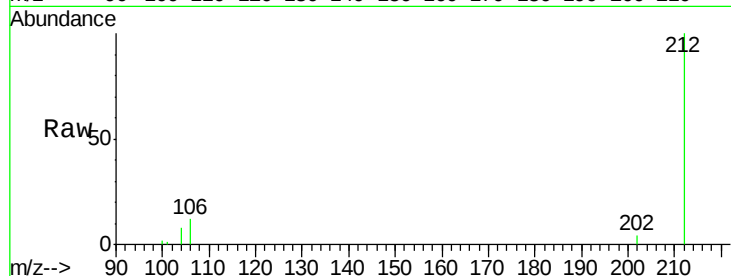

#18
 Benzo(a)anthracene
 Concen: 0.03 ng/ul
 RT: 21.41 min Scan# 3211
 Delta R.T. 0.01 min
 Lab File: BE094831.D
 Acq: 22 Nov 2017 14:46

Tgt Ion:228 Resp: 687
 Ion Ratio Lower Upper
 228 100
 229 41.7 22.8 34.2#
 226 39.8 17.0 25.6#

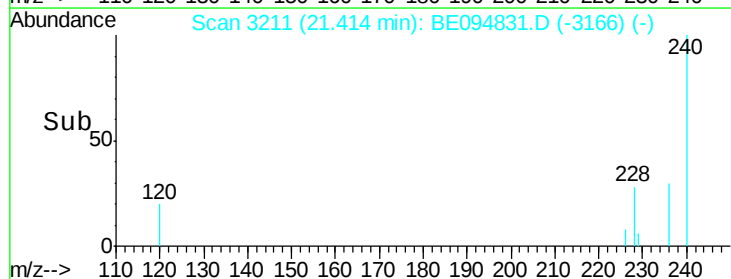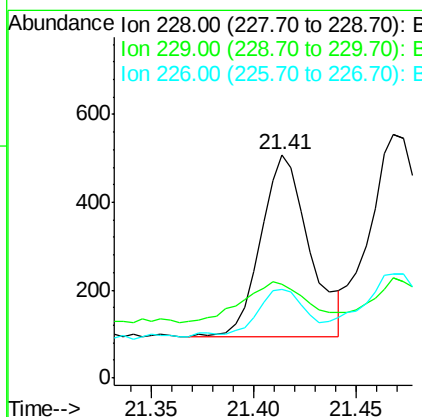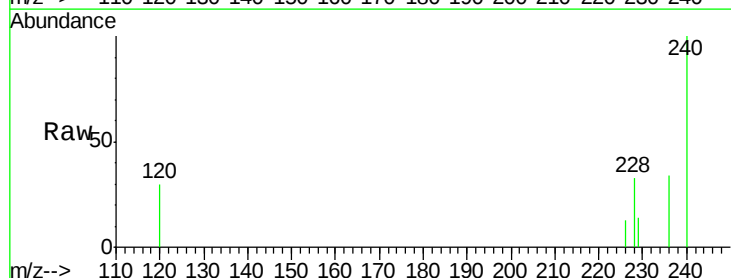

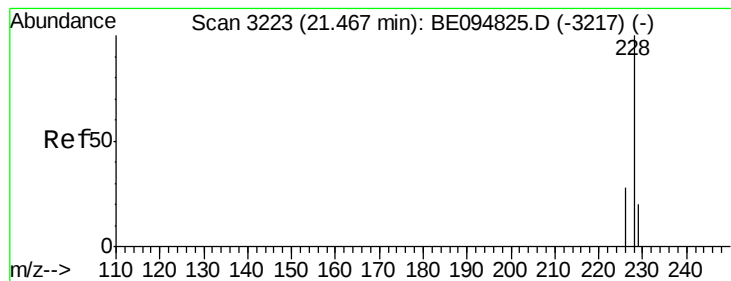

#19
 Chrysene
 Concen: 0.03 ng/ul
 RT: 21.47 min Scan# 3223
 Delta R.T. 0.00 min
 Lab File: BE094831.D
 Acq: 22 Nov 2017 14:46

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion: 228 Resp: 840
 Ion Ratio Lower Upper
 228 100
 226 42.6 23.4 35.0#
 229 41.0 17.7 26.5#

