

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094835.D
 Acq On : 22 Nov 2017 17:07
 Operator : SJ/JU
 Sample : I6514-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 23 00:58:28 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	752	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.67	136	4893	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.50	164	3493	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.42	240	8767	0.40	ng/ul	0.00
20) Perylene-d12	23.78	264	368340	0.40	ng/ul	-0.19
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	2523	0.32	ng/ul	0.01
14) Fluoranthene-d10	19.27	212	7982	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.66	202	10308	0.38	ng/ul#	83
18) Benzo(a)anthracene	21.41	228	7046	0.26	ng/ul#	90
19) Chrysene	21.46	228	6548	0.25	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
Data File : BE094835.D
Acq On : 22 Nov 2017 17:07
Operator : SJ/JU
Sample : I6514-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 23 00:58:28 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 23 00:56:52 2017
Response via : Initial Calibration




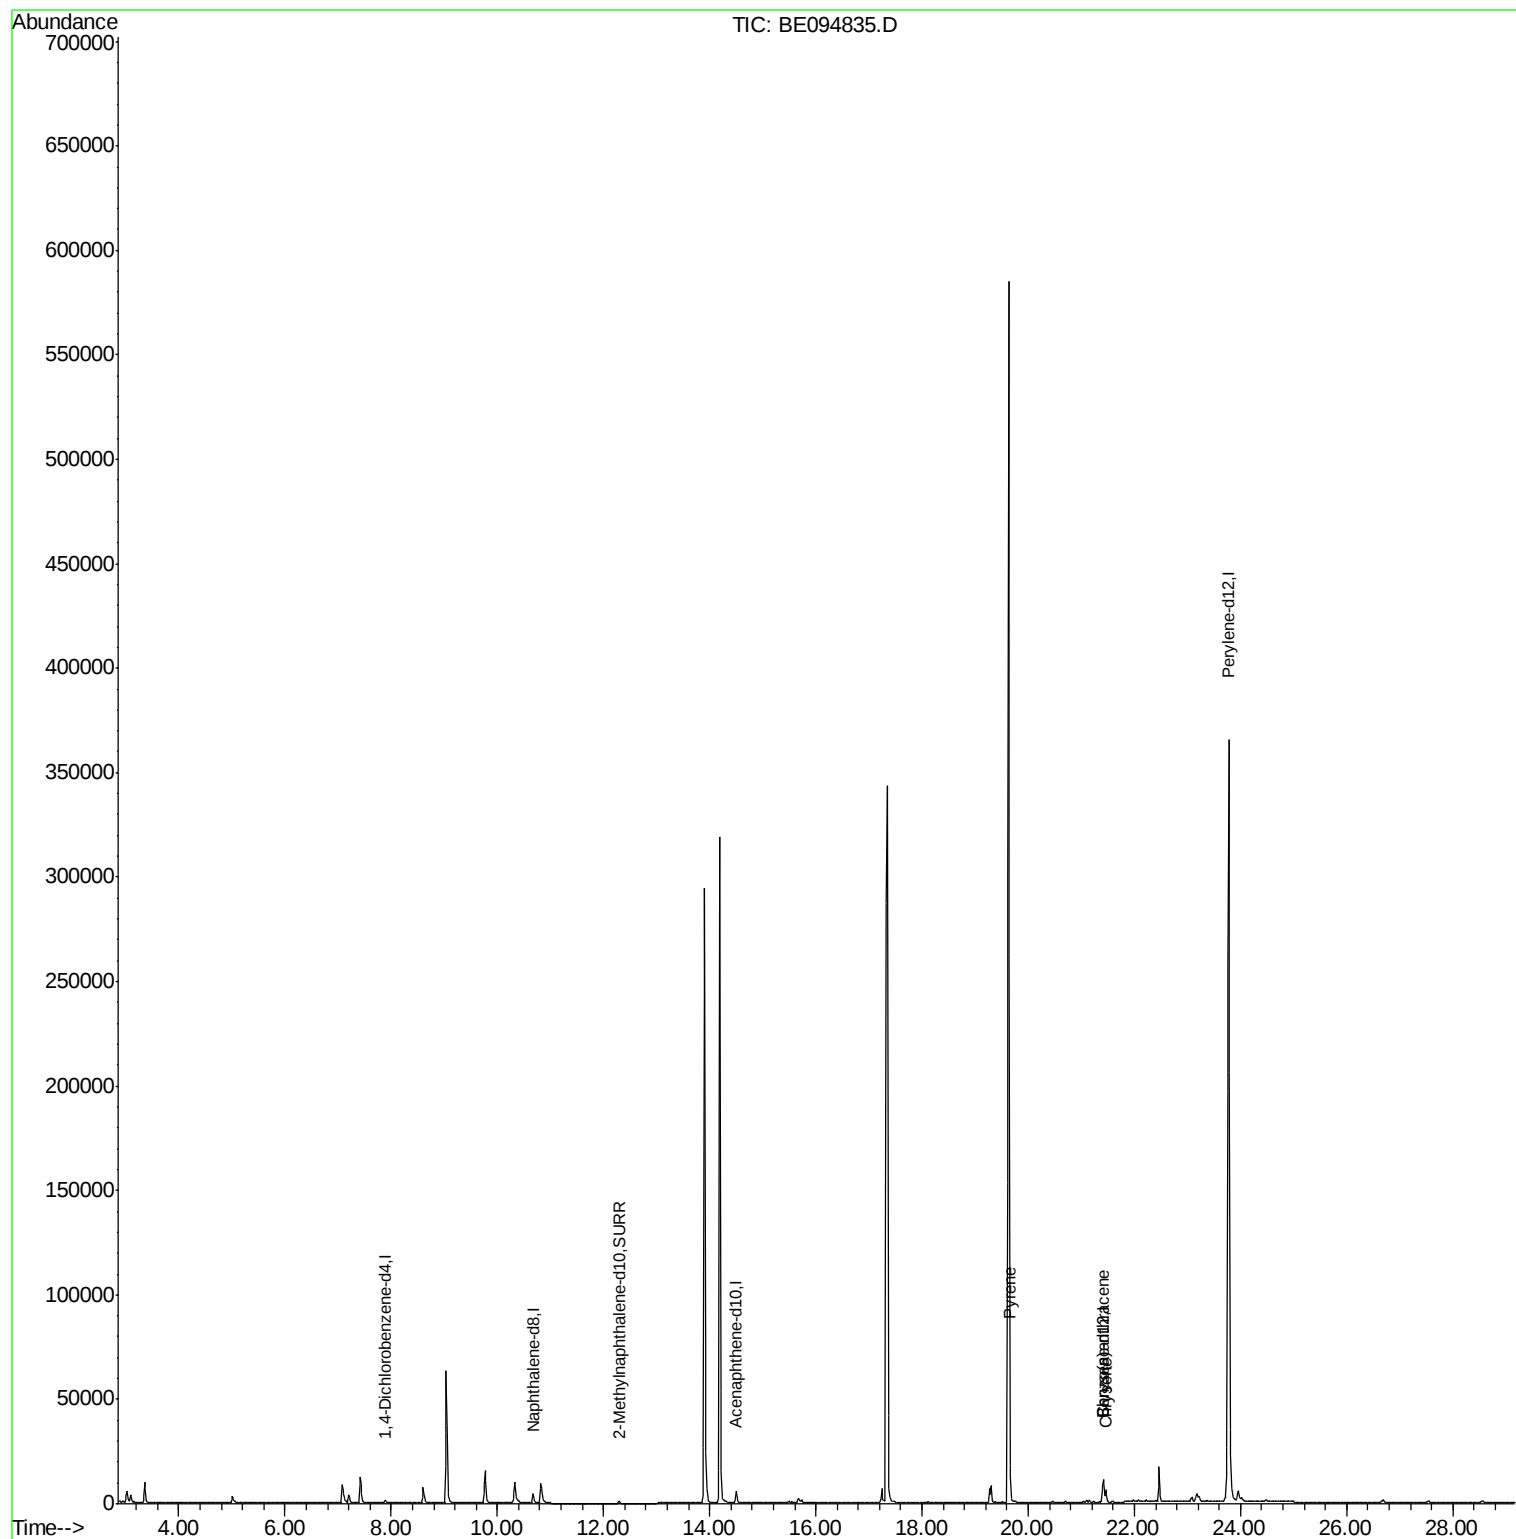


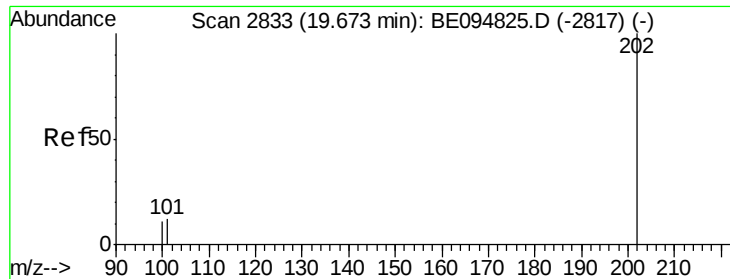

#17
Pvrene
Concen: 0.38 ng/ul
RT: 19.66 min Scan# 2829
Delta R.T. -0.01 min
Lab File: BE094835.D
Acq: 22 Nov 2017 17:07




Instrument :
BNA_E
ClientSampleId :


Tot Ion:202 Resp: 10308
Ion Ratio Lower Upper
202 100
101 13.9 18.2 27.4#
100 12.8 15.6 23.4#

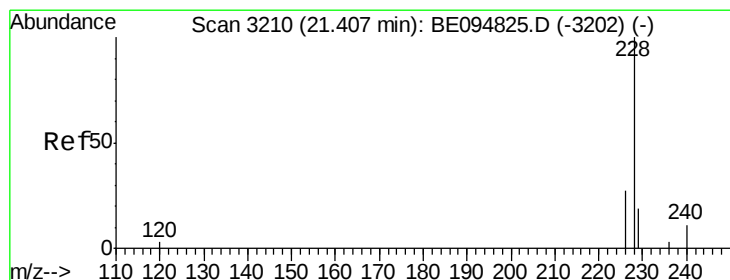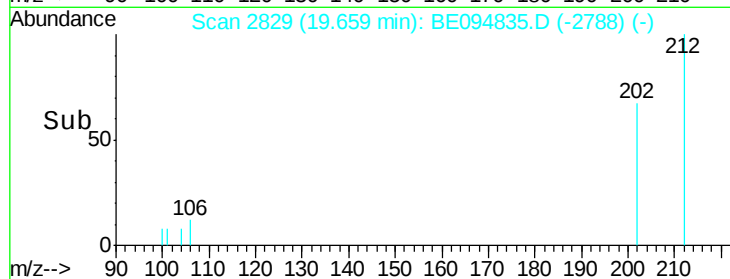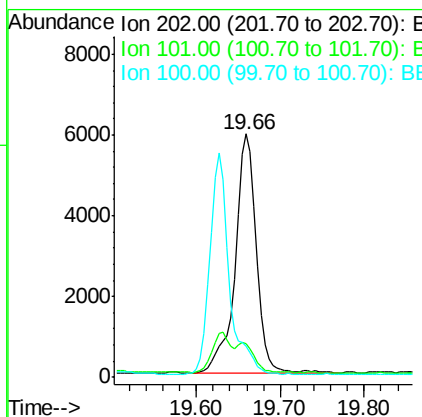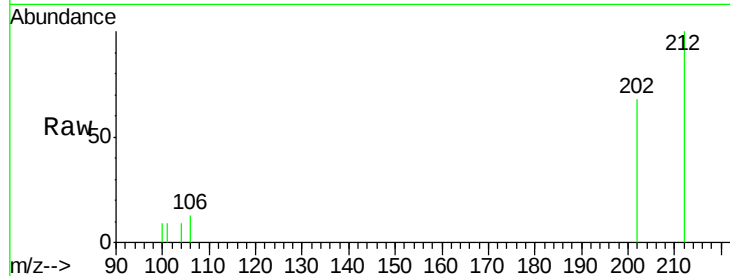

#18
Benzo(a)anthracene
Concen: 0.26 ng/ul
RT: 21.41 min Scan# 3210
Delta R.T. 0.00 min
Lab File: BE094835.D
Acq: 22 Nov 2017 17:07

Tgt Ion:228 Resp: 7046
Ion Ratio Lower Upper
228 100
229 23.7 22.8 34.2
226 26.7 17.0 25.6#

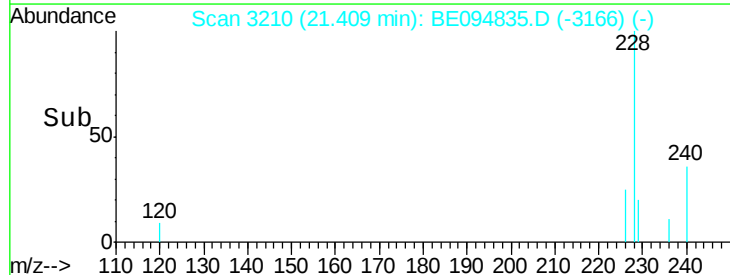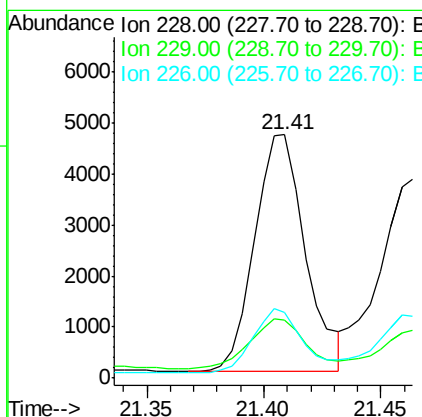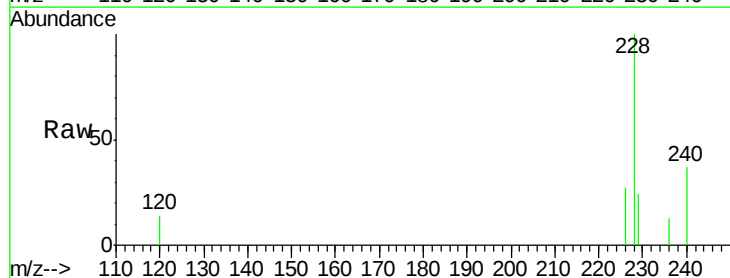

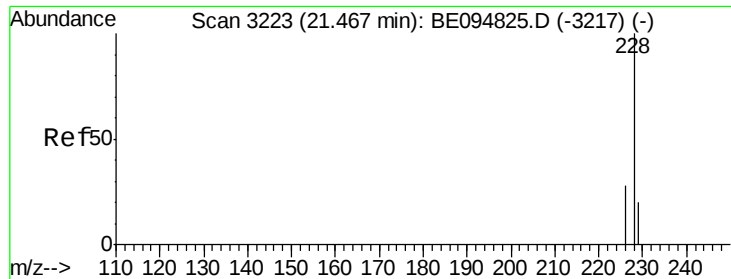

#19

Chrysene

Concen: 0.25 ng/ul

RT: 21.46 min Scan# 3222

Delta R.T. -0.00 min

Lab File: BE094835.D

Acq: 22 Nov 2017 17:07

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 228 Resp: 6548

Ion Ratio Lower Upper

228 100

226 31.0 23.4 35.0

229 24.0 17.7 26.5

