

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094836.D
 Acq On : 22 Nov 2017 17:46
 Operator : SJ/JU
 Sample : PB104368BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 23 00:58:37 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	668	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.67	136	4321	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.50	164	3169	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.44	240	8069	0.40	ng/ul	0.01
20) Perylene-d12	23.97	264	9337	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.30	152	2542	0.36	ng/ul	0.03
14) Fluoranthene-d10	19.27	212	8489	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.49	166	768	0.06	ng/ul#	22
17) Pyrene	19.63	202	1120	0.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
Data File : BE094836.D
Acq On : 22 Nov 2017 17:46
Operator : SJ/JU
Sample : PB104368BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 23 00:58:37 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 23 00:56:52 2017
Response via : Initial Calibration

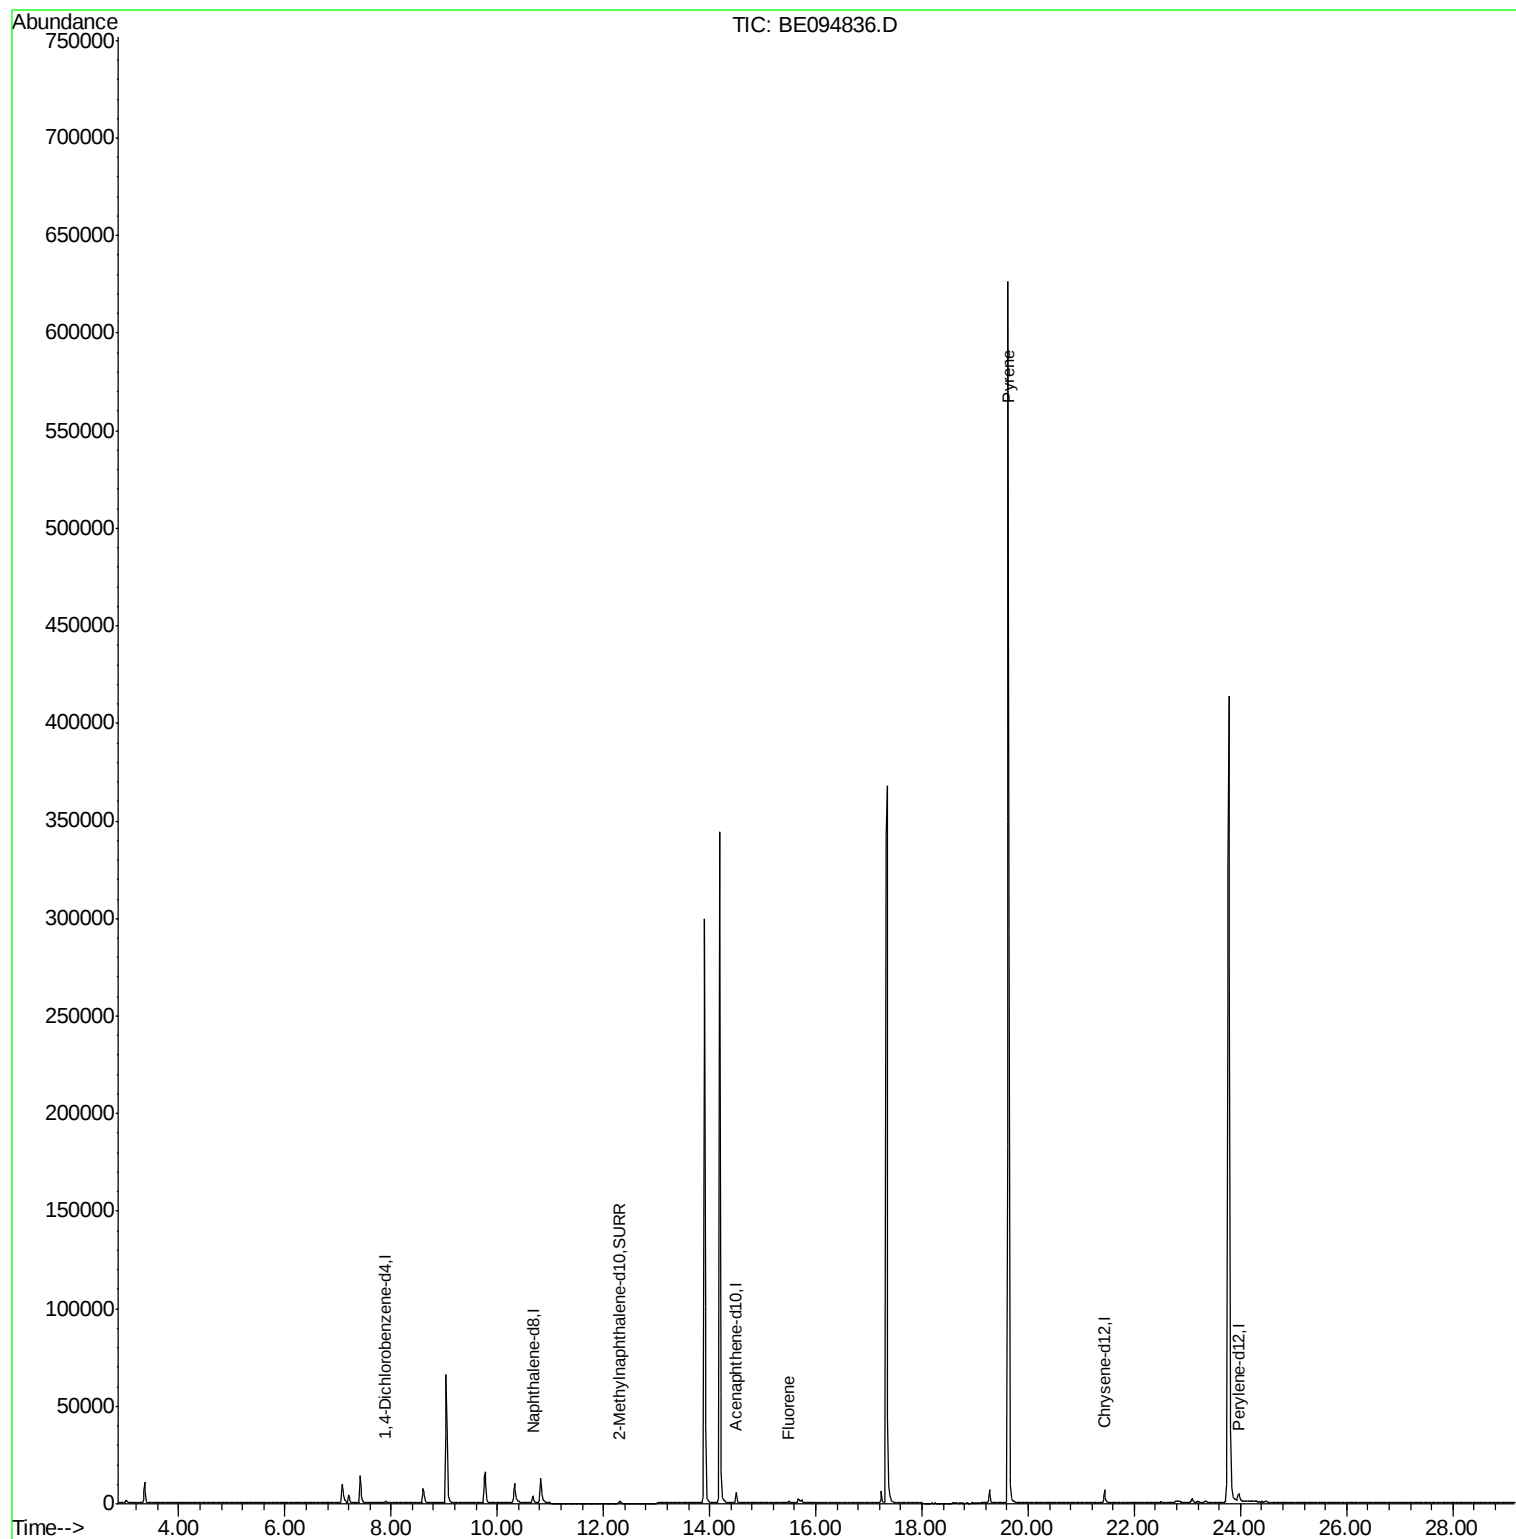

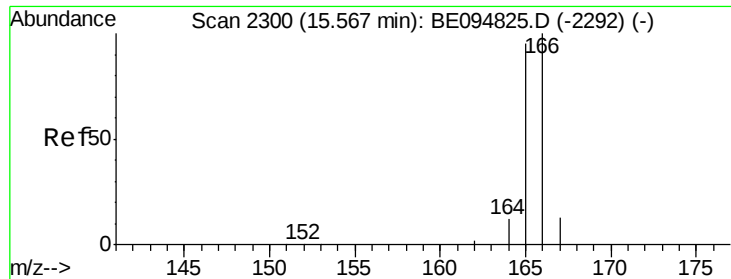

#9

Fluorene

Concen: 0.06 ng/ul

RT: 15.49 min Scan# 2290

Delta R.T. -0.08 min

Lab File: BE094836.D

Acq: 22 Nov 2017 17:46

Instrument :

BNA_E

ClientSampleId :





Tot Ion:166 Resp: 768

Ion Ratio Lower Upper

166 100

165 11.7 73.4 110.2#

167 39.4 14.6 22.0#

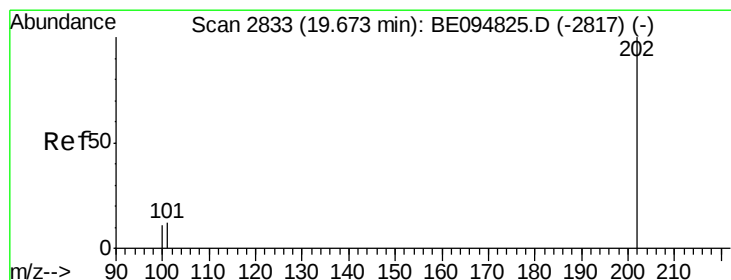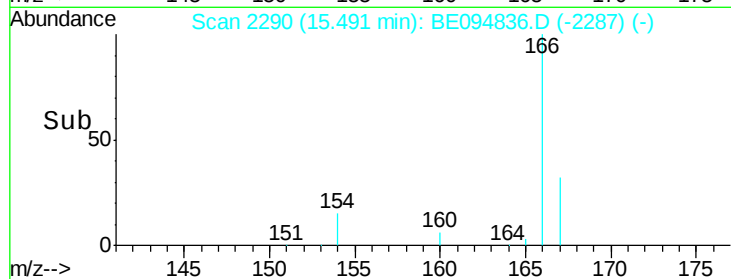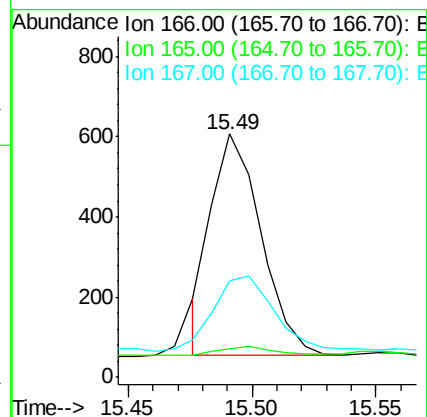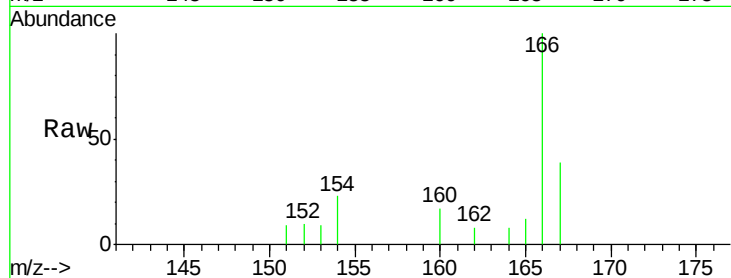

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.63 min Scan# 2824

Delta R.T. -0.04 min

Lab File: BE094836.D

Acq: 22 Nov 2017 17:46

Tgt Ion:202 Resp: 1120

Ion Ratio Lower Upper

202 100

101 145.9 18.2 27.4#

100 718.6 15.6 23.4#

