

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094837.D
 Acq On : 22 Nov 2017 18:21
 Operator : SJ/JU
 Sample : I6514-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 23 00:58:44 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	651	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	4216	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.50	164	3059	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	7175	0.40	ng/ul	-0.02
16) Chrysene-d12	21.43	240	7683	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	8377	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	1216	0.18	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	4127	0.17	ng/ul	-0.01
Target Compounds						
11) Pentachlorophenol	17.03	266	11	0.03	ng/ul#	20
17) Pyrene	19.63	202	589	0.02	ng/ul#	1
23) Benzo(a)pyrene	23.77	252	726	0.03	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
Data File : BE094837.D
Acq On : 22 Nov 2017 18:21
Operator : SJ/JU
Sample : I6514-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 23 00:58:44 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 23 00:56:52 2017
Response via : Initial Calibration




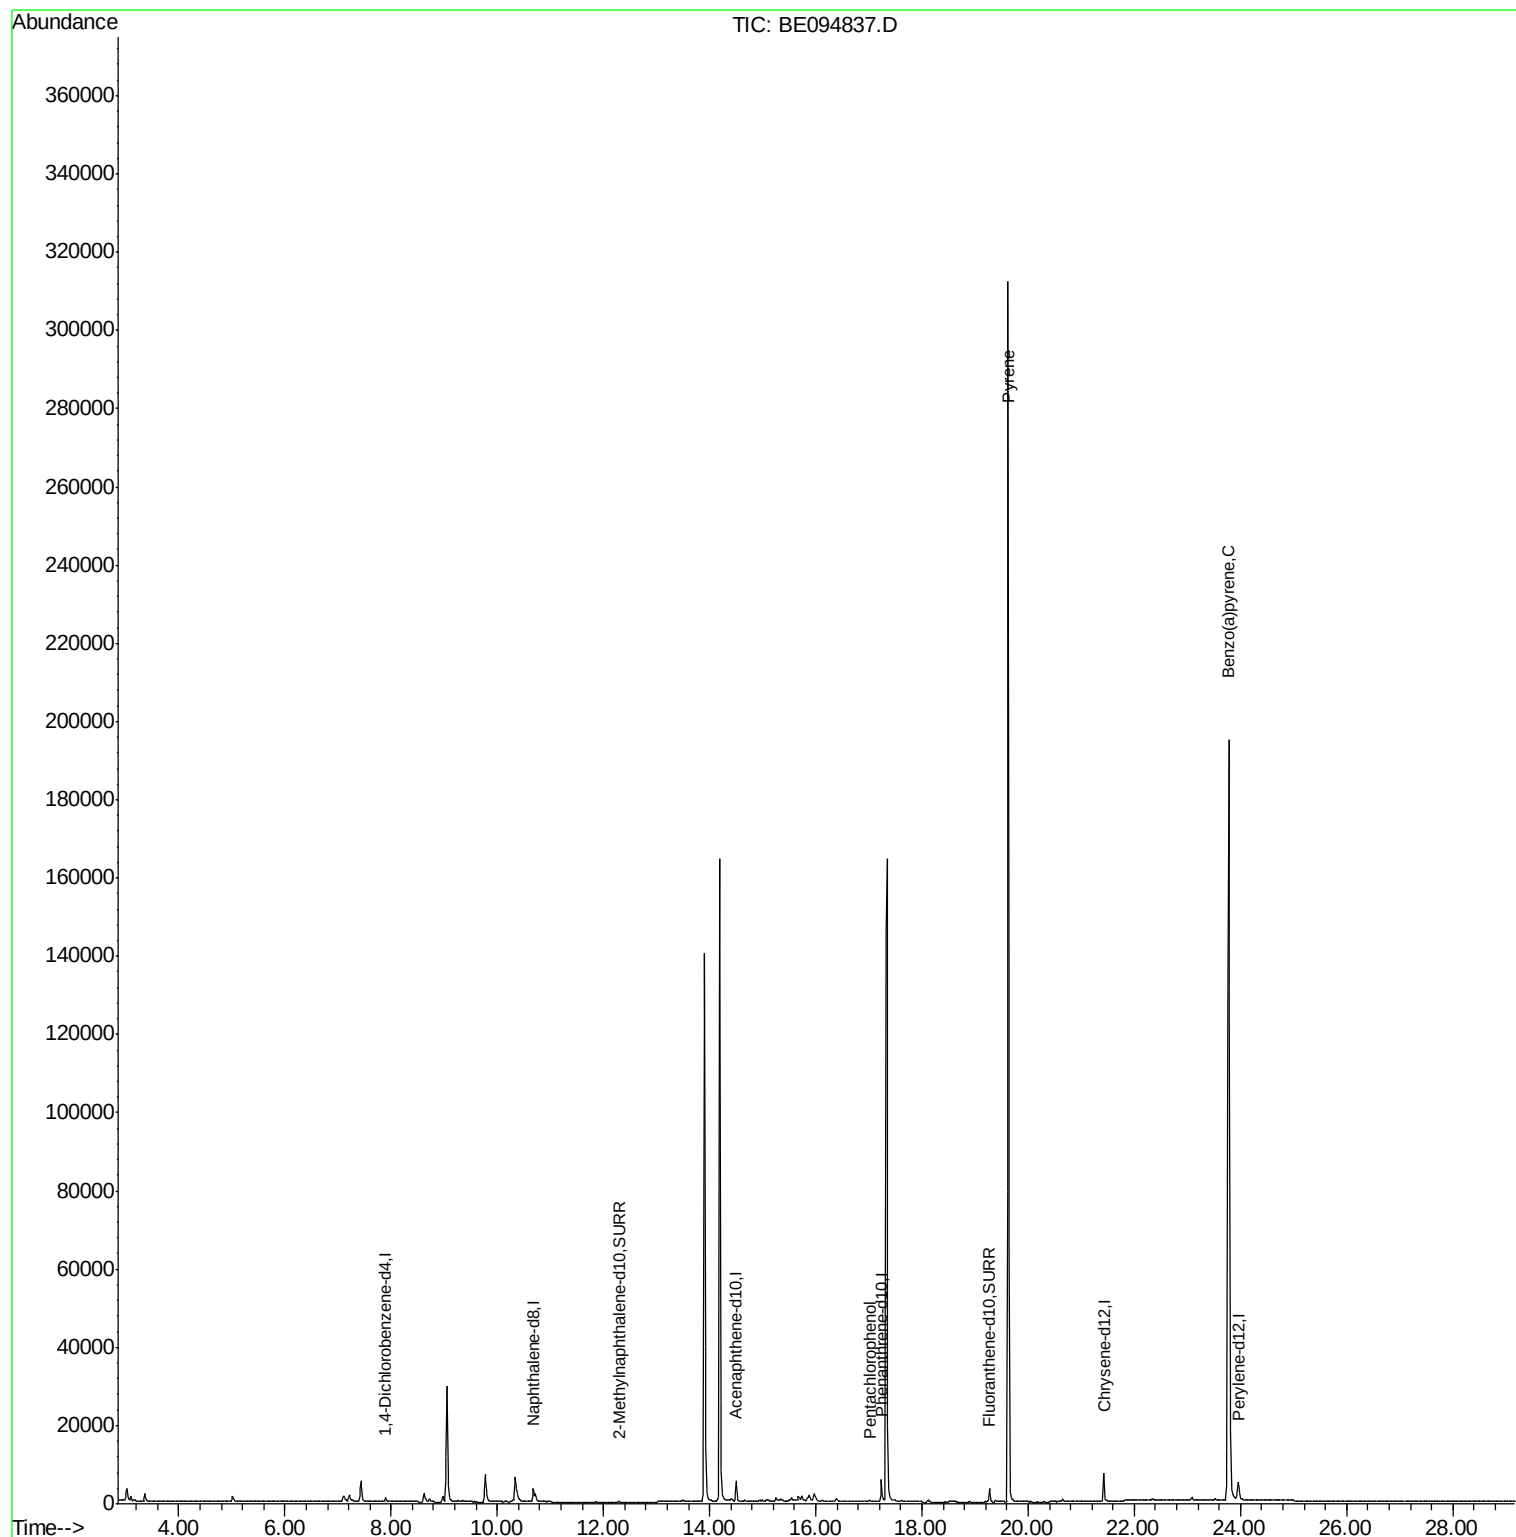


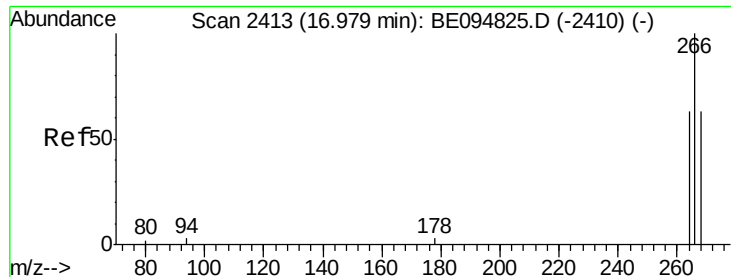

#11
 Pentachlorophenol
 Concen: 0.03 ng/ul
 RT: 17.03 min Scan# 2416
 Delta R.T. 0.05 min
 Lab File: BE094837.D
 Acq: 22 Nov 2017 18:21




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 11
 Ion Ratio Lower Upper
 266 100
 264 0.0 47.9 71.9#
 268 0.0 49.8 74.8#

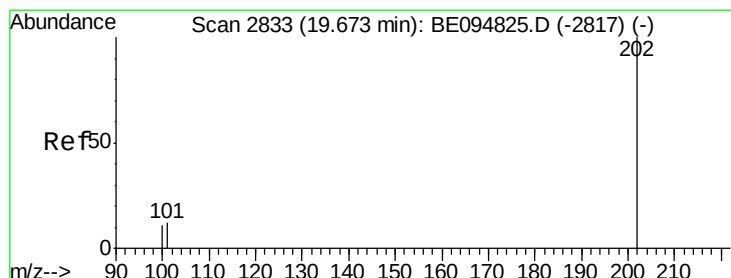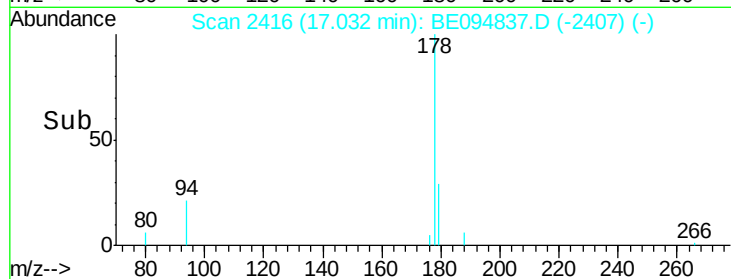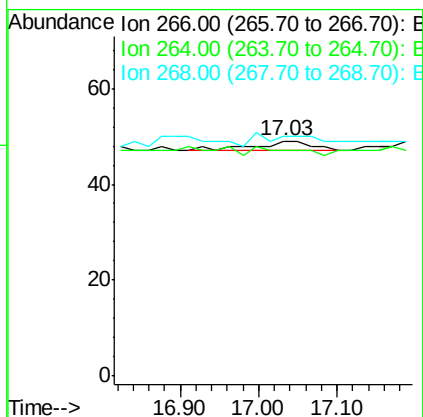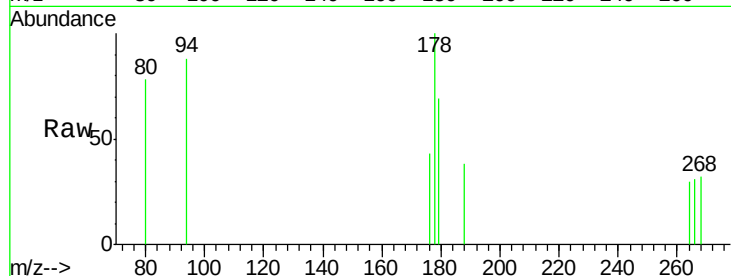

#17
 Pyrene
 Concen: 0.02 ng/ul
 RT: 19.63 min Scan# 2823
 Delta R.T. -0.04 min
 Lab File: BE094837.D
 Acq: 22 Nov 2017 18:21

Tgt Ion:202 Resp: 589
 Ion Ratio Lower Upper
 202 100
 101 144.7 18.2 27.4#
 100 641.3 15.6 23.4#

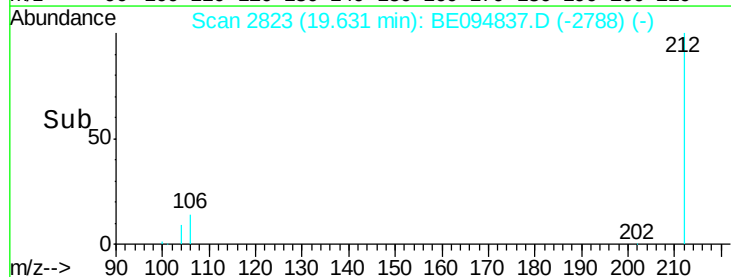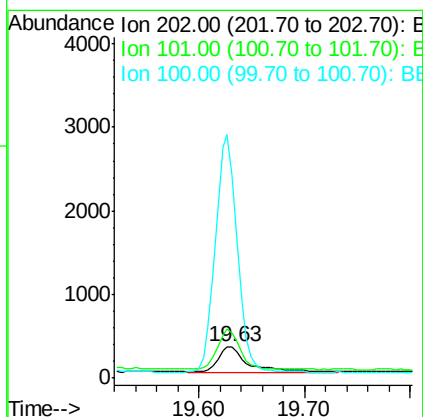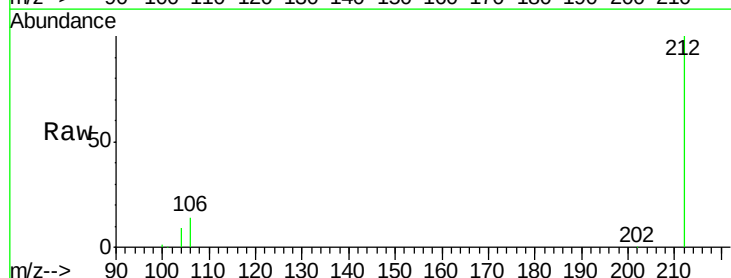

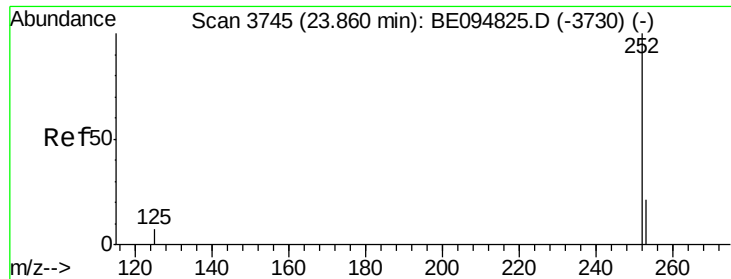

#23

Benzo(a)pyrene

Concen: 0.03 ng/ul

RT: 23.77 min Scan# 3726

Delta R.T. -0.09 min


Lab File: BE094837.D

Acq: 22 Nov 2017 18:21

Instrument :

BNA_E

ClientSampleId :

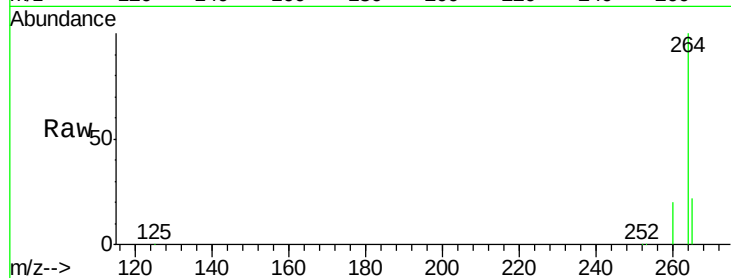


Tot Ion: 252 Resp: 726

Ion Ratio Lower Upper

252 100

253 52.2 28.5 42.7#

125 54.9 18.1 27.1#

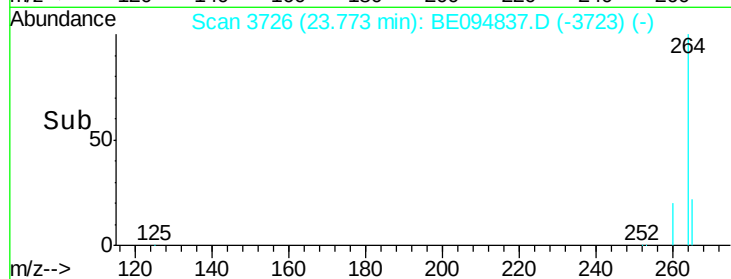

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

