

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094838.D
 Acq On : 22 Nov 2017 18:54
 Operator : SJ/JU
 Sample : I6514-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 23 00:58:51 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 00:56:52 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	674	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	4294	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.50	164	3231	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	7515	0.40	ng/ul	-0.02
16) Chrysene-d12	21.43	240	7908	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	8643	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	1529	0.22	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	5048	0.20	ng/ul	0.00
Target Compounds						
17) Pyrene	19.63	202	673	0.03	ng/ul#	1
23) Benzo(a)pyrene	23.77	252	1009	0.04	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
Data File : BE094838.D
Acq On : 22 Nov 2017 18:54
Operator : SJ/JU
Sample : I6514-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 23 00:58:51 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 23 00:56:52 2017
Response via : Initial Calibration




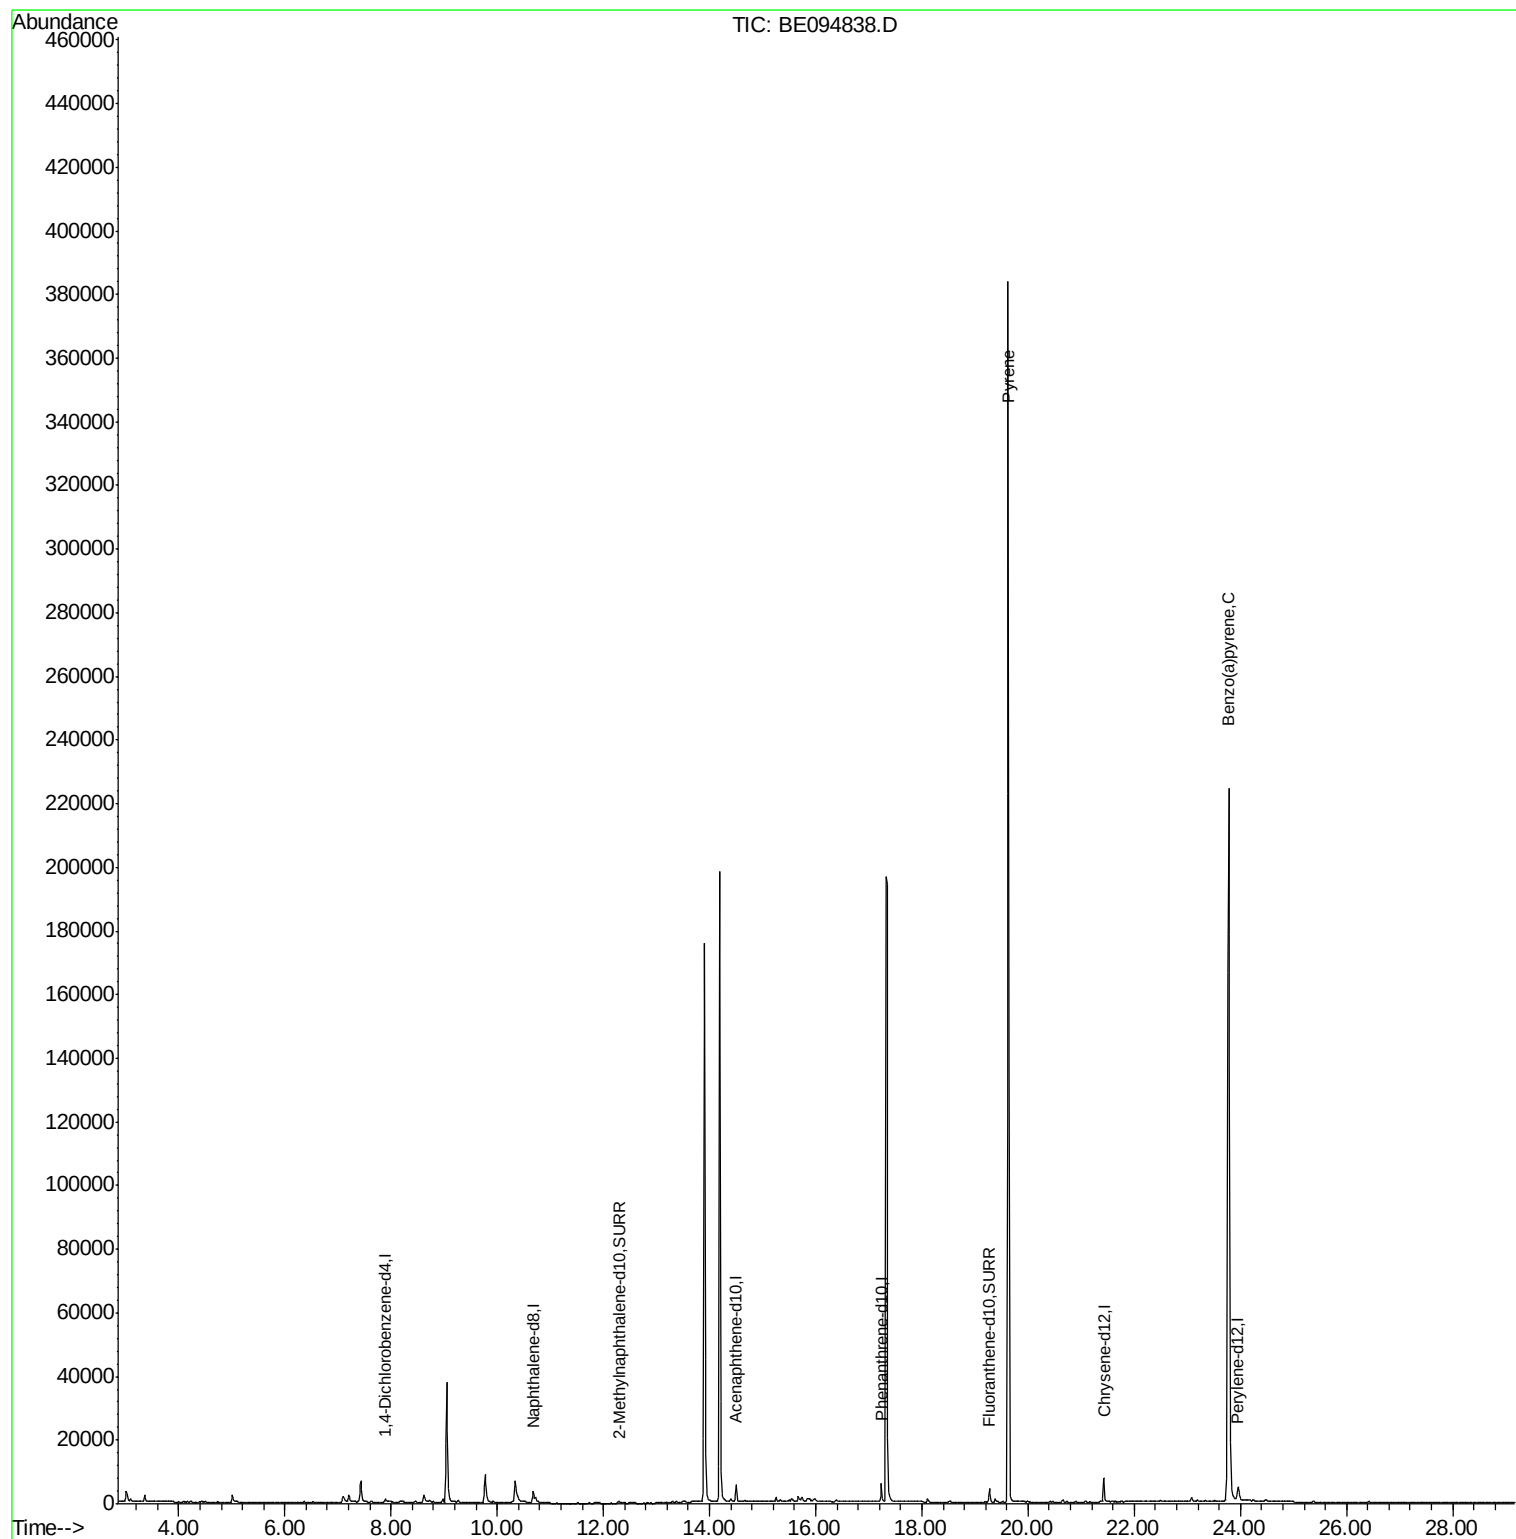


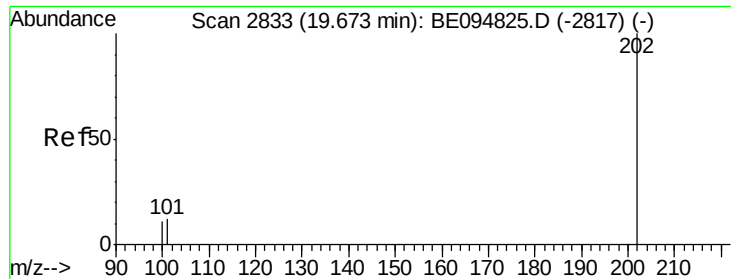

#17
Pvrene
Concen: 0.03 ng/ul
RT: 19.63 min Scan# 2823
Delta R.T. -0.05 min
Lab File: BE094838.D
Acq: 22 Nov 2017 18:54

Instrument :
BNA_E
ClientSampleId :

Tot Ion:202 Resp: 673
Ion Ratio Lower Upper
202 100
101 163.6 18.2 27.4#
100 799.1 15.6 23.4#

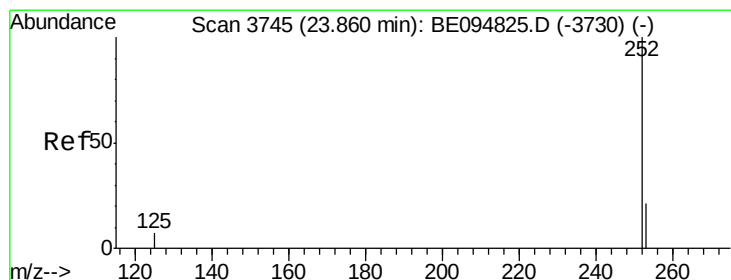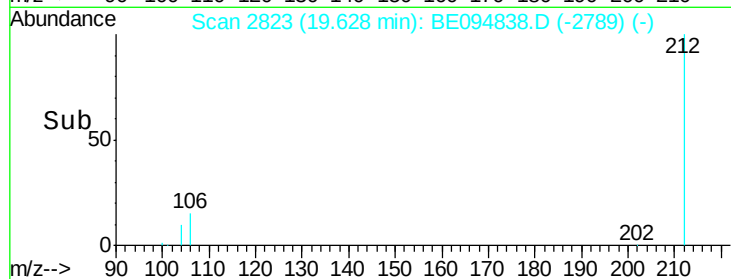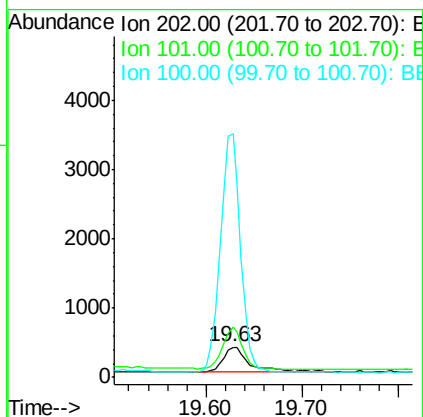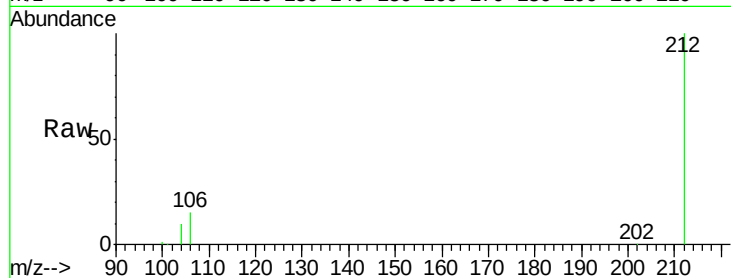

#23
Benzo(a)pyrene
Concen: 0.04 ng/ul
RT: 23.77 min Scan# 3726
Delta R.T. -0.09 min
Lab File: BE094838.D
Acq: 22 Nov 2017 18:54

Tgt Ion:252 Resp: 1009
Ion Ratio Lower Upper
252 100
253 50.8 28.5 42.7#
125 50.6 18.1 27.1#

