

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
 Data File : BE094840.D
 Acq On : 22 Nov 2017 20:06
 Operator : SJ/JU
 Sample : PB104341BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 23 02:51:20 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 23 02:50:08 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	699	0.40	ng/ul	-0.04
2) Naphthalene-d8	10.67	136	4476	0.40	ng/ul	-0.04
6) Acenaphthene-d10	14.50	164	3313	0.40	ng/ul	-0.01
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.44	240	8308	0.40	ng/ul	0.01
20) Perylene-d12	23.96	264	9785	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.31	152	2618	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	9071	0.00	ng/ul	-0.01
Target Compounds						
9) Fluorene	15.49	166	819	0.06	ng/ul#	21
17) Pyrene	19.63	202	1134	0.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE112217\
Data File : BE094840.D
Acq On : 22 Nov 2017 20:06
Operator : SJ/JU
Sample : PB104341BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 23 02:51:20 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE111417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 23 02:50:08 2017
Response via : Initial Calibration

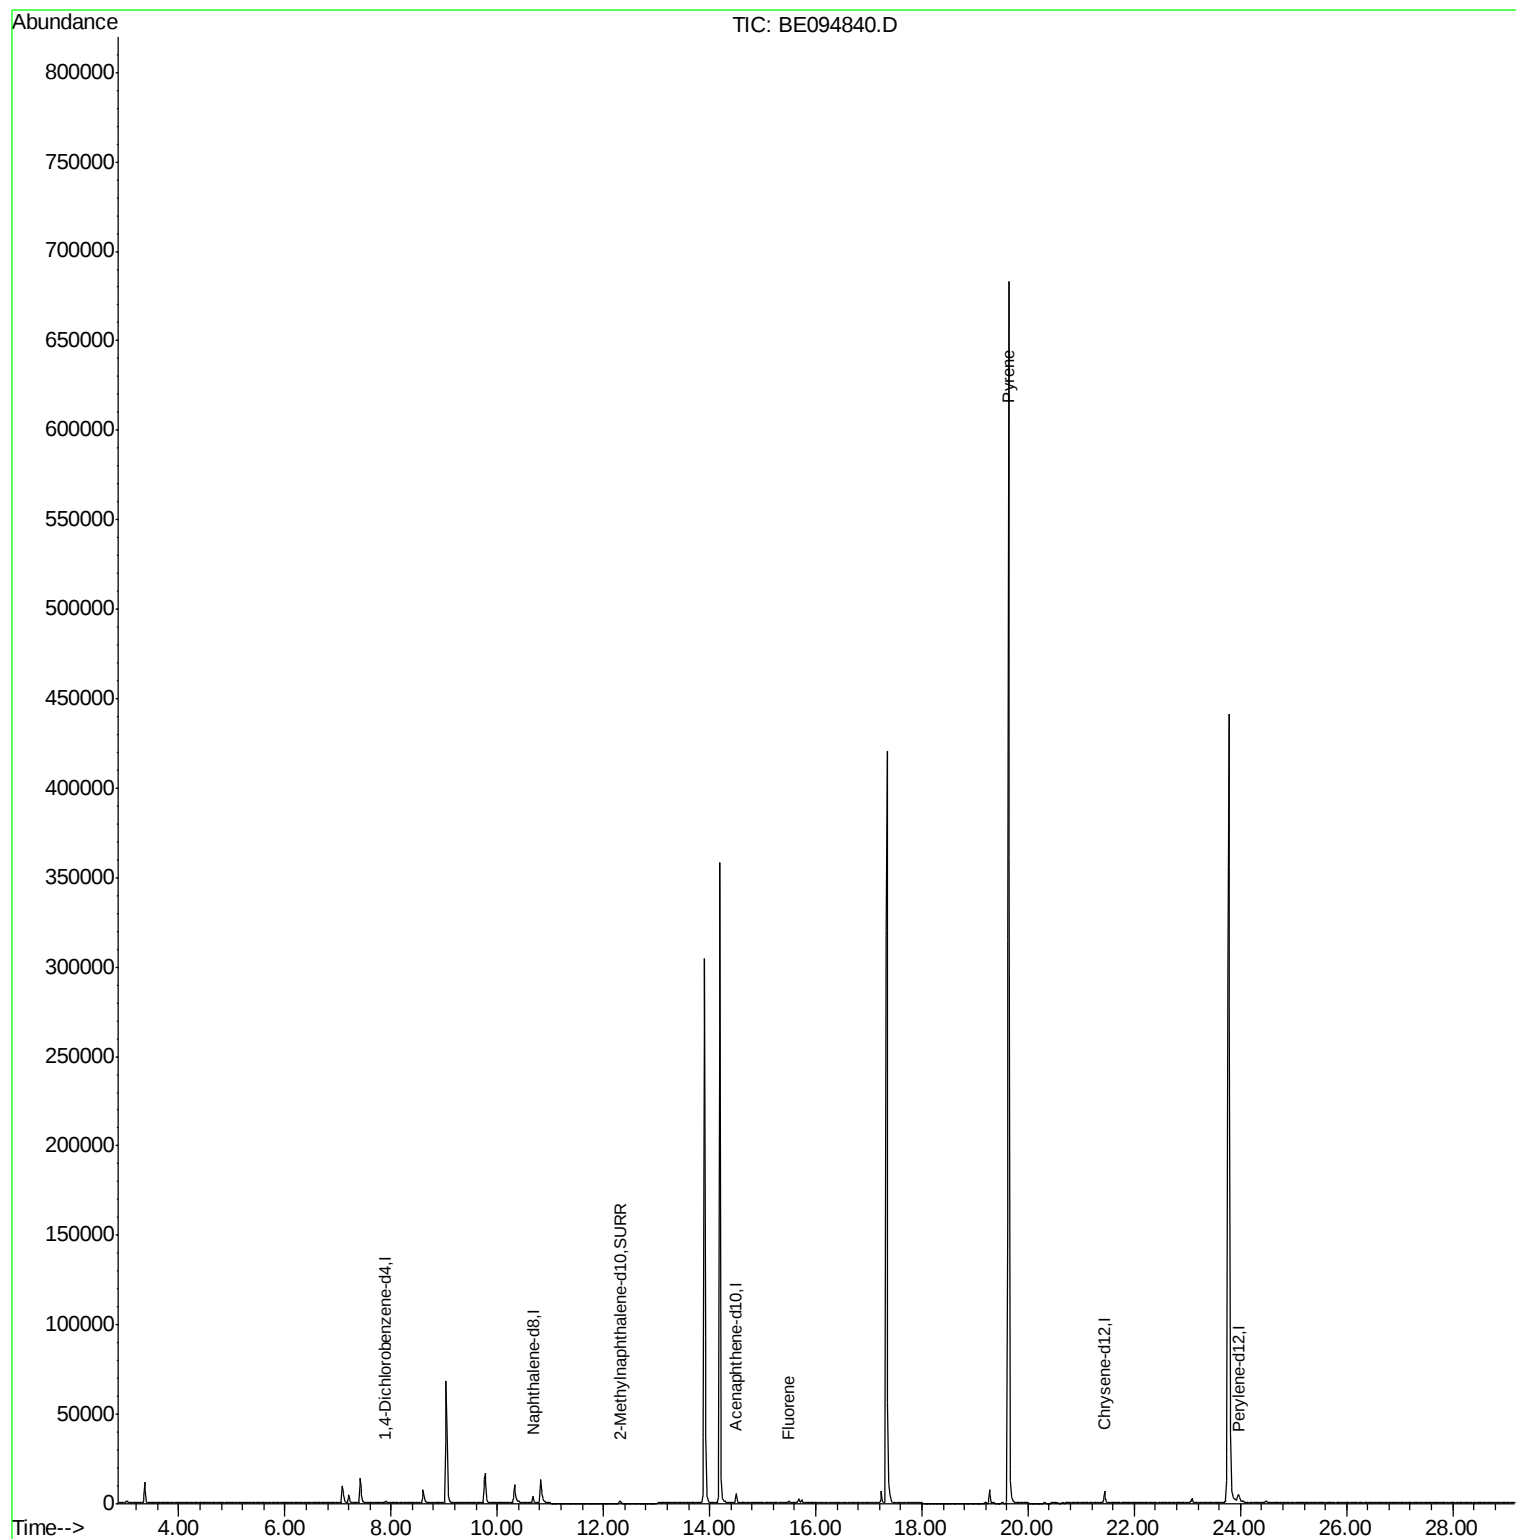

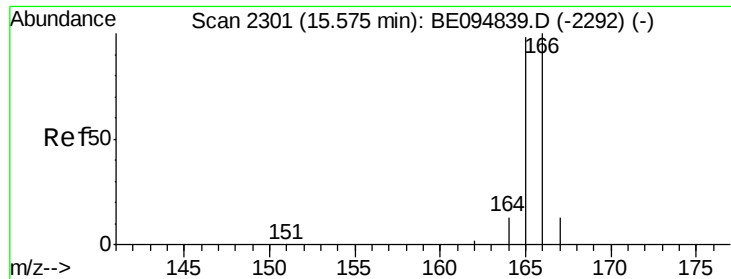

#9

Fluorene

Concen: 0.06 ng/ul

RT: 15.49 min Scan# 2290

Delta R.T. -0.08 min

Lab File: BE094840.D

Acq: 22 Nov 2017 20:06

Instrument :

BNA_E

ClientSampleId :





Tot Ion:166 Resp: 819

Ion Ratio Lower Upper

166 100

165 11.7 73.4 110.2#

167 41.1 14.6 22.0#

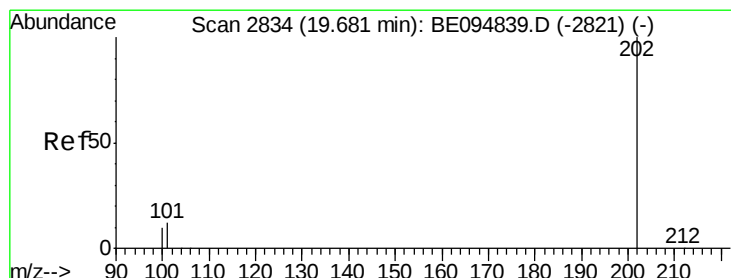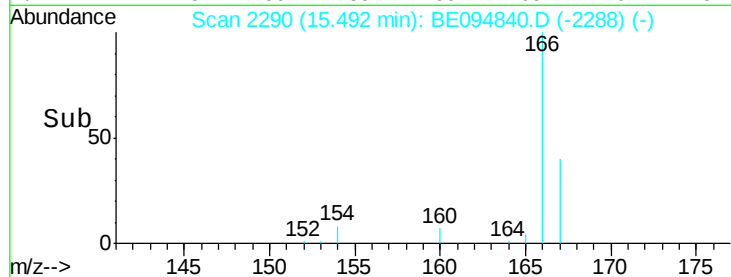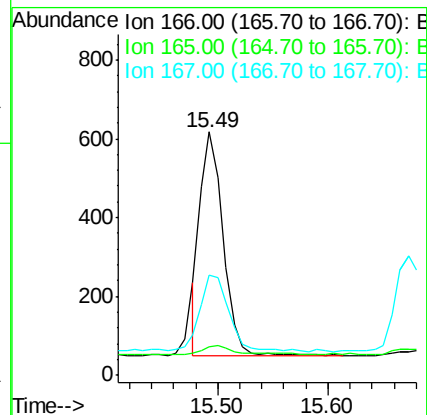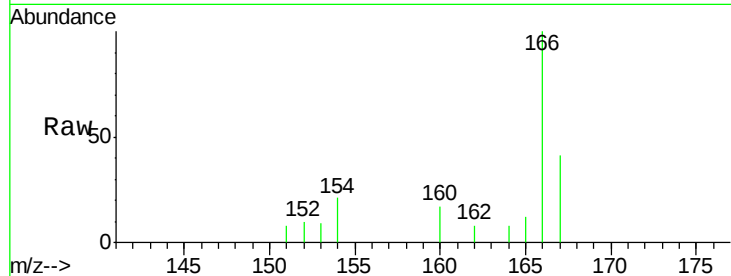

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.63 min Scan# 2824

Delta R.T. -0.05 min

Lab File: BE094840.D

Acq: 22 Nov 2017 20:06

Tgt Ion:202 Resp: 1134

Ion Ratio Lower Upper

202 100

101 146.4 18.2 27.4#

100 764.3 15.6 23.4#

